

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022316.D
 Acq On : 10 Oct 2024 10:05
 Operator : RC/JU
 Sample : PB163720BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK720

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022316.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	37	41	51	rVB	25130	36372	1.05%	0.112%
2	3.640	107	111	130	rBV	313447	475092	13.67%	1.464%
3	3.964	162	166	170	rVB2	4159	5707	0.16%	0.018%
4	6.852	653	657	658	rBV2	6015	7386	0.21%	0.023%
5	6.893	658	664	675	rVB	392793	637710	18.35%	1.965%
6	7.046	683	690	705	rVB	284829	457831	13.17%	1.411%
7	7.246	717	724	735	rBV	382582	635083	18.27%	1.957%
8	7.705	795	802	810	rBV	369963	581034	16.72%	1.791%
9	8.405	914	921	937	rBV	508830	824454	23.72%	2.541%
10	8.846	988	996	1006	rBV	399396	644013	18.53%	1.985%
11	9.252	1060	1065	1073	rBV2	10605	19015	0.55%	0.059%
12	9.557	1108	1117	1128	rBV	312790	579217	16.66%	1.785%
13	10.093	1200	1208	1220	rBV	589891	913787	26.29%	2.816%
14	10.463	1263	1271	1285	rVB	508334	839668	24.16%	2.588%
15	10.604	1285	1295	1306	rBV	470323	853642	24.56%	2.631%
16	11.734	1483	1487	1497	rVB2	8964	14858	0.43%	0.046%
17	12.057	1536	1542	1549	rVB2	7859	14517	0.42%	0.045%
18	13.722	1818	1825	1837	rBV	986470	1496017	43.04%	4.610%
19	13.998	1864	1872	1882	rBV	1216499	1740025	50.06%	5.362%
20	14.304	1917	1924	1938	rVB	996681	1404537	40.41%	4.329%
21	14.534	1957	1963	1983	rBV	505871	789822	22.72%	2.434%
22	14.734	1994	1997	2005	rVB10	2144	5402	0.16%	0.017%
23	15.322	2089	2097	2109	rBV	1667294	2315869	66.62%	7.137%
24	15.457	2113	2120	2134	rBV	447014	706630	20.33%	2.178%
25	15.569	2136	2139	2144	rVB4	8401	11402	0.33%	0.035%
26	16.592	2309	2313	2319	rBV8	3618	5728	0.16%	0.018%
27	16.781	2343	2345	2349	rVB5	3369	4024	0.12%	0.012%
28	16.892	2358	2364	2368	rBV6	5466	9688	0.28%	0.030%
29	17.110	2394	2401	2410	rVB	1333256	1968921	56.64%	6.068%
30	17.210	2411	2418	2431	rBV	1807107	2730184	78.54%	8.414%
31	17.386	2445	2448	2449	rBV3	3987	4405	0.13%	0.014%
32	17.704	2499	2502	2505	rVB5	3528	4044	0.12%	0.012%
33	19.133	2741	2745	2751	rBV4	29315	44293	1.27%	0.137%
34	19.204	2753	2757	2763	rVV	26981	41951	1.21%	0.129%
35	19.580	2816	2821	2828	rBV	2383869	3457134	99.45%	10.654%
36	21.539	3148	3154	3162	rBV2	1419030	2345338	67.47%	7.228%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022316.D
Acq On : 10 Oct 2024 10:05
Operator : RC/JU
Sample : PB163720BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK720

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	24.598	3666	3674	3686	rVB2	1339696	3476088	100.00%	10.713%
38	24.821	3705	3712	3724	rVB	867964	2347323	67.53%	7.234%




Sum of corrected areas: 32448211

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022316.D
Acq On : 10 Oct 2024 10:05
Operator : RC/JU
Sample : PB163720BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK720

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

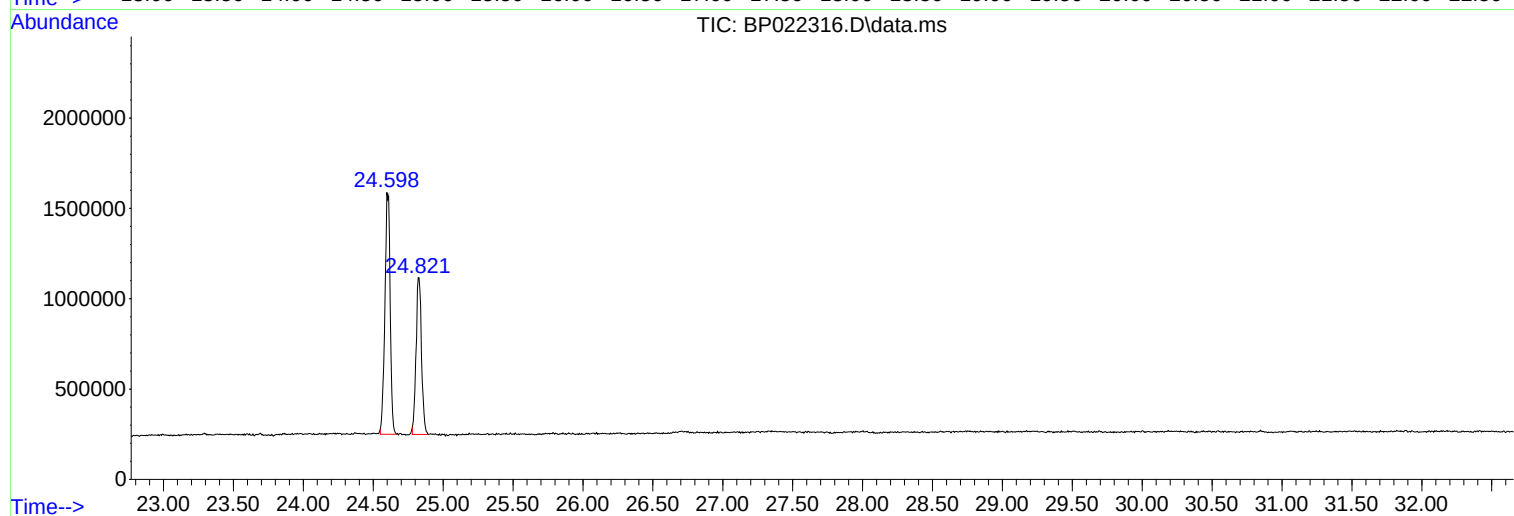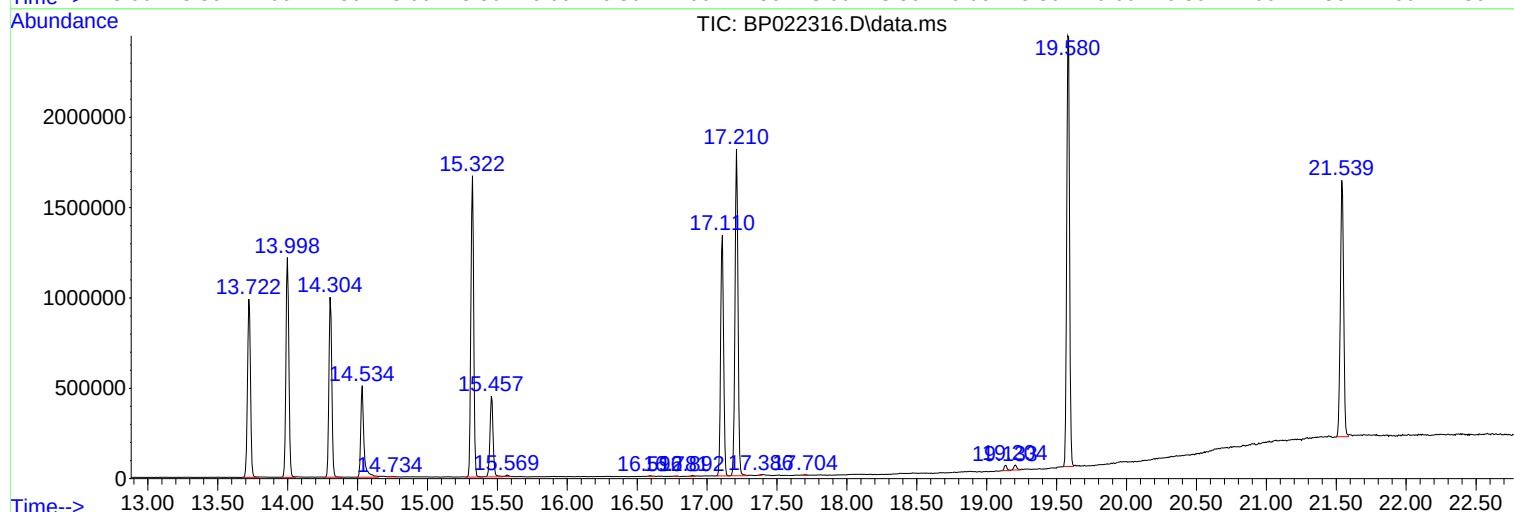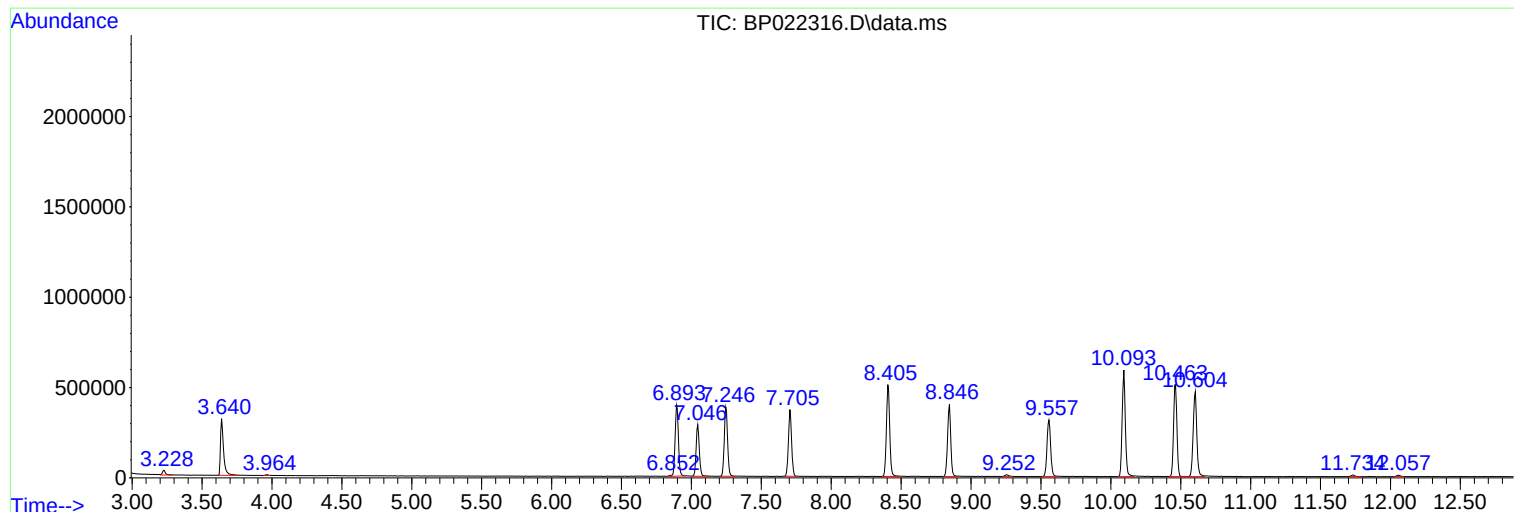

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022316.D
Acq On : 10 Oct 2024 10:05
Operator : RC/JU
Sample : PB163720BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK720

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022316.D
Acq On : 10 Oct 2024 10:05
Operator : RC/JU
Sample : PB163720BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK720

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc