

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022318.D
 Acq On : 10 Oct 2024 11:27
 Operator : RC/JU
 Sample : P4207-04
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY063

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022318.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	37	rVV4	4155	5063	0.10%	0.013%
2	3.228	37	41	43	rVV	18556	24106	0.50%	0.061%
3	3.258	43	46	52	rVB	26867	36412	0.75%	0.093%
4	3.646	108	112	119	rBV	112984	176247	3.63%	0.449%
5	3.964	162	166	170	rBV2	6560	9448	0.19%	0.024%
6	4.399	234	240	244	rBV4	3878	6551	0.13%	0.017%
7	4.481	249	254	261	rVB	26768	42565	0.88%	0.109%
8	4.746	295	299	304	rVB5	6158	8865	0.18%	0.023%
9	4.869	315	320	326	rVB3	8385	16282	0.34%	0.042%
10	5.993	505	511	519	rBV2	13969	22130	0.46%	0.056%
11	6.852	652	657	659	rBV2	7059	10641	0.22%	0.027%
12	6.893	659	664	675	rVB	156206	252791	5.20%	0.645%
13	7.046	683	690	702	rVB	374106	553244	11.38%	1.411%
14	7.252	717	725	737	rBV	427230	717798	14.77%	1.830%
15	7.705	793	802	810	rBV	423980	686165	14.12%	1.750%
16	7.781	810	815	818	rVB6	2688	5150	0.11%	0.013%
17	8.063	858	863	869	rVB10	4290	7003	0.14%	0.018%
18	8.410	913	922	935	rBV	405640	704720	14.50%	1.797%
19	8.846	988	996	1009	rBV	504674	792715	16.31%	2.022%
20	9.257	1059	1066	1074	rVB3	10506	19144	0.39%	0.049%
21	9.405	1086	1091	1098	rVB3	10755	18126	0.37%	0.046%
22	9.557	1110	1117	1125	rBV	425372	719074	14.80%	1.834%
23	10.099	1200	1209	1225	rBV	712015	1125216	23.15%	2.869%
24	10.457	1263	1270	1280	rVB	579655	981087	20.19%	2.502%
25	10.604	1286	1295	1308	rBV	466899	867986	17.86%	2.213%
26	11.275	1405	1409	1417	rBV	2883	6724	0.14%	0.017%
27	11.734	1481	1487	1494	rVB2	8932	14414	0.30%	0.037%
28	11.999	1524	1532	1537	rBV6	4826	9810	0.20%	0.025%
29	12.051	1537	1541	1548	rVB3	11409	19423	0.40%	0.050%
30	13.734	1817	1827	1835	rBV	1315783	1816376	37.37%	4.632%
31	14.010	1863	1874	1883	rBV	1460384	2020155	41.57%	5.152%
32	14.310	1918	1925	1935	rVB	1048940	1581947	32.55%	4.034%
33	14.534	1957	1963	1983	rBV	156702	290990	5.99%	0.742%
34	14.751	1994	2000	2010	rVB	6267	16325	0.34%	0.042%
35	15.128	2059	2064	2069	rBV5	4186	9216	0.19%	0.024%
36	15.322	2090	2097	2104	rBV	2100518	2799945	57.61%	7.140%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022318.D
 Acq On : 10 Oct 2024 11:27
 Operator : RC/JU
 Sample : P4207-04
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY063

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	15.457	2114	2120	2132	rBV	684303	1003070	20.64%	2.558%
38	15.569	2136	2139	2146	rVB3	11468	18475	0.38%	0.047%
39	15.692	2153	2160	2171	rBV	298115	436948	8.99%	1.114%
40	16.269	2252	2258	2263	rBV	39706	49754	1.02%	0.127%
41	16.516	2296	2300	2304	rBV7	4888	6421	0.13%	0.016%
42	16.587	2310	2312	2320	rVB8	4550	7615	0.16%	0.019%
43	17.116	2395	2402	2410	rBV	1553058	2216450	45.61%	5.652%
44	17.216	2412	2419	2429	rBV	2621400	3647610	75.05%	9.302%
45	17.386	2444	2448	2451	rBV5	4079	7675	0.16%	0.020%
46	17.510	2465	2469	2473	rBV7	4371	7896	0.16%	0.020%
47	17.922	2533	2539	2541	rBV7	6649	10484	0.22%	0.027%
48	18.039	2554	2559	2566	rBV3	82335	147664	3.04%	0.377%
49	18.351	2609	2612	2616	rBV3	11054	14220	0.29%	0.036%
50	18.675	2665	2667	2669	rBV3	6457	5822	0.12%	0.015%
51	18.928	2707	2710	2715	rVB6	17872	30804	0.63%	0.079%
52	19.139	2741	2746	2751	rBV2	32699	51363	1.06%	0.131%
53	19.216	2755	2759	2763	rBV	33110	51480	1.06%	0.131%
54	19.375	2782	2786	2793	rBV3	51074	75563	1.55%	0.193%
55	19.598	2817	2824	2831	rBV	3028529	4600737	94.66%	11.732%
56	21.216	3096	3099	3105	rVB4	67877	102233	2.10%	0.261%
57	21.545	3149	3155	3164	rVB	1846469	2666664	54.87%	6.800%
58	24.604	3666	3675	3692	rVB	1850928	4860103	100.00%	12.394%
59	24.839	3706	3715	3726	rVB	1069676	2801040	57.63%	7.143%




Sum of corrected areas: 39213945

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022318.D
Acq On : 10 Oct 2024 11:27
Operator : RC/JU
Sample : P4207-04
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY063

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

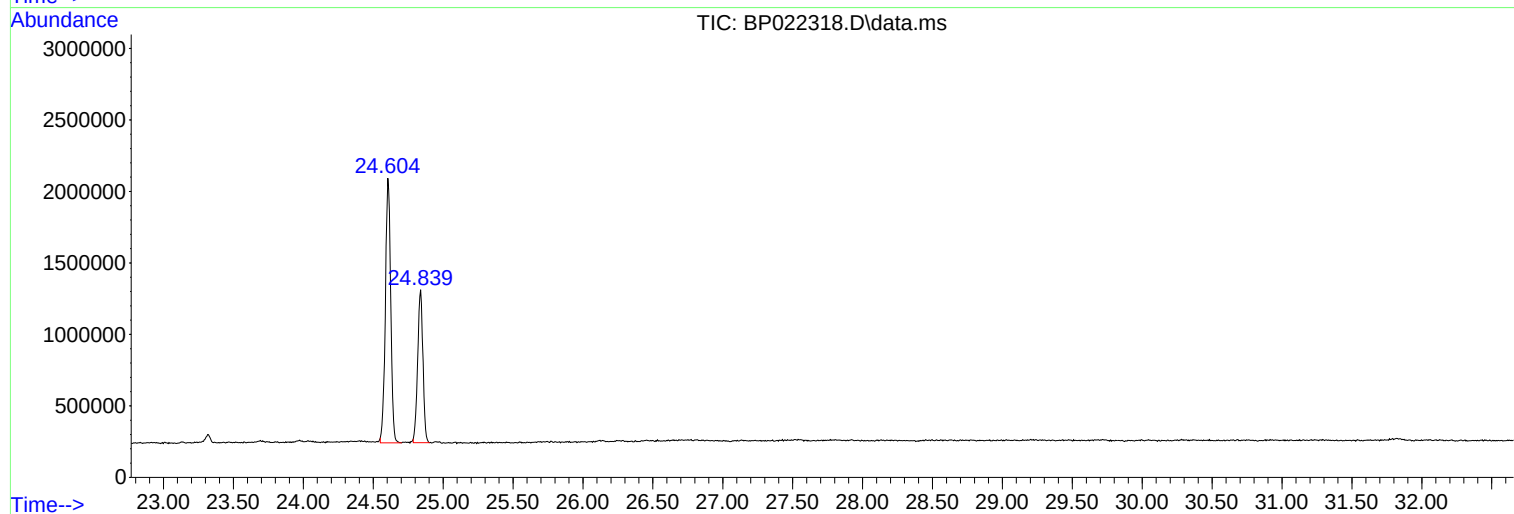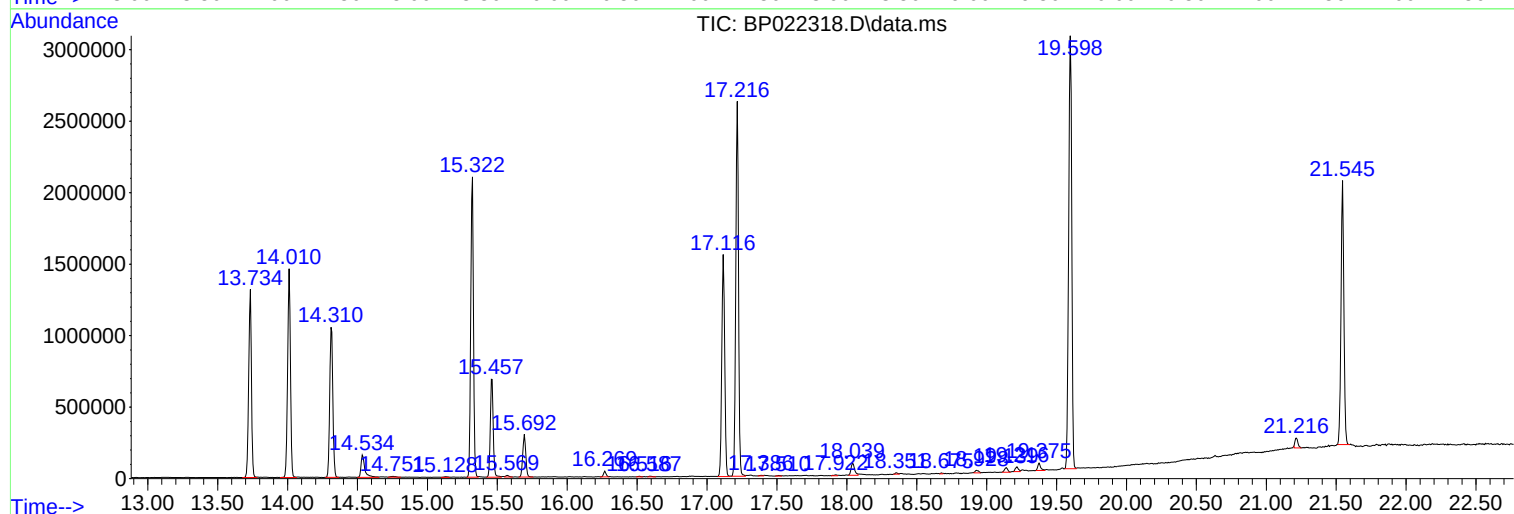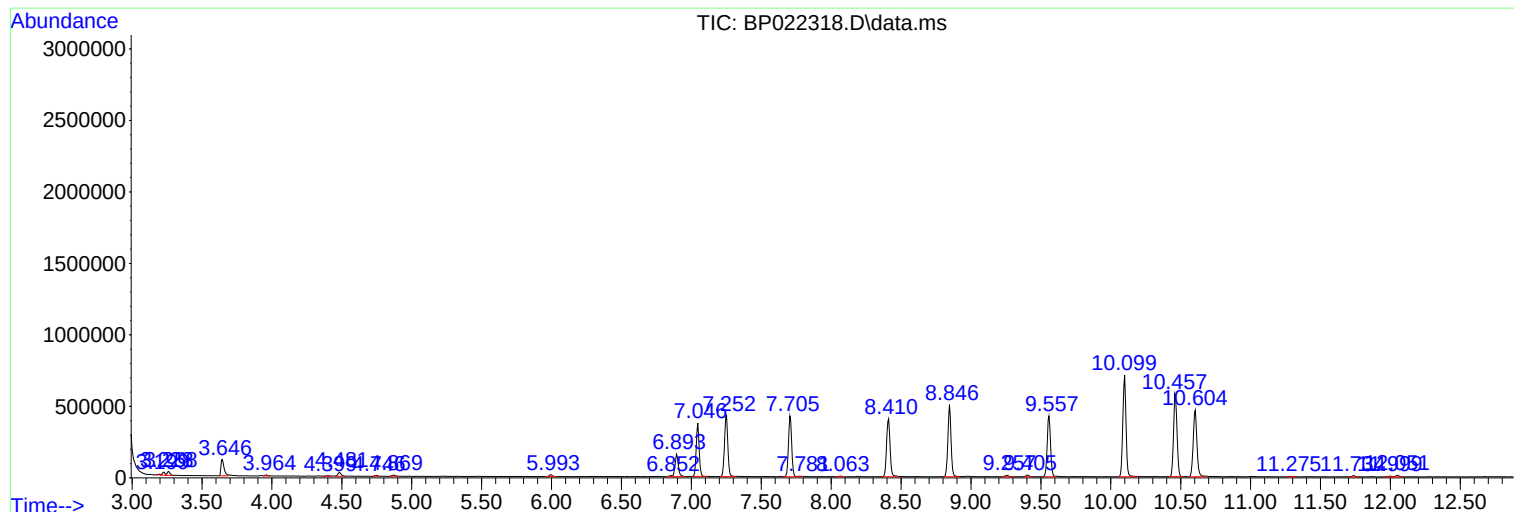

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022318.D
Acq On : 10 Oct 2024 11:27
Operator : RC/JU
Sample : P4207-04
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY063










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.692	5.52 ng/ul	436948	Acenaphthene-d10	14.310

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	94
4			Benzophenone	182	C13H10O	000119-61-9	91
5			Benzophenone	182	C13H10O	000119-61-9	91

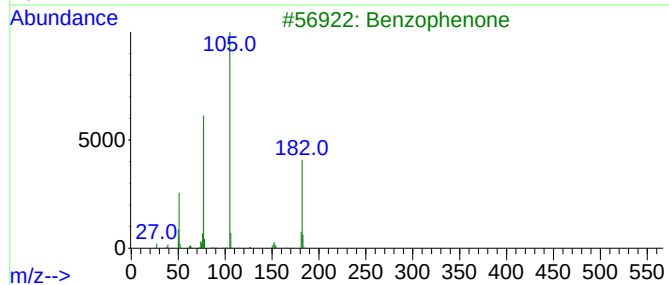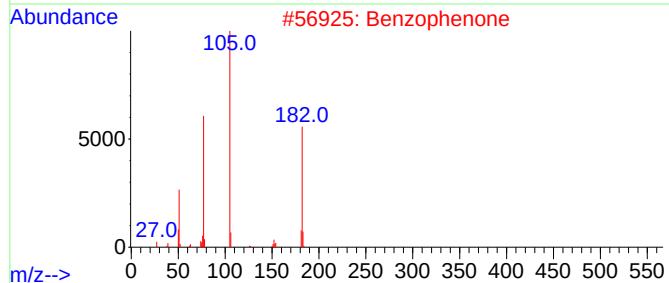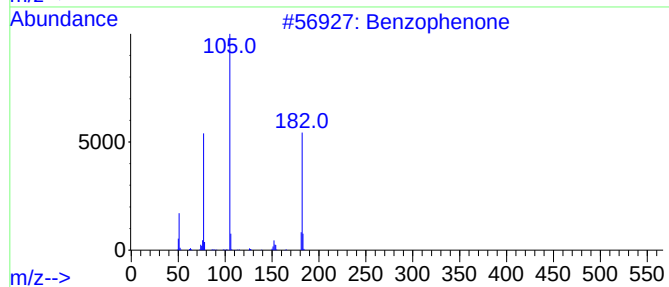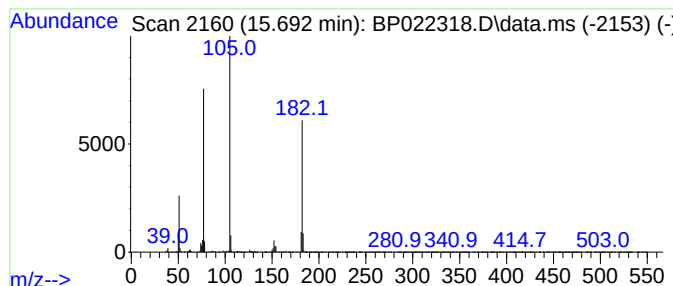

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022318.D
Acq On : 10 Oct 2024 11:27
Operator : RC/JU
Sample : P4207-04
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY063

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.692	5.5	ng/u1	436948	3	14.310	1581950	20.0