

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022320.D
 Acq On : 10 Oct 2024 12:48
 Operator : RC/JU
 Sample : P4207-06
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY068

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022320.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	37	41	47	rVB	19891	26357	0.63%	0.075%
2	3.646	108	112	131	rVB	86625	138426	3.29%	0.394%
3	3.957	162	165	171	rVB2	7701	10538	0.25%	0.030%
4	4.481	251	254	260	rVB4	8747	13523	0.32%	0.038%
5	4.746	294	299	306	rVB8	5583	9695	0.23%	0.028%
6	4.863	313	319	325	rBV3	6087	12060	0.29%	0.034%
7	5.993	506	511	518	rVB3	11316	18561	0.44%	0.053%
8	6.893	659	664	676	rVB	130709	221358	5.27%	0.630%
9	7.046	683	690	704	rBV	360094	559481	13.31%	1.591%
10	7.251	715	725	736	rBV	429027	706705	16.81%	2.010%
11	7.704	795	802	810	rBV	392349	638661	15.19%	1.817%
12	8.069	858	864	867	rBV7	4639	7755	0.18%	0.022%
13	8.193	880	885	892	rVB10	3749	7211	0.17%	0.021%
14	8.410	914	922	931	rBV	378412	637449	15.16%	1.813%
15	8.845	987	996	1005	rBV	467330	799628	19.02%	2.274%
16	9.263	1061	1067	1075	rVB7	4815	9067	0.22%	0.026%
17	9.410	1086	1092	1096	rVB8	3104	5572	0.13%	0.016%
18	9.557	1108	1117	1133	rBV	437499	728291	17.32%	2.071%
19	9.739	1142	1148	1154	rBV7	4188	9938	0.24%	0.028%
20	10.098	1200	1209	1219	rBV	634890	1107292	26.34%	3.149%
21	10.469	1261	1272	1282	rBV	497807	918744	21.85%	2.613%
22	10.598	1285	1294	1308	rBV	480376	820076	19.51%	2.332%
23	11.728	1480	1486	1490	rBV9	2949	5086	0.12%	0.014%
24	12.045	1534	1540	1548	rVB	9401	16379	0.39%	0.047%
25	13.492	1781	1786	1789	rBV6	2562	4552	0.11%	0.013%
26	13.722	1816	1825	1833	rBV	1260185	1765014	41.98%	5.020%
27	14.004	1866	1873	1886	rBV	1294263	1993647	47.42%	5.670%
28	14.316	1918	1926	1937	rVB	957812	1451350	34.52%	4.128%
29	14.539	1959	1964	1982	rBV	120938	245040	5.83%	0.697%
30	14.751	1996	2000	2005	rVB8	5220	9792	0.23%	0.028%
31	15.139	2061	2066	2071	rBV7	3264	5984	0.14%	0.017%
32	15.316	2089	2096	2106	rBV	1797392	2694940	64.10%	7.665%
33	15.457	2113	2120	2134	rBV	657668	933771	22.21%	2.656%
34	15.563	2134	2138	2147	rVB2	11568	21790	0.52%	0.062%
35	15.692	2154	2160	2166	rBV2	21681	34353	0.82%	0.098%
36	16.127	2229	2234	2238	rBV8	2903	5392	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022320.D
 Acq On : 10 Oct 2024 12:48
 Operator : RC/JU
 Sample : P4207-06
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY068

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	16.510	2293	2299	2302	rBV8	3082	5412	0.13%	0.015%
38	16.774	2338	2344	2350	rBV8	5119	11642	0.28%	0.033%
39	16.898	2361	2365	2367	rBV5	3503	4266	0.10%	0.012%
40	17.104	2392	2400	2408	rBV	1205057	1996761	47.50%	5.679%
41	17.221	2412	2420	2431	rBV	2116755	3248298	77.26%	9.239%
42	17.410	2449	2452	2458	rVB4	5675	8898	0.21%	0.025%
43	18.039	2554	2559	2567	rBV2	32055	54841	1.30%	0.156%
44	18.380	2614	2617	2625	rVB7	7976	15698	0.37%	0.045%
45	18.539	2640	2644	2648	rBV6	5000	9905	0.24%	0.028%
46	19.127	2740	2744	2749	rBV3	35998	53015	1.26%	0.151%
47	19.210	2754	2758	2762	rVV	25761	38069	0.91%	0.108%
48	19.374	2783	2786	2790	rBV5	12595	18778	0.45%	0.053%
49	19.533	2811	2813	2816	rBV3	12225	9339	0.22%	0.027%
50	19.586	2816	2822	2830	rBV	2670255	4072523	96.87%	11.583%
51	21.539	3148	3154	3162	rBV	1514565	2350966	55.92%	6.687%
52	24.609	3665	3676	3685	rVB	1564821	4204106	100.00%	11.958%
53	24.827	3704	3713	3725	rVB	839672	2462707	58.58%	7.005%




Sum of corrected areas: 35158702

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022320.D
Acq On : 10 Oct 2024 12:48
Operator : RC/JU
Sample : P4207-06
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY068

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

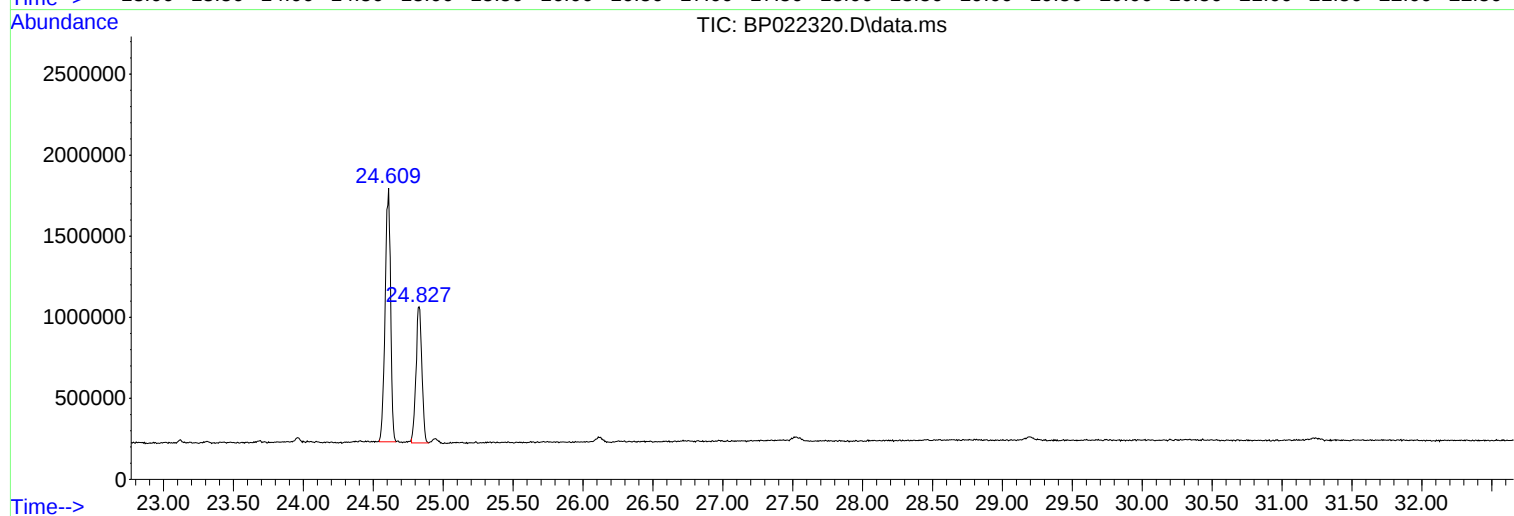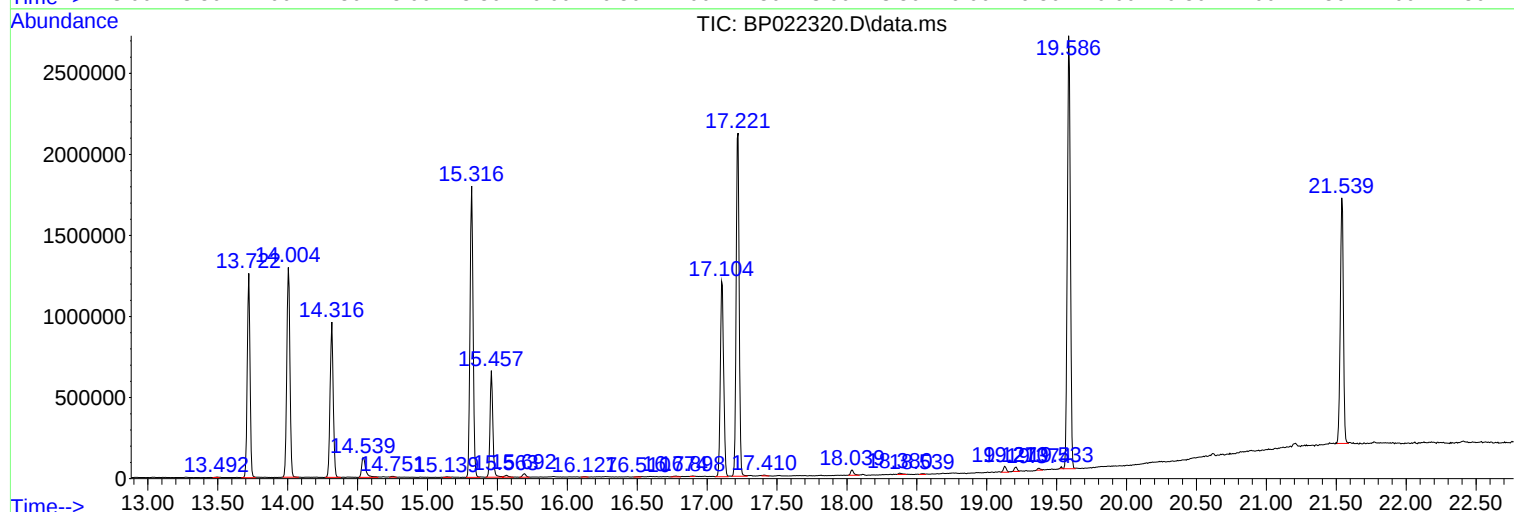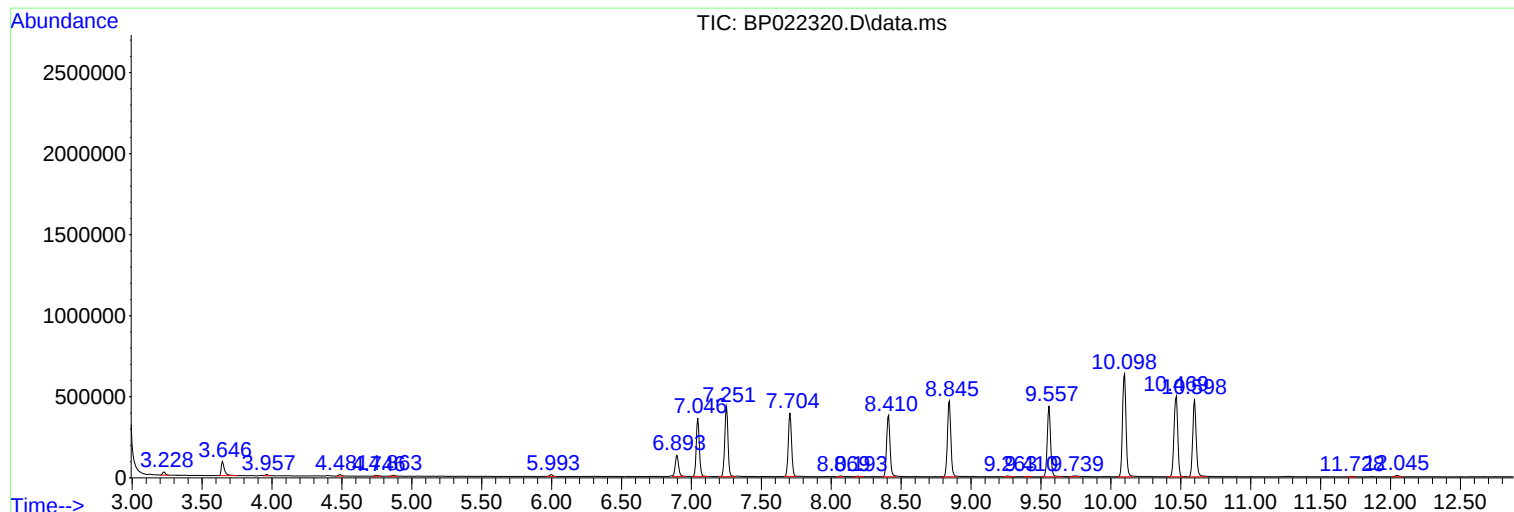

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022320.D
Acq On : 10 Oct 2024 12:48
Operator : RC/JU
Sample : P4207-06
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY068

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022320.D
Acq On : 10 Oct 2024 12:48
Operator : RC/JU
Sample : P4207-06
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY068

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc