

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022321.D
 Acq On : 10 Oct 2024 13:29
 Operator : RC/JU
 Sample : P4187-19
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY056

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	37	41	49	rVB	23780	29313	0.57%	0.073%
2	3.646	108	112	123	rBV	110245	171936	3.36%	0.427%
3	3.957	161	165	171	rVB2	9348	14158	0.28%	0.035%
4	4.399	235	240	245	rBV5	4274	8280	0.16%	0.021%
5	4.481	251	254	259	rVB6	4085	5222	0.10%	0.013%
6	4.752	296	300	306	rVB4	6366	10150	0.20%	0.025%
7	4.869	315	320	327	rVB3	6669	12689	0.25%	0.032%
8	5.993	505	511	518	rVB3	13451	21016	0.41%	0.052%
9	6.893	653	664	677	rBV	148647	253479	4.96%	0.630%
10	7.046	682	690	705	rVB	334461	558471	10.93%	1.388%
11	7.251	718	725	735	rBV	433950	702228	13.74%	1.745%
12	7.704	794	802	810	rBV	465363	733979	14.36%	1.824%
13	8.069	858	864	869	rBV9	4222	7258	0.14%	0.018%
14	8.187	880	884	889	rBV8	3151	5371	0.11%	0.013%
15	8.404	913	921	930	rBV2	421088	694297	13.58%	1.725%
16	8.840	988	995	1008	rBV	459893	788075	15.42%	1.959%
17	9.257	1061	1066	1073	rVB8	3826	6284	0.12%	0.016%
18	9.557	1108	1117	1128	rBV	395778	713905	13.97%	1.774%
19	10.092	1200	1208	1224	rBV	655755	1121042	21.93%	2.786%
20	10.457	1263	1270	1283	rVB	605805	1036422	20.28%	2.576%
21	10.598	1286	1294	1310	rBV	524153	925692	18.11%	2.301%
22	11.263	1400	1407	1416	rBV	4615	12158	0.24%	0.030%
23	12.045	1534	1540	1548	rBV	9720	19259	0.38%	0.048%
24	13.722	1818	1825	1834	rBV	1541571	1853018	36.25%	4.605%
25	14.004	1861	1873	1884	rBV2	1266085	2074759	40.59%	5.156%
26	14.310	1916	1925	1935	rBV	1085722	1704860	33.35%	4.237%
27	14.527	1957	1962	1981	rBV	149803	301171	5.89%	0.748%
28	14.757	1999	2001	2008	rVB8	7676	10160	0.20%	0.025%
29	15.316	2089	2096	2109	rBV	1999386	2906437	56.86%	7.223%
30	15.457	2114	2120	2130	rVV	877428	1111402	21.74%	2.762%
31	15.563	2134	2138	2144	rVB	10785	17917	0.35%	0.045%
32	16.780	2343	2345	2349	rVB5	4232	5333	0.10%	0.013%
33	16.892	2359	2364	2368	rBV4	3750	5681	0.11%	0.014%
34	17.110	2394	2401	2411	rBV	1546438	2360696	46.18%	5.867%
35	17.216	2412	2419	2431	rVV	2565908	3878715	75.88%	9.639%
36	17.816	2517	2521	2525	rBV7	5352	7837	0.15%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022321.D
Acq On : 10 Oct 2024 13:29
Operator : RC/JU
Sample : P4187-19
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY056

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	18.039	2554	2559	2569	rBV4	35360	67616	1.32%	0.168%
38	18.386	2614	2618	2621	rBV3	8758	11688	0.23%	0.029%
39	19.133	2740	2745	2750	rBV2	39368	55956	1.09%	0.139%
40	19.204	2753	2757	2762	rBV	34128	52285	1.02%	0.130%
41	19.374	2782	2786	2790	rBV4	32234	50383	0.99%	0.125%
42	19.533	2810	2813	2815	rBV3	16522	17708	0.35%	0.044%
43	19.586	2816	2822	2830	rVV	3611873	4943679	96.71%	12.286%
44	19.857	2865	2868	2872	rVB2	22618	26111	0.51%	0.065%
45	21.551	3149	3156	3163	rVB2	1753207	2898628	56.71%	7.204%
46	24.609	3666	3676	3688	rVB	1998641	5111754	100.00%	12.704%
47	24.839	3706	3715	3727	rVB	1027642	2913816	57.00%	7.241%




Sum of corrected areas: 40238294

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022321.D
Acq On : 10 Oct 2024 13:29
Operator : RC/JU
Sample : P4187-19
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY056

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

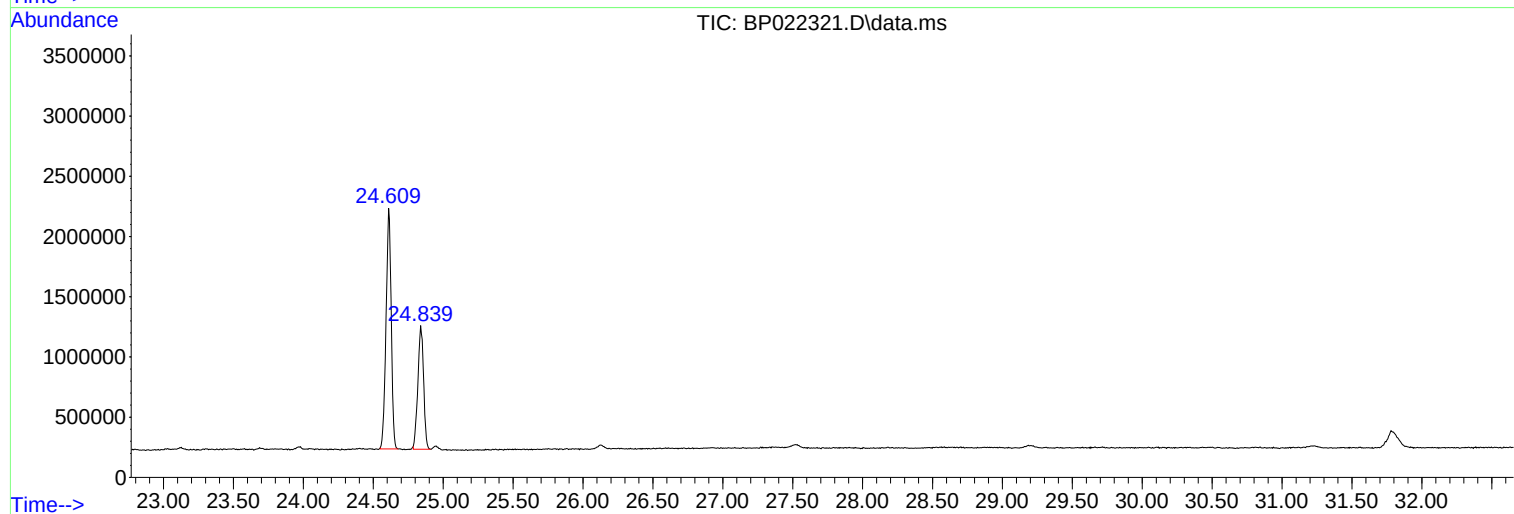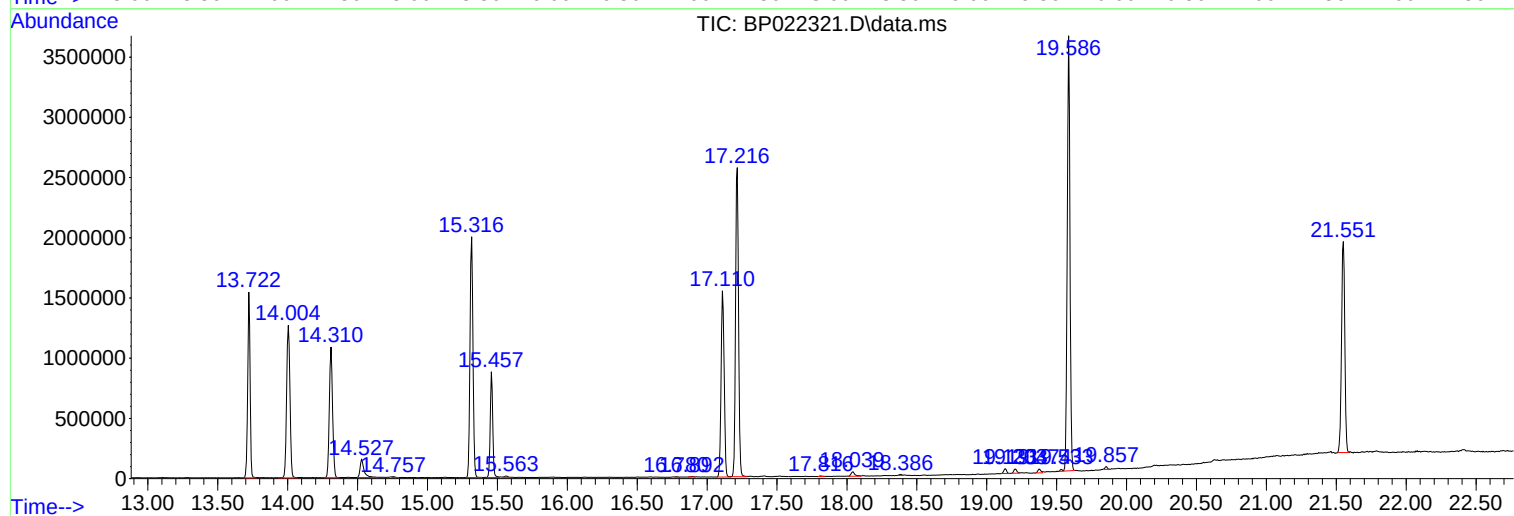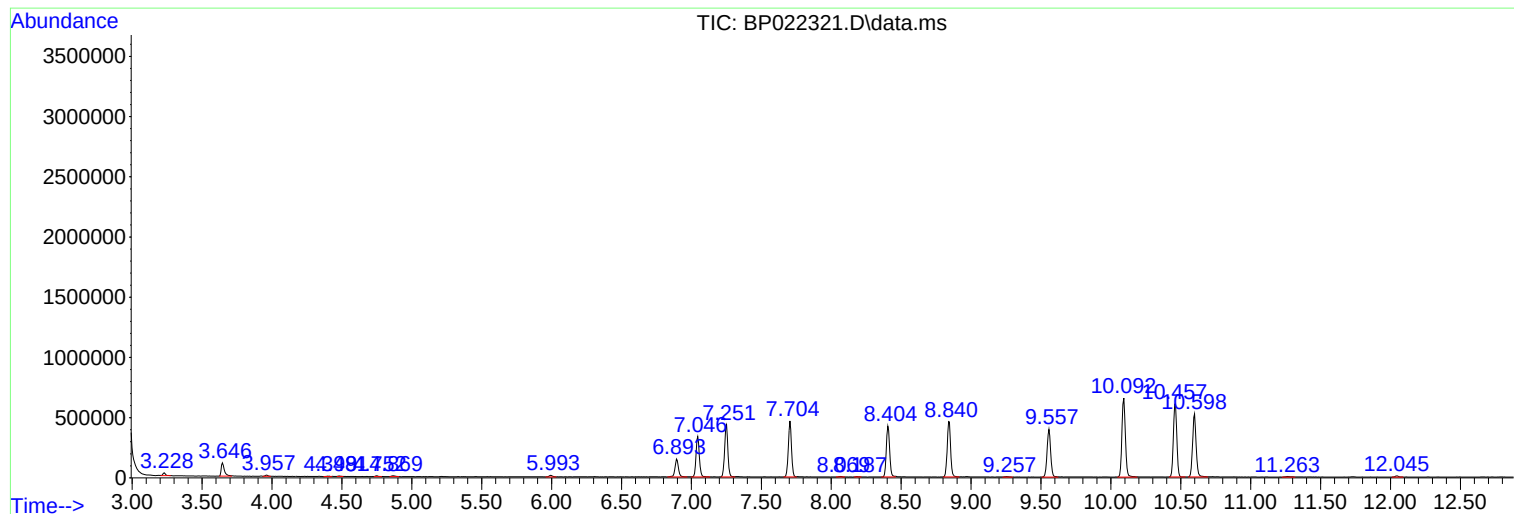

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022321.D
Acq On : 10 Oct 2024 13:29
Operator : RC/JU
Sample : P4187-19
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY056

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022321.D
Acq On : 10 Oct 2024 13:29
Operator : RC/JU
Sample : P4187-19
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY056

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc