

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022322.D
 Acq On : 10 Oct 2024 14:10
 Operator : RC/JU
 Sample : P4187-20
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY059

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022322.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	37	40	44	rBV	25438	32609	0.69%	0.086%
2	3.258	44	46	52	rVB	14931	17948	0.38%	0.047%
3	3.640	107	111	124	rBV	95429	156669	3.33%	0.414%
4	3.958	162	165	170	rVB	9797	13670	0.29%	0.036%
5	4.399	237	240	246	rVB3	3829	6296	0.13%	0.017%
6	4.740	295	298	304	rVB6	5590	8509	0.18%	0.022%
7	4.869	315	320	326	rVB4	10350	17505	0.37%	0.046%
8	5.669	452	456	459	rVB3	3716	4741	0.10%	0.013%
9	5.993	505	511	517	rVB2	14424	23079	0.49%	0.061%
10	6.293	553	562	567	rBV2	2881	6436	0.14%	0.017%
11	6.858	651	658	659	rBV4	8907	14932	0.32%	0.039%
12	6.893	659	664	677	rVB	150451	253919	5.39%	0.671%
13	7.046	683	690	699	rVB	358291	559546	11.88%	1.479%
14	7.246	715	724	734	rBV	451028	718776	15.26%	1.900%
15	7.328	735	738	743	rVB7	3685	5275	0.11%	0.014%
16	7.705	794	802	810	rBV	435572	701392	14.89%	1.854%
17	7.958	834	845	850	rBV	3860	9511	0.20%	0.025%
18	8.063	858	863	868	rBV4	5138	8415	0.18%	0.022%
19	8.187	880	884	890	rVB9	4308	6200	0.13%	0.016%
20	8.405	912	921	936	rBV	406997	688093	14.61%	1.819%
21	8.840	988	995	1009	rBV	466850	775306	16.46%	2.049%
22	9.252	1060	1065	1071	rVB3	10509	16848	0.36%	0.045%
23	9.399	1086	1090	1097	rBV9	3711	6892	0.15%	0.018%
24	9.552	1109	1116	1125	rBV	436749	715182	15.19%	1.890%
25	9.734	1140	1147	1157	rBV	40375	85801	1.82%	0.227%
26	10.093	1199	1208	1224	rBV	653171	1121252	23.81%	2.963%
27	10.457	1262	1270	1279	rBV	591464	959997	20.39%	2.537%
28	10.599	1285	1294	1310	rBV	419947	767474	16.30%	2.028%
29	10.887	1339	1343	1350	rVB10	3094	5905	0.13%	0.016%
30	11.275	1403	1409	1421	rBV10	7583	20515	0.44%	0.054%
31	11.728	1480	1486	1492	rBV4	7019	12804	0.27%	0.034%
32	11.828	1496	1503	1506	rBV6	4050	8538	0.18%	0.023%
33	12.046	1535	1540	1548	rBV2	10208	16569	0.35%	0.044%
34	13.034	1704	1708	1714	rBV8	4440	6478	0.14%	0.017%
35	13.722	1816	1825	1833	rBV	1461246	1762411	37.43%	4.658%
36	14.004	1863	1873	1881	rBV	1298191	1957485	41.57%	5.173%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022322.D
 Acq On : 10 Oct 2024 14:10
 Operator : RC/JU
 Sample : P4187-20
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY059

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	14.187	1899	1904	1909	rBV	8017	12731	0.27%	0.034%
38	14.316	1917	1926	1934	rBV	1082521	1550778	32.93%	4.099%
39	14.428	1941	1945	1950	rVB7	3489	6506	0.14%	0.017%
40	14.534	1957	1963	1977	rBV2	116983	272324	5.78%	0.720%
41	14.751	1994	2000	2007	rVB7	8328	17406	0.37%	0.046%
42	15.122	2058	2063	2066	rBV3	3590	5062	0.11%	0.013%
43	15.322	2089	2097	2104	rBV	1894204	2735304	58.09%	7.229%
44	15.369	2104	2105	2113	rVV6	13612	23166	0.49%	0.061%
45	15.451	2113	2119	2130	rVV	827330	997538	21.18%	2.636%
46	15.563	2134	2138	2146	rVB5	9929	17056	0.36%	0.045%
47	15.704	2154	2162	2167	rBV	43582	65164	1.38%	0.172%
48	15.892	2190	2194	2201	rVB10	3399	6114	0.13%	0.016%
49	16.769	2338	2343	2345	rBV6	6366	9920	0.21%	0.026%
50	16.892	2359	2364	2368	rVB3	4010	6723	0.14%	0.018%
51	17.116	2394	2402	2409	rBV	1621128	2175160	46.19%	5.749%
52	17.210	2411	2418	2431	rVB	2550816	3501421	74.36%	9.254%
53	17.416	2447	2453	2460	rBV	14433	22874	0.49%	0.060%
54	17.810	2516	2520	2525	rBV7	6158	9956	0.21%	0.026%
55	18.051	2555	2561	2569	rBV3	37646	72338	1.54%	0.191%
56	18.122	2570	2573	2577	rVB	7799	10762	0.23%	0.028%
57	18.557	2644	2647	2652	rBV7	7165	11889	0.25%	0.031%
58	18.763	2678	2682	2687	rVB3	24496	31004	0.66%	0.082%
59	19.133	2741	2745	2751	rVB2	30571	48354	1.03%	0.128%
60	19.216	2755	2759	2764	rBV	33864	56513	1.20%	0.149%
61	19.598	2817	2824	2831	rBV	3196571	4563637	96.91%	12.061%
62	21.545	3150	3155	3162	rVB2	1716635	2646703	56.20%	6.995%
63	24.615	3667	3677	3688	rVB	1668948	4709033	100.00%	12.445%
64	24.839	3706	3715	3725	rVB	1022322	2759053	58.59%	7.292%




Sum of corrected areas: 37837467

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022322.D
Acq On : 10 Oct 2024 14:10
Operator : RC/JU
Sample : P4187-20
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY059

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

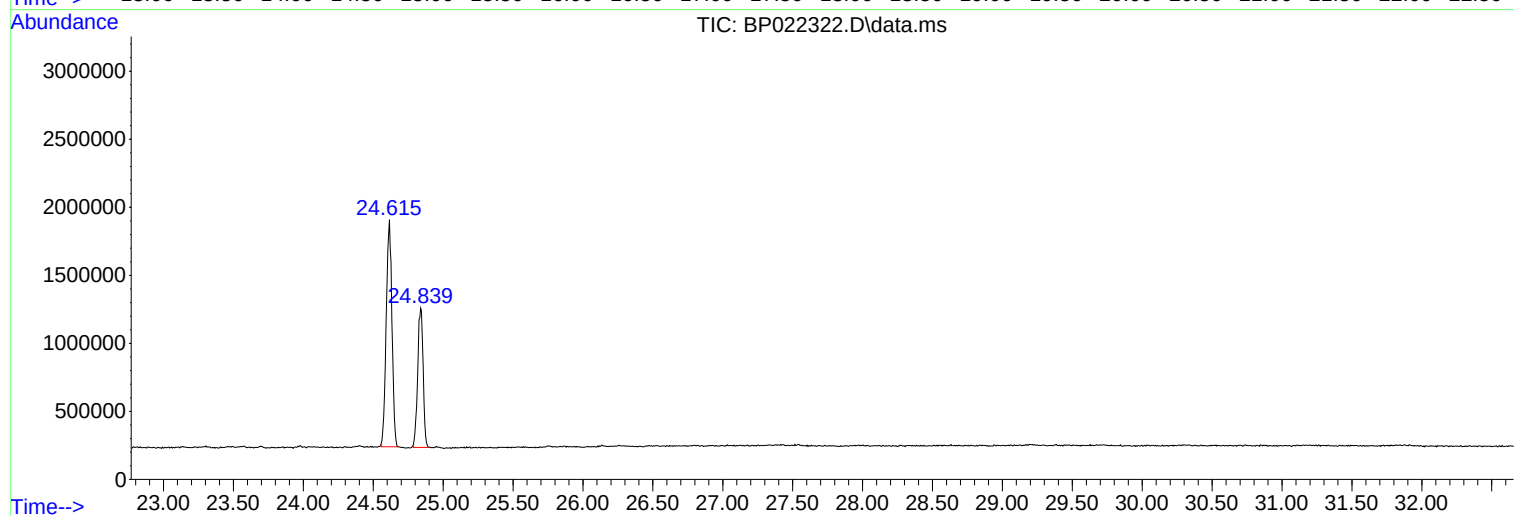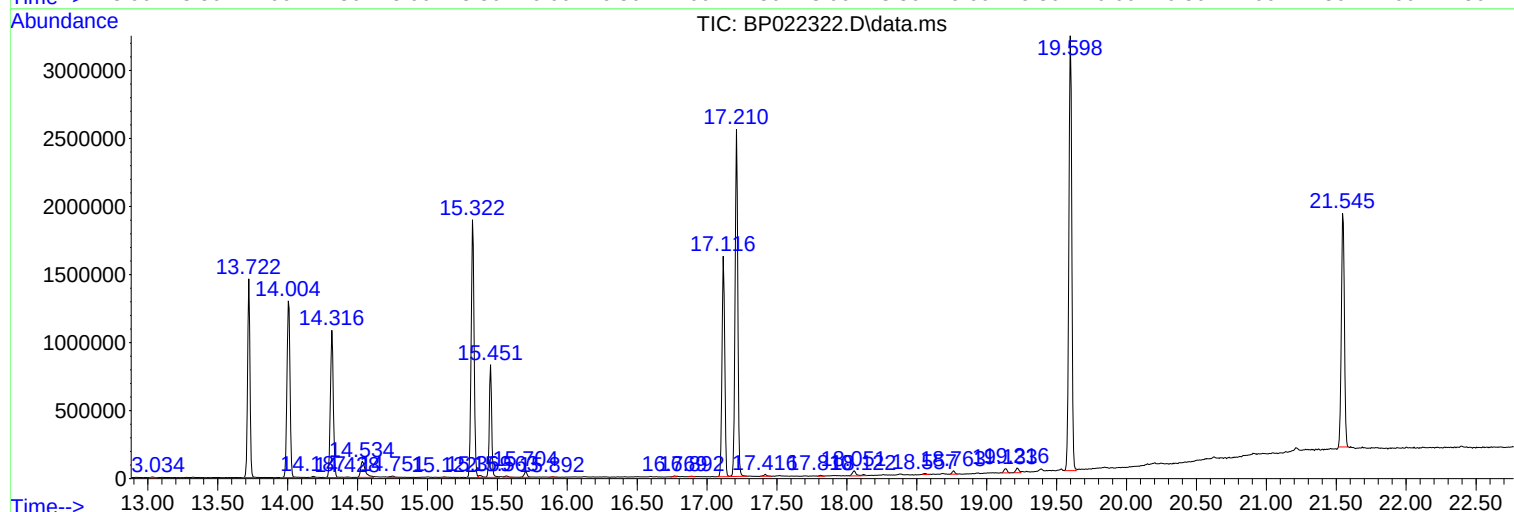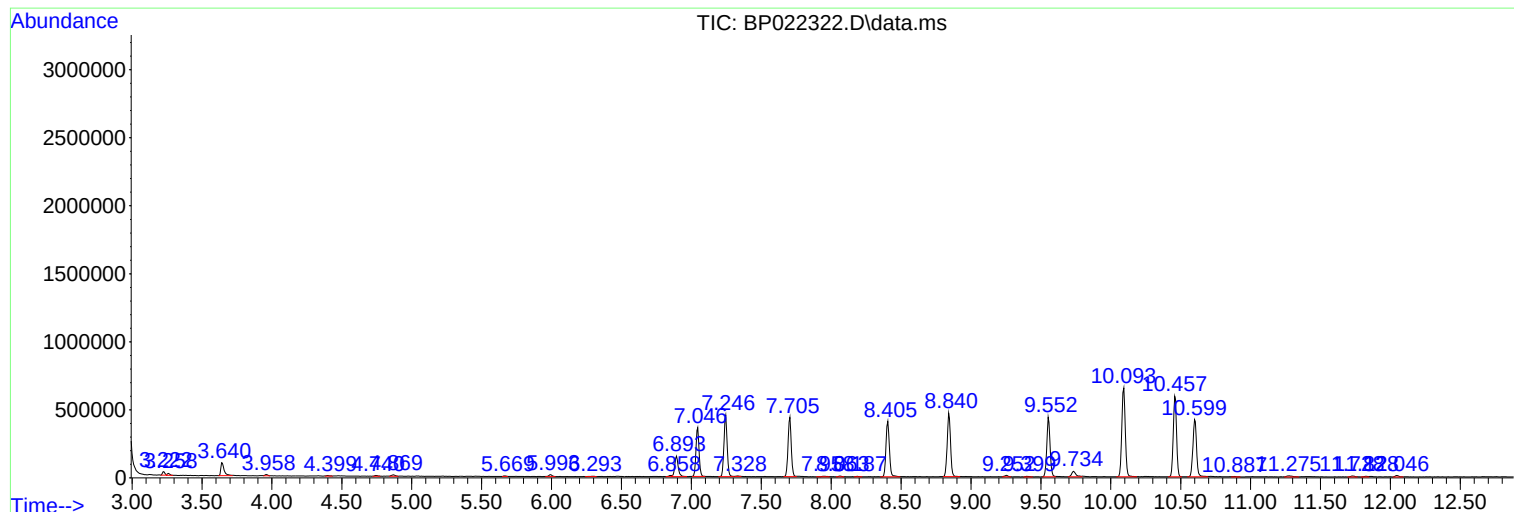

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022322.D
Acq On : 10 Oct 2024 14:10
Operator : RC/JU
Sample : P4187-20
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY059

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022322.D
Acq On : 10 Oct 2024 14:10
Operator : RC/JU
Sample : P4187-20
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY059

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc