

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022323.D
 Acq On : 10 Oct 2024 14:51
 Operator : RC/JU
 Sample : P4187-21
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY076

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022323.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	21	23	29	rVB6	4735	6990	0.17%	0.021%
2	3.193	31	35	38	rBV2	16240	22363	0.56%	0.068%
3	3.222	38	40	44	rVB	20468	21858	0.55%	0.067%
4	3.640	107	111	124	rBV	116501	179947	4.49%	0.549%
5	3.957	162	165	171	rVB	8179	10017	0.25%	0.031%
6	4.057	178	182	188	rVB3	11445	15275	0.38%	0.047%
7	4.481	248	254	265	rVB	183367	268136	6.69%	0.817%
8	4.752	294	300	304	rBV6	6217	10768	0.27%	0.033%
9	4.863	315	319	323	rBV	5260	6109	0.15%	0.019%
10	5.840	480	485	490	rBV9	2195	4058	0.10%	0.012%
11	5.987	505	510	516	rBV4	11998	20052	0.50%	0.061%
12	6.081	522	526	530	rBV5	6242	9081	0.23%	0.028%
13	6.851	653	657	658	rBV2	5126	6531	0.16%	0.020%
14	6.893	658	664	674	rVB	127919	213718	5.33%	0.651%
15	7.046	683	690	702	rVB	310430	505138	12.60%	1.540%
16	7.245	716	724	732	rBV	410029	644995	16.08%	1.966%
17	7.310	732	735	744	rVV5	7812	16698	0.42%	0.051%
18	7.428	748	755	762	rVB7	4826	9858	0.25%	0.030%
19	7.604	780	785	794	rVB	21367	34225	0.85%	0.104%
20	7.698	794	801	811	rBV	418801	657079	16.39%	2.003%
21	7.816	816	821	825	rVB6	4258	6864	0.17%	0.021%
22	8.045	853	860	868	rBV	26714	51515	1.28%	0.157%
23	8.175	877	882	887	rBV8	2795	4400	0.11%	0.013%
24	8.245	890	894	897	rVB4	2791	4247	0.11%	0.013%
25	8.404	912	921	939	rBV	392746	620022	15.46%	1.890%
26	8.598	949	954	961	rVB10	2979	5180	0.13%	0.016%
27	8.787	982	986	988	rBV5	3120	4338	0.11%	0.013%
28	8.840	988	995	1014	rVB	407764	742037	18.50%	2.262%
29	9.257	1061	1066	1072	rVB2	8420	15576	0.39%	0.047%
30	9.404	1086	1091	1097	rVB8	4670	8137	0.20%	0.025%
31	9.557	1110	1117	1125	rBV	378404	624606	15.58%	1.904%
32	9.881	1169	1172	1176	rBV5	4013	5588	0.14%	0.017%
33	9.951	1179	1184	1192	rBV10	2705	4608	0.11%	0.014%
34	10.092	1200	1208	1221	rBV	557636	983846	24.54%	2.999%
35	10.463	1261	1271	1279	rBV	500467	878908	21.92%	2.679%
36	10.592	1285	1293	1309	rBV	425030	733506	18.29%	2.236%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022323.D
 Acq On : 10 Oct 2024 14:51
 Operator : RC/JU
 Sample : P4187-21
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY076

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	10.975	1348	1358	1364	rBV2	11905	24500	0.61%	0.075%
38	11.269	1401	1408	1414	rBV10	5863	14260	0.36%	0.043%
39	11.575	1458	1460	1466	rVB7	3210	4745	0.12%	0.014%
40	11.728	1481	1486	1491	rBV6	8036	15032	0.37%	0.046%
41	12.016	1526	1535	1537	rBV10	3482	8321	0.21%	0.025%
42	12.051	1537	1541	1548	rVB	8007	13807	0.34%	0.042%
43	12.416	1599	1603	1608	rVB7	3736	6200	0.15%	0.019%
44	12.645	1635	1642	1652	rVB9	5277	12439	0.31%	0.038%
45	12.828	1668	1673	1677	rBV7	3800	6875	0.17%	0.021%
46	12.928	1684	1690	1696	rBV5	5023	12030	0.30%	0.037%
47	13.016	1696	1705	1706	rBV9	2514	6061	0.15%	0.018%
48	13.186	1729	1734	1741	rVB9	5285	9929	0.25%	0.030%
49	13.345	1752	1761	1770	rVV3	13817	35029	0.87%	0.107%
50	13.716	1817	1824	1834	rBV	1050901	1489572	37.15%	4.541%
51	13.851	1844	1847	1856	rVB	3164	7536	0.19%	0.023%
52	14.010	1864	1874	1888	rBV	1048160	1695552	42.28%	5.169%
53	14.104	1888	1890	1897	rVB8	2366	4606	0.11%	0.014%
54	14.322	1918	1927	1938	rBV	910793	1326822	33.09%	4.045%
55	14.551	1959	1966	1973	rBV	98634	195801	4.88%	0.597%
56	14.739	1994	1998	2003	rVB8	4401	7103	0.18%	0.022%
57	14.851	2012	2017	2022	rBV8	3034	4906	0.12%	0.015%
58	14.969	2032	2037	2038	rBV5	5219	7239	0.18%	0.022%
59	15.063	2050	2053	2057	rVB5	3862	4464	0.11%	0.014%
60	15.127	2061	2064	2067	rBV5	3397	4439	0.11%	0.014%
61	15.327	2090	2098	2104	rBV	1419940	2281173	56.89%	6.954%
62	15.374	2104	2106	2112	rVV2	22976	28866	0.72%	0.088%
63	15.439	2112	2117	2129	rVV	579188	757147	18.88%	2.308%
64	15.563	2132	2138	2144	rVV	19908	31626	0.79%	0.096%
65	15.704	2154	2162	2167	rBV	39576	59095	1.47%	0.180%
66	15.845	2182	2186	2190	rVB5	4596	6338	0.16%	0.019%
67	16.280	2255	2260	2263	rBV7	2620	5485	0.14%	0.017%
68	16.386	2272	2278	2280	rBV7	5337	9284	0.23%	0.028%
69	16.774	2338	2344	2350	rBV7	7579	16061	0.40%	0.049%
70	17.116	2395	2402	2412	rBV	1322595	1848830	46.11%	5.636%
71	17.210	2412	2418	2429	rVB	1869035	2859159	71.30%	8.716%
72	17.757	2507	2511	2513	rBV5	3359	5514	0.14%	0.017%
73	17.804	2517	2519	2524	rVB5	4728	7094	0.18%	0.022%
74	18.051	2556	2561	2569	rBV	76957	107678	2.69%	0.328%
75	19.139	2742	2746	2750	rBV4	25445	37338	0.93%	0.114%
76	19.215	2756	2759	2763	rBV	32702	38277	0.95%	0.117%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022323.D
Acq On : 10 Oct 2024 14:51
Operator : RC/JU
Sample : P4187-21
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY076

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

77	19.386	2784	2788	2794	rBV6	26782	39734	0.99%	0.121%
78	19.598	2818	2824	2830	rBV	3032022	3760525	93.78%	11.463%
79	21.539	3148	3154	3163	rVB2	1463746	2241870	55.91%	6.834%
80	24.603	3665	3675	3689	rVB	1440003	4009962	100.00%	12.224%
81	24.833	3705	3714	3725	rVB	904763	2380296	59.36%	7.256%




Sum of corrected areas: 32804894

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022323.D
Acq On : 10 Oct 2024 14:51
Operator : RC/JU
Sample : P4187-21
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY076

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

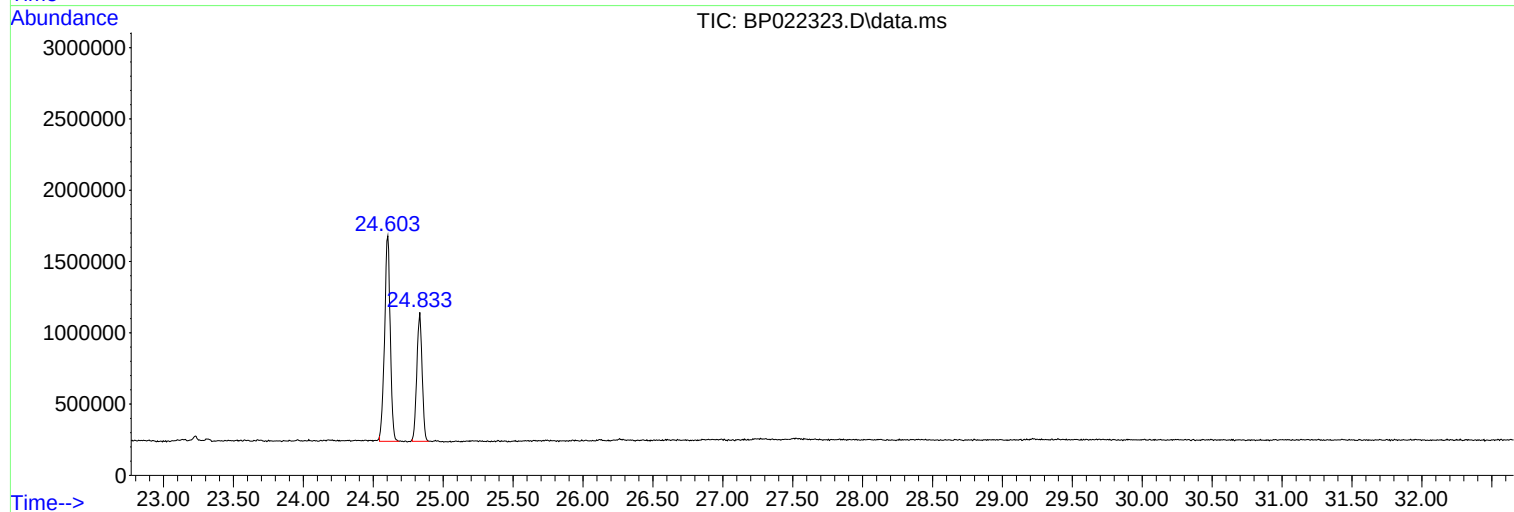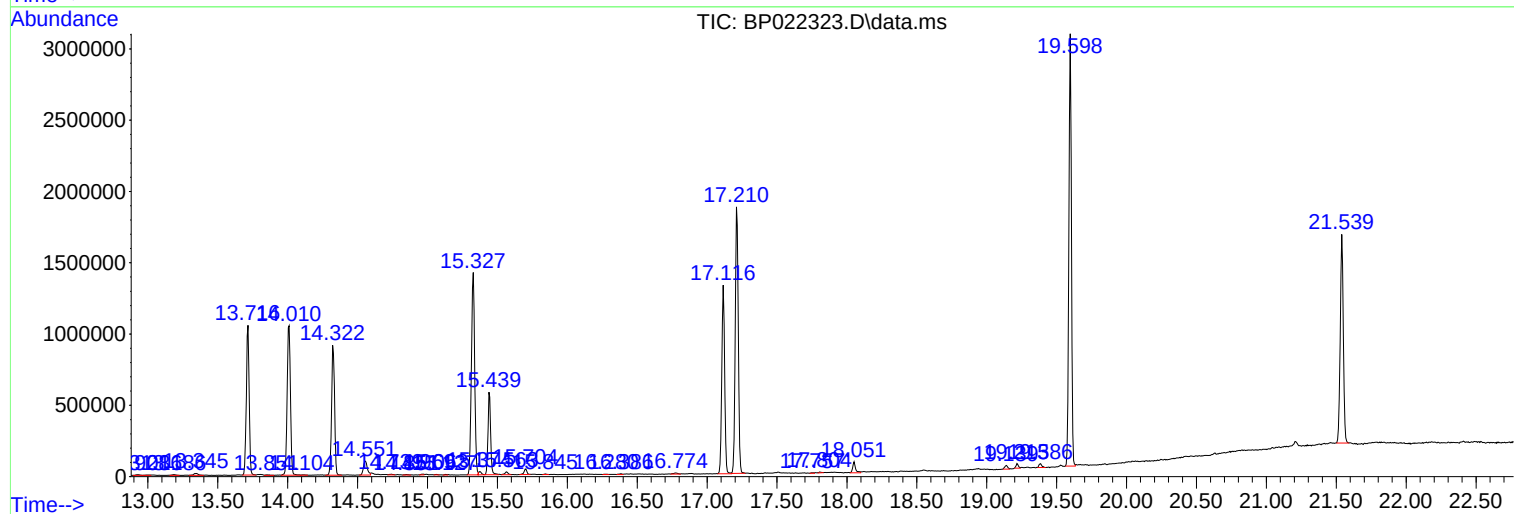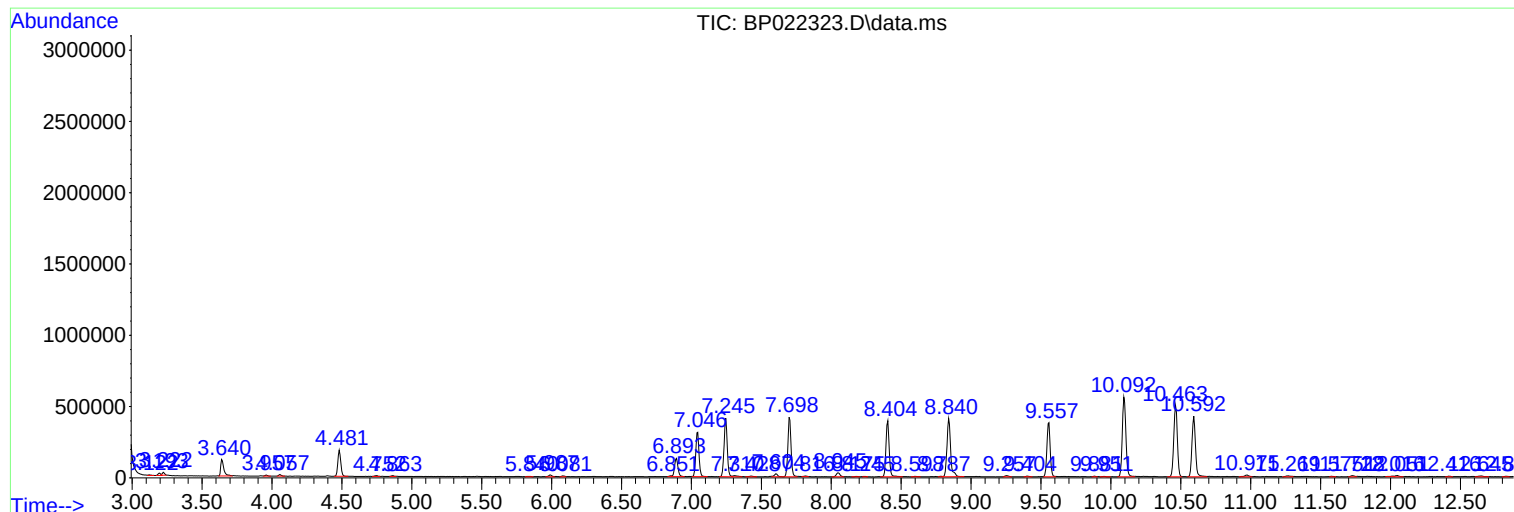

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022323.D
Acq On : 10 Oct 2024 14:51
Operator : RC/JU
Sample : P4187-21
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY076










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.481	8.16 ng/ul	268136	1,4-Dichlorobenzene-d4	7.698

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

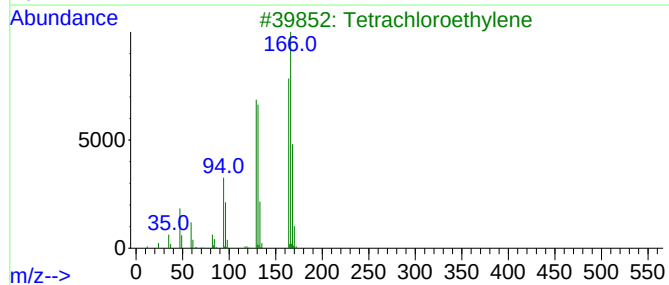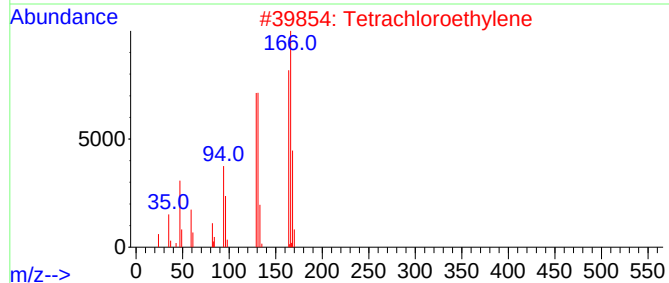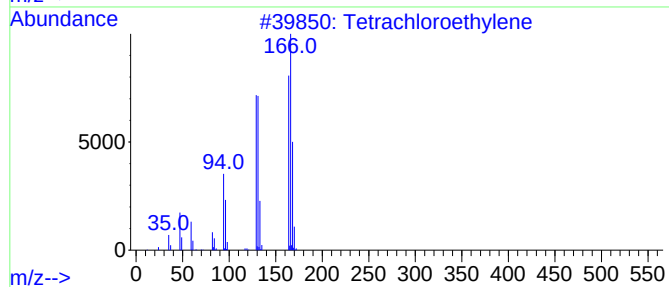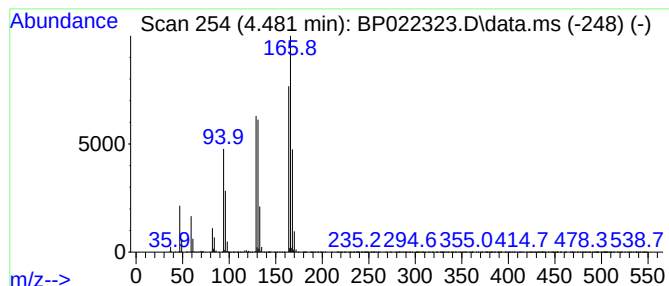

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022323.D
Acq On : 10 Oct 2024 14:51
Operator : RC/JU
Sample : P4187-21
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY076

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.481	8.2	ng/ul	268136	1	7.698	657079	20.0