
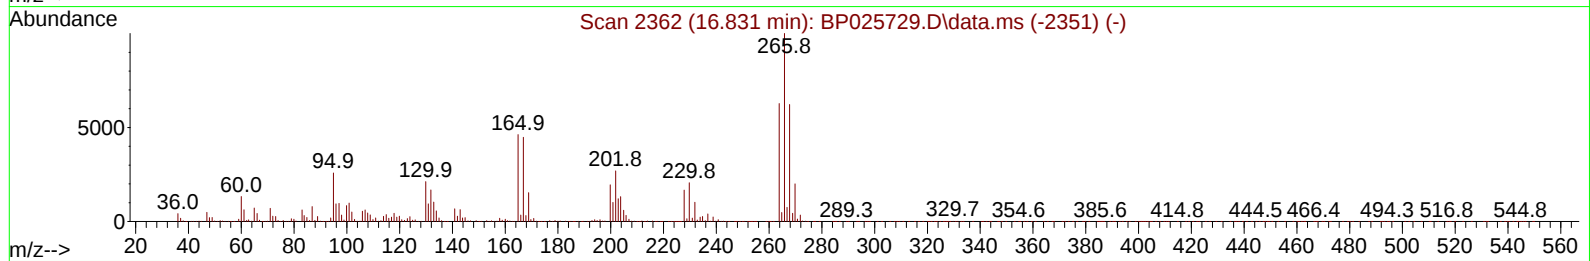
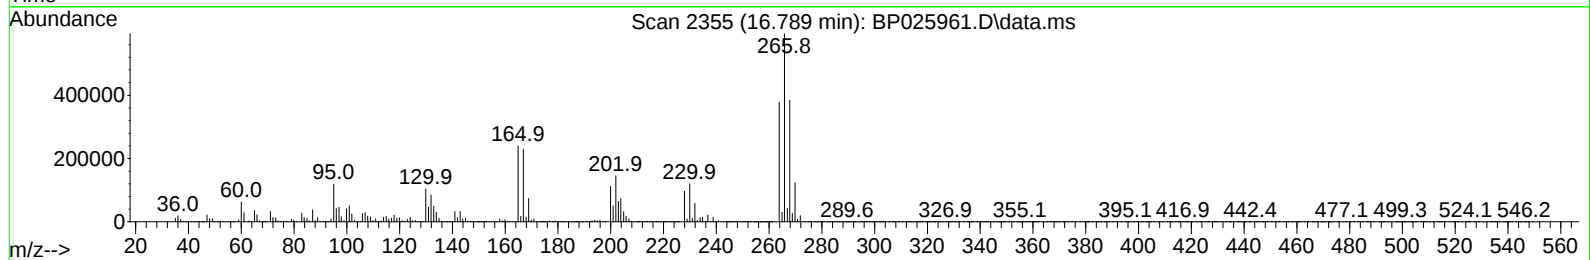


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100925\
Data File : BP025961.D
Acq On : 09 Oct 2025 11:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 09 13:24:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 08 16:22:13 2025
Response via : Initial Calibration

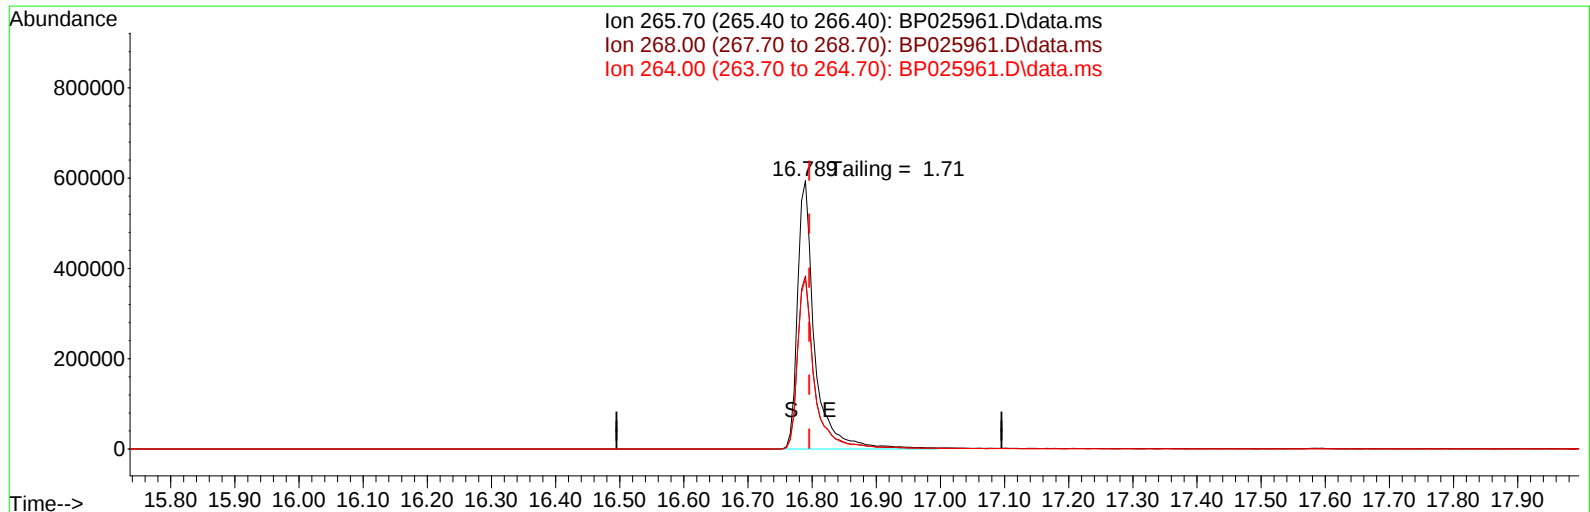

TIC: BP025961.D\data.ms

(70) Pentachlorophenol (C)




16.789min (-0.006) 25595.25 ng

response 1100185

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.49
264.00	62.70	63.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100925\
Data File : BP025961.D
Acq On : 09 Oct 2025 11:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 09 13:24:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 08 16:22:13 2025
Response via : Initial Calibration

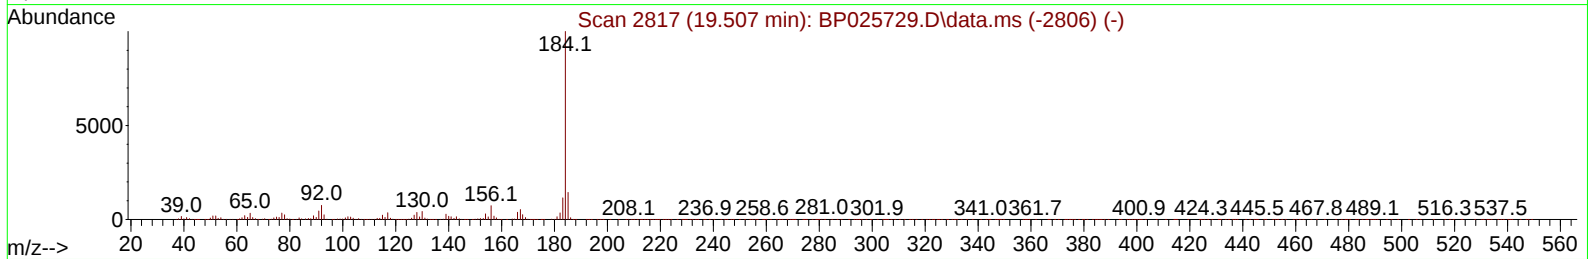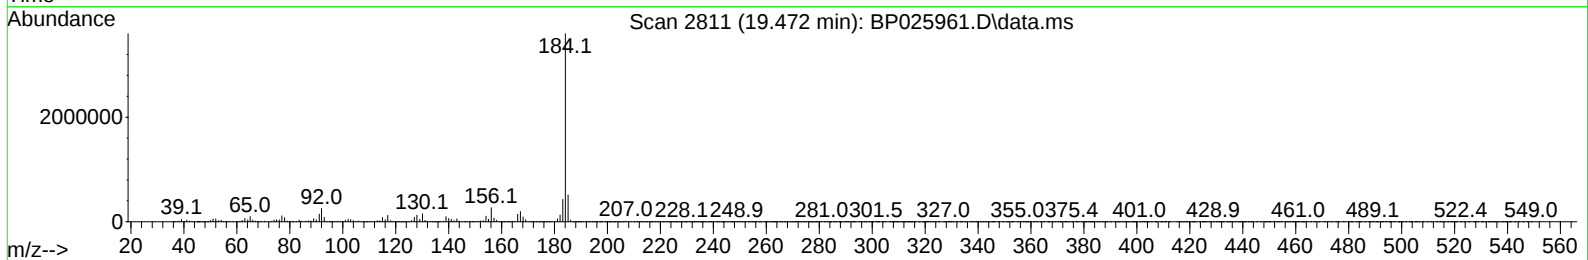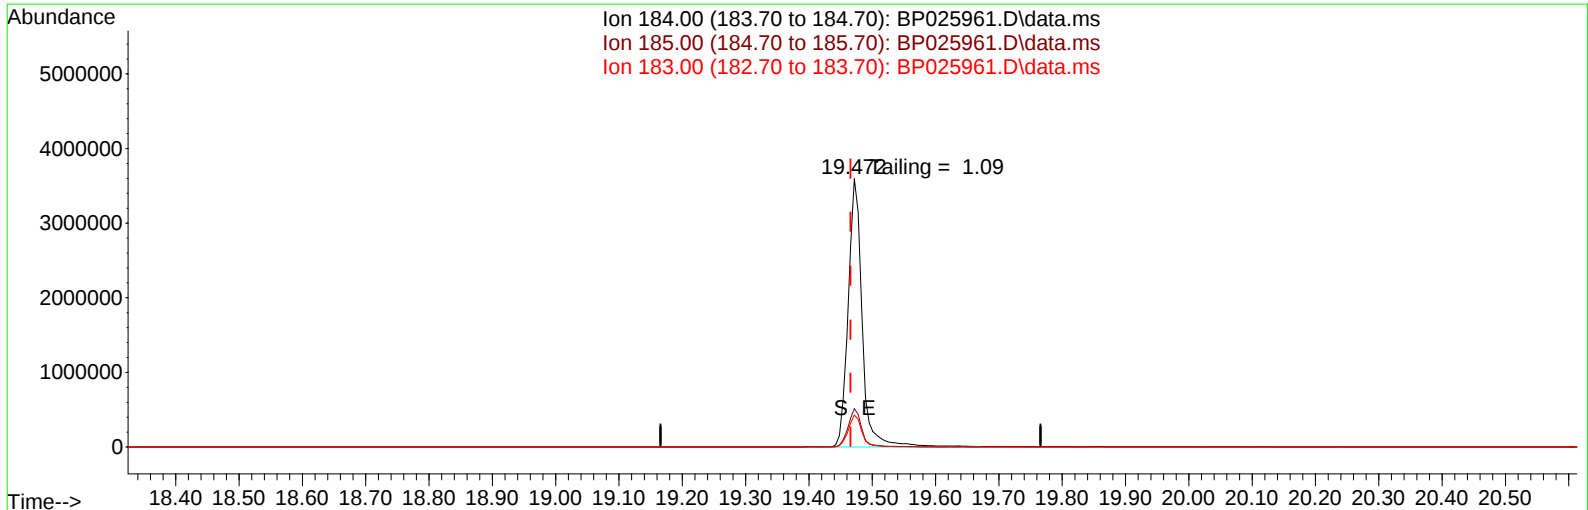

TIC: BP025961.D\data.ms

(77) Benzidine

19.472min (+ 0.006) 5582.46 ng m

response 5546705

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.31
183.00	11.50	11.94
0.00	0.00	0.00