

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100925\
Data File : BP025963.D
Acq On : 09 Oct 2025 13:44
Operator : RC/JU
Sample : PB170038BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170038BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP025963.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.372	408	414	442	rBV	2578581	4622034	40.62%	10.023%
2	6.937	673	680	717	rBV	2176732	4592195	40.35%	9.958%
3	7.725	807	814	830	rBV	520437	884133	7.77%	1.917%
4	8.878	1002	1010	1047	rBV	1370503	2967082	26.07%	6.434%
5	10.502	1276	1286	1304	rBV	442159	1161630	10.21%	2.519%
6	12.948	1692	1702	1718	rBV	3087487	6683155	58.73%	14.492%
7	14.354	1932	1941	1966	rBV	764980	1595328	14.02%	3.459%
8	15.860	2189	2197	2223	rBV	2557917	5639891	49.56%	12.230%
9	17.148	2408	2416	2446	rBV2	764999	2036026	17.89%	4.415%
10	19.854	2870	2876	2891	rBV	8102926	11379602	100.00%	24.676%
11	21.595	3165	3172	3189	rBV	1002870	2357182	20.71%	5.111%
12	24.924	3731	3738	3758	rVB	672615	2197494	19.31%	4.765%




Sum of corrected areas: 46115752

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100925\
Data File : BP025963.D
Acq On : 09 Oct 2025 13:44
Operator : RC/JU
Sample : PB170038BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170038BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

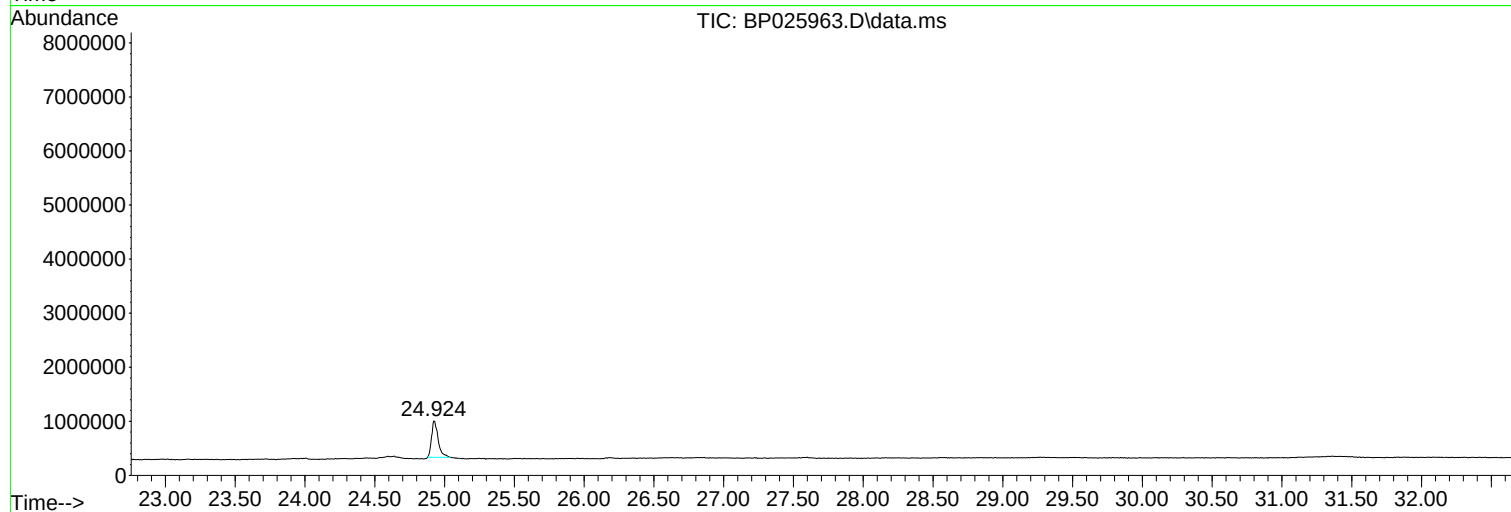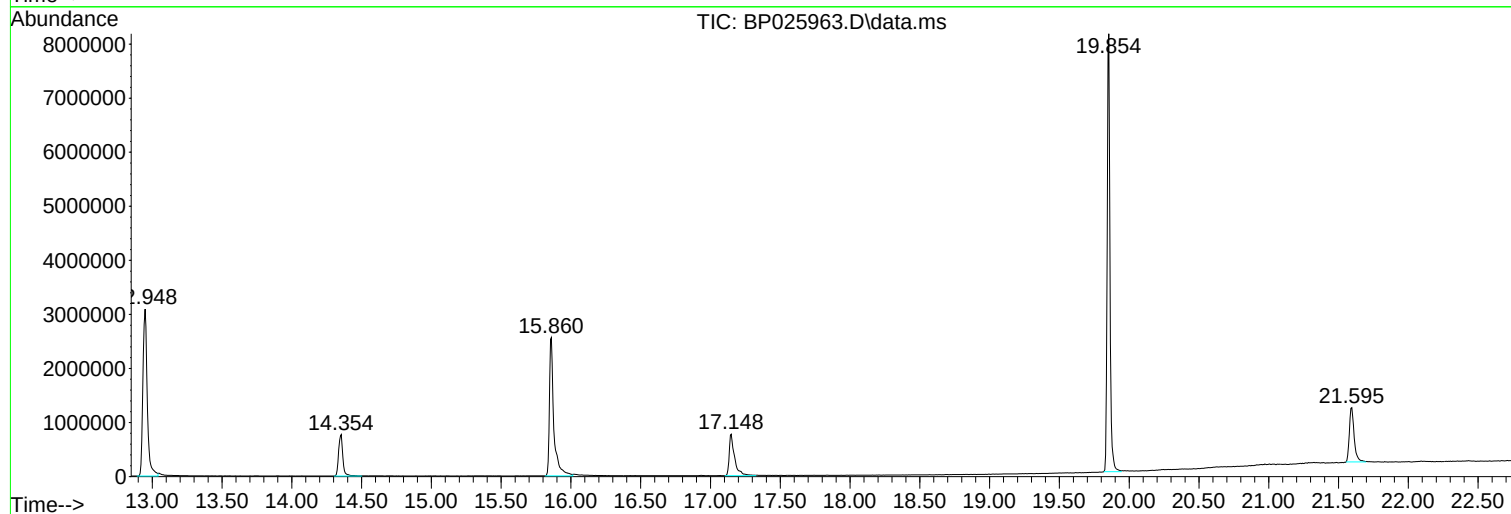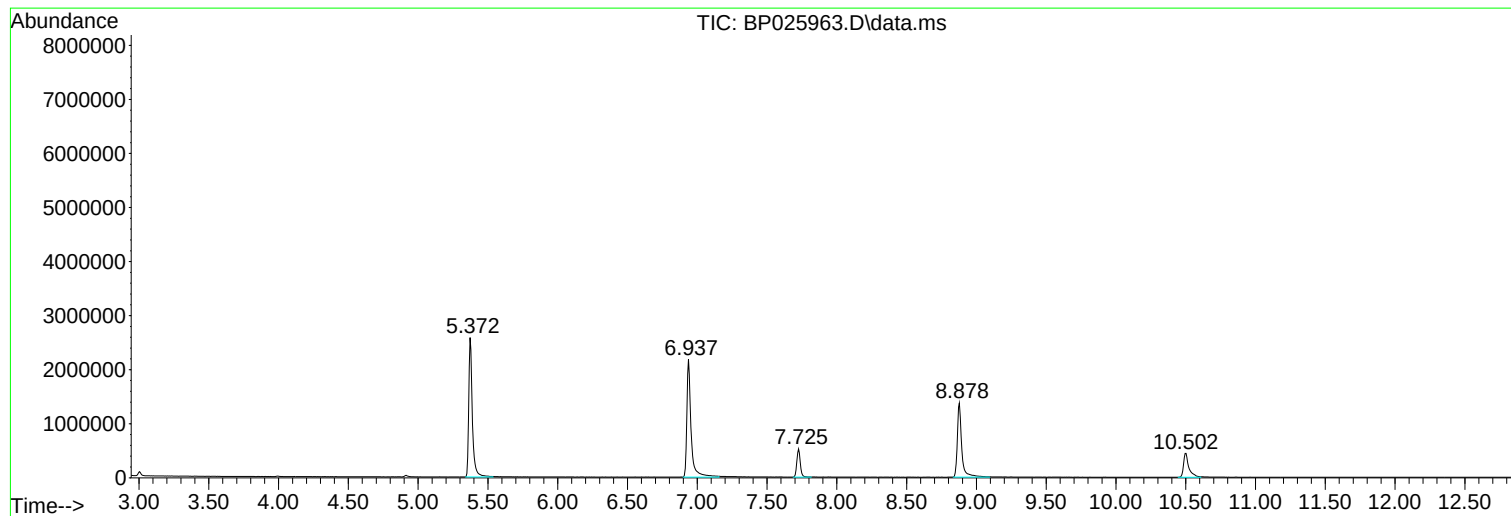

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100925\
Data File : BP025963.D
Acq On : 09 Oct 2025 13:44
Operator : RC/JU
Sample : PB170038BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170038BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100925\
Data File : BP025963.D
Acq On : 09 Oct 2025 13:44
Operator : RC/JU
Sample : PB170038BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170038BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------