


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100925\
Data File : BP025961.D
Acq On : 09 Oct 2025 11:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 08 16:22:13 2025

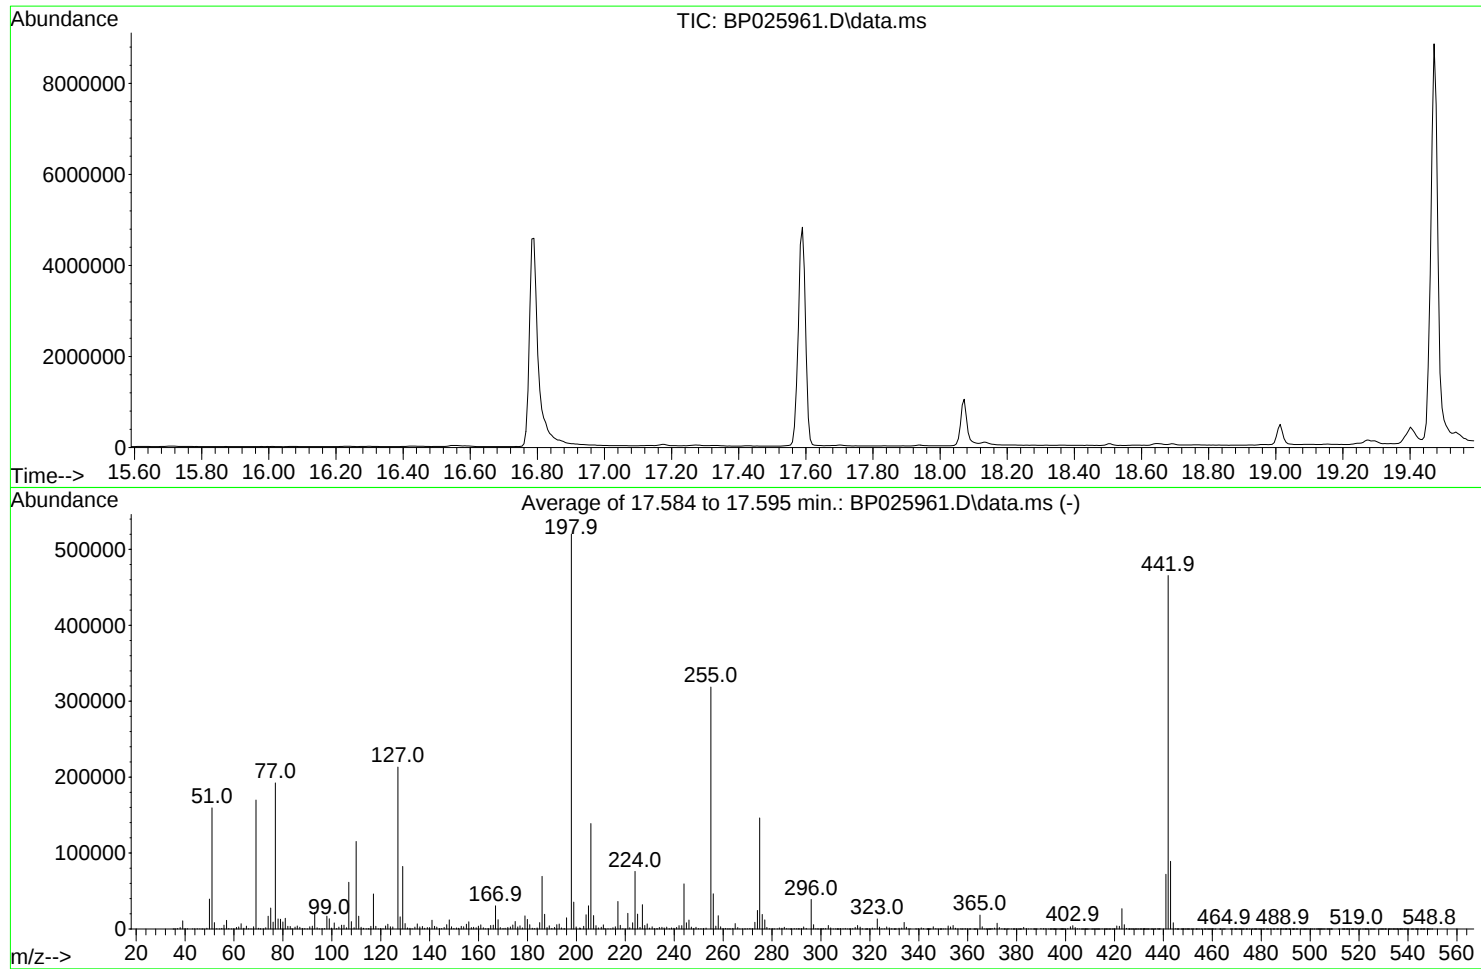




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2478

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	2950	PASS
69	69	100	100	100.0	169756	PASS
70	69	0.00	2	0.6	1024	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	520145	PASS
199	198	5	9	6.8	35307	PASS
365	198	1	100	3.5	18208	PASS
441	443	0.01	150	80.9	72056	PASS
442	442	100	100	100.0	465594	PASS
443	442	15	24	19.1	89031	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100925\
Data File : BP025961.D
Acq On : 09 Oct 2025 11:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 09 13:24:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 08 16:22:13 2025
Response via : Initial Calibration

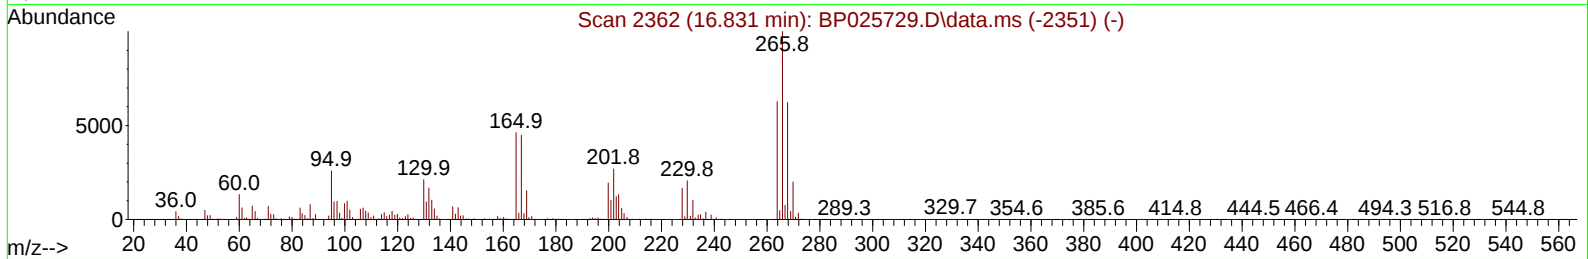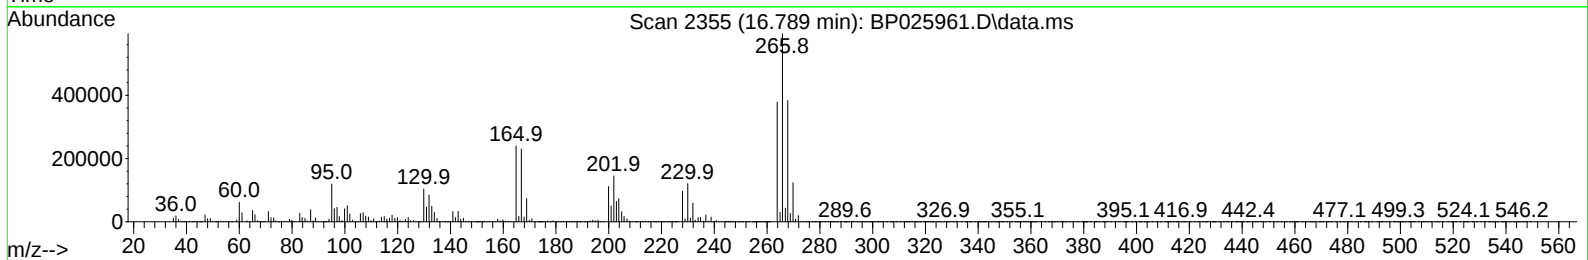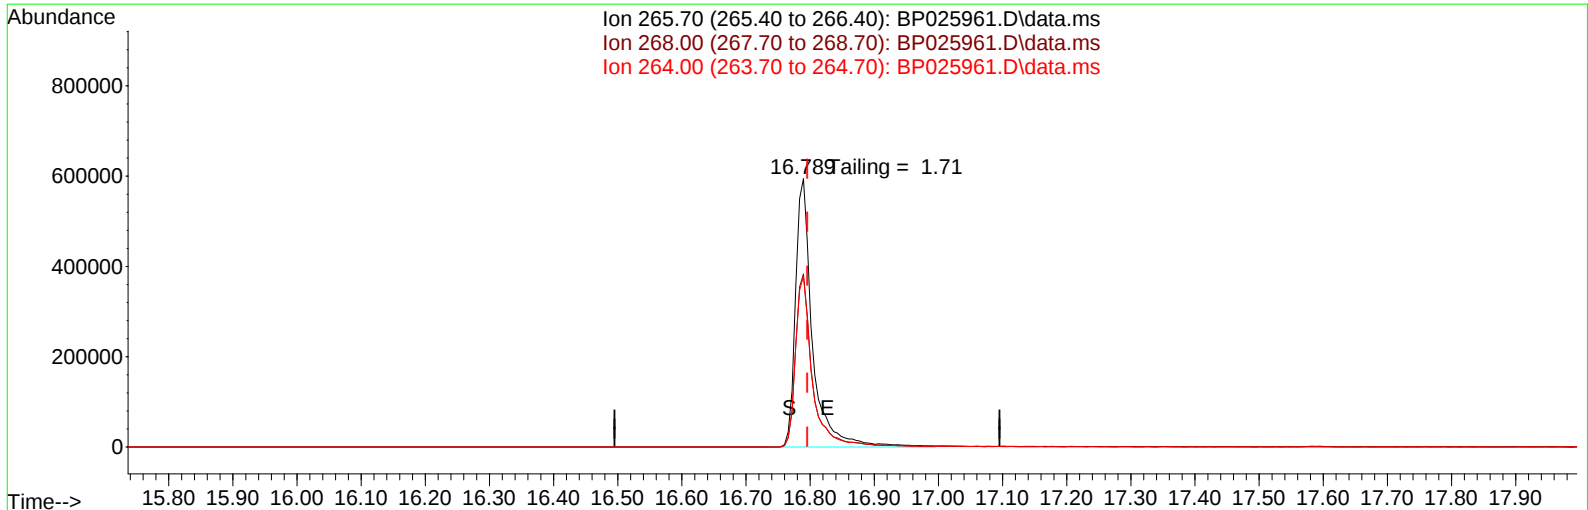

TIC: BP025961.D\data.ms

(70) Pentachlorophenol (C)

16.789min (-0.006) 25595.25 ng




response 1100185

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.49
264.00	62.70	63.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100925\
Data File : BP025961.D
Acq On : 09 Oct 2025 11:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 09 13:24:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 08 16:22:13 2025
Response via : Initial Calibration

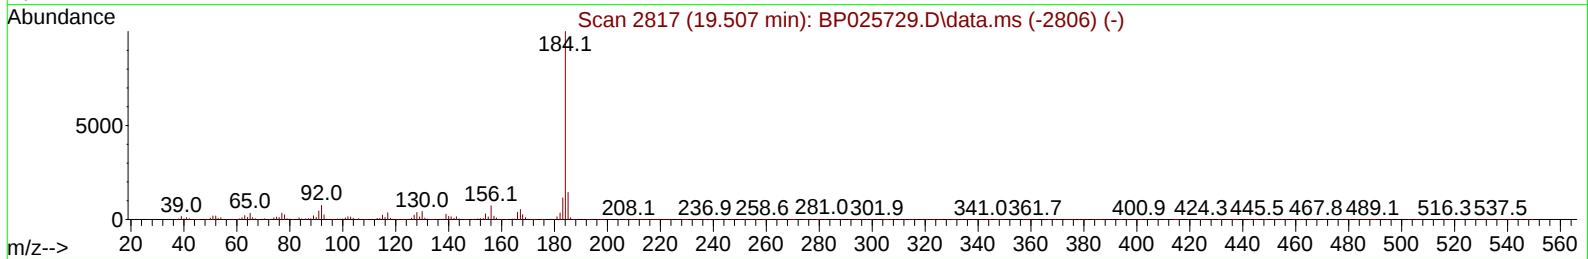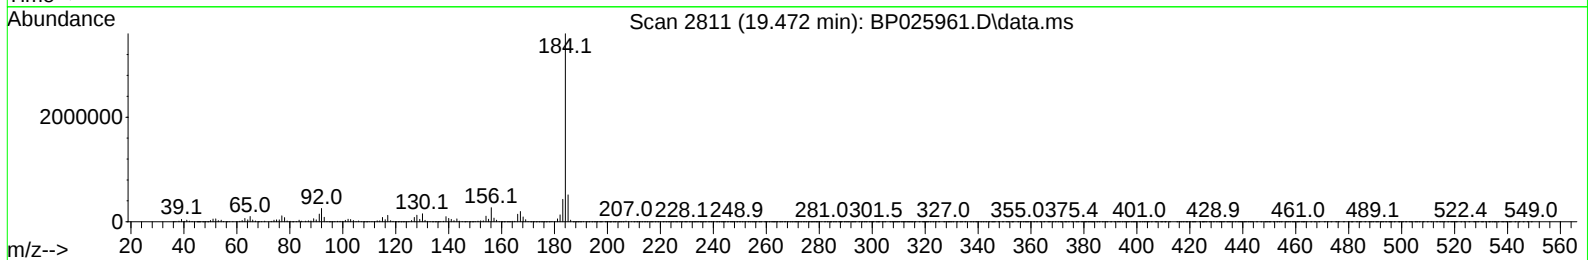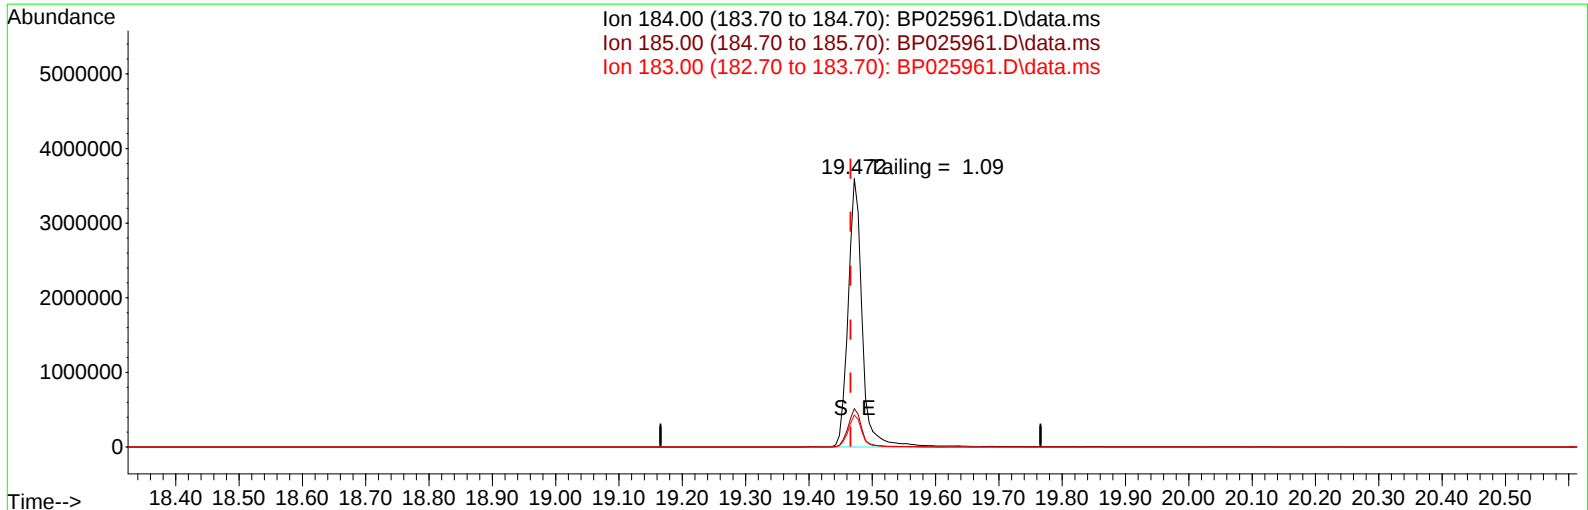

TIC: BP025961.D\data.ms

(77) Benzidine

19.472min (+ 0.006) 5582.46 ng m

response 5546705

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.31
183.00	11.50	11.94
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/9/2025	BNA_P	<u>BP025961.D</u>
Compound Name	Response	Retention Time
DDT	2521730	20.748
DDD	47719	20.295
DDE	375	19.095
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
48094	2569824	1.87

Instrument :
BNA_P
ClientSampleId :
DFTPP