

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012054.D
 Acq On : 11 Oct 2022 23:09
 Operator : CG/JU
 Sample : N4991-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BF3

Quant Time: Oct 12 00:25:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 11 23:54:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.858	152	261890	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	1093263	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.504	164	665234	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.263	188	1447342	20.000	ng/ul	0.00
79) Chrysene-d12	21.351	240	1505049	20.000	ng/ul	0.00
88) Perylene-d12	23.769	264	1626326	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	23847	3.590	ng/uL	0.00
4) Pyridine-d5	3.711	84	164	0.009	ng/ul	0.00
7) Phenol-d5	7.022	99	426930	20.269	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	261616	21.882	ng/ul	0.00
11) 2-Chlorophenol-d4	7.387	132	372947	22.307	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	311438	19.251	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	177555	22.996	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143	172959	22.092	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	326404	21.512	ng/ul	0.00
31) 4-Chloroaniline-d4	10.804	131	371717	16.624	ng/ul	0.00
46) Dimethylphthalate-d6	13.916	166	952483	22.608	ng/ul	0.00
49) Acenaphthylene-d8	14.198	160	1227683	23.565	ng/ul	0.00
54) 4-Nitrophenol-d4	14.716	143	91911	11.112	ng/ul	0.00
60) Fluorene-d10	15.498	176	974752	25.572	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.628	200	73440	9.610	ng/ul	0.00
73) Anthracene-d10	17.363	188	1544569	24.576	ng/ul	0.00
81) Pyrene-d10	19.598	212	1979258	25.670	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.610	264	2005614	25.368	ng/ul	0.00
Target Compounds						
					Qvalue	
80) Fluoranthene	19.275	202	101973	1.079	ng/ul	98
82) Pyrene	19.628	202	101724	1.017	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012054.D
Acq On : 11 Oct 2022 23:09
Operator : CG/JU
Sample : N4991-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BF3

Quant Time: Oct 12 00:25:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 11 23:54:43 2022
Response via : Initial Calibration

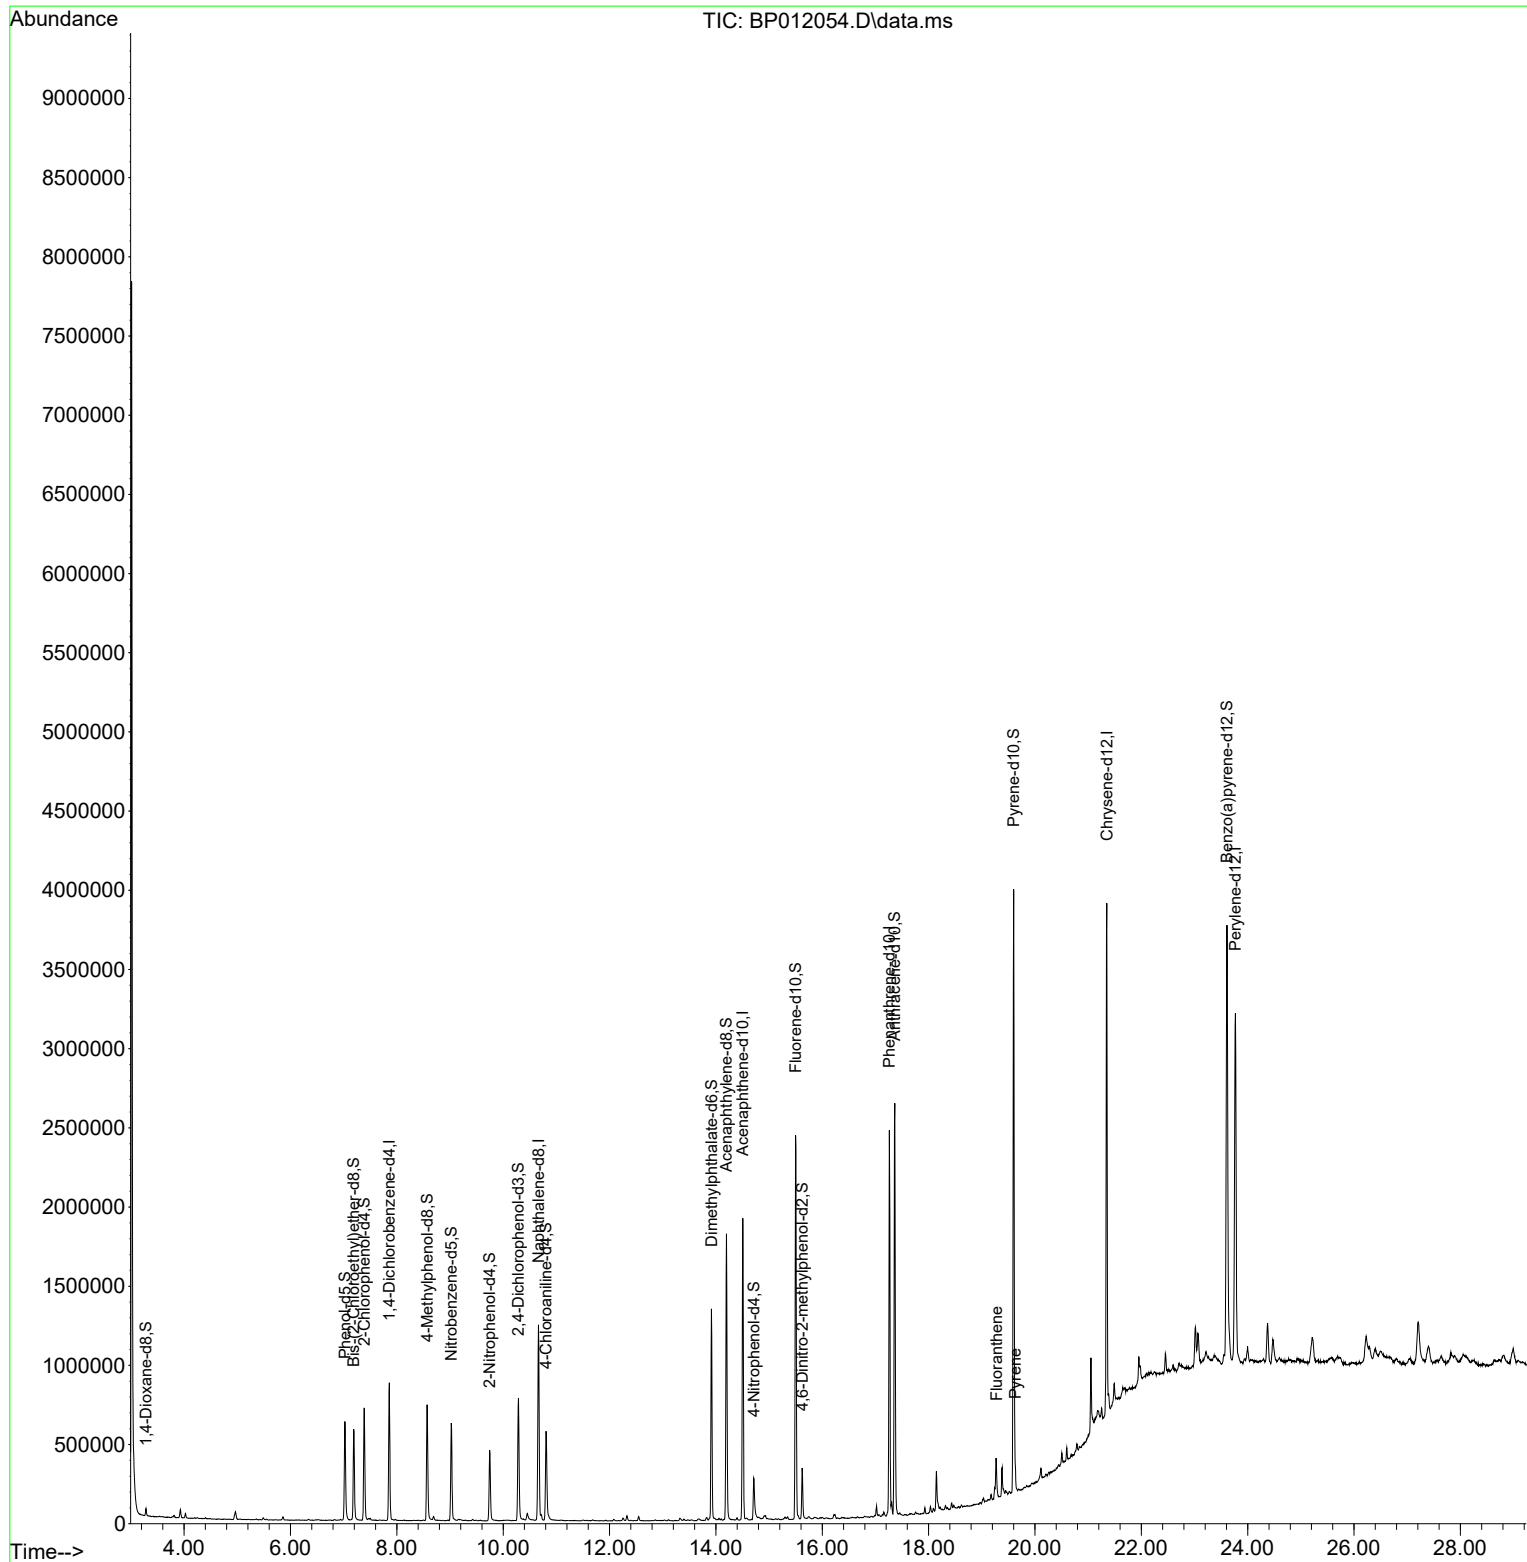

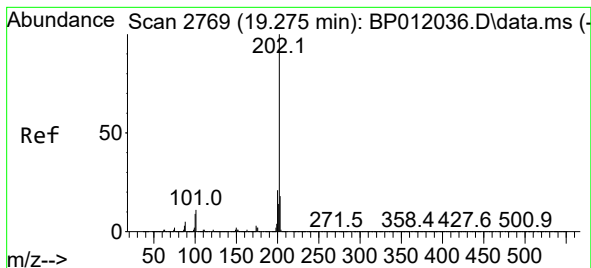

#80

Fluoranthene

Concen: 1.079 ng/ul

RT: 19.275 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP012054.D

Acq: 11 Oct 2022 23:09

Instrument :

BNA_P

ClientSampleId :

C0BF3





Tgt Ion:202 Resp: 101973

Ion Ratio Lower Upper

202 100

101 11.7 9.0 13.6

100 7.8 7.0 10.6

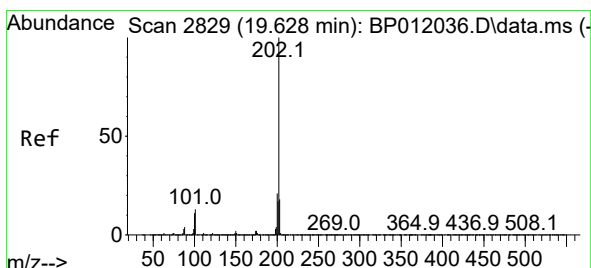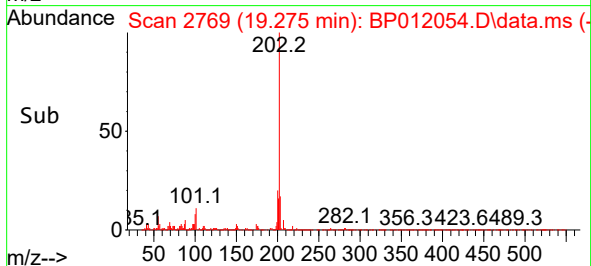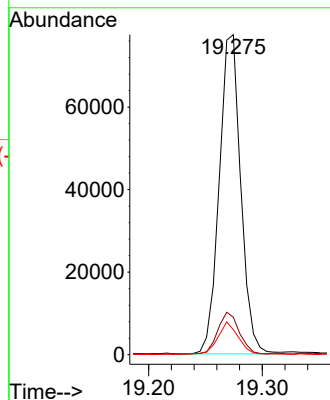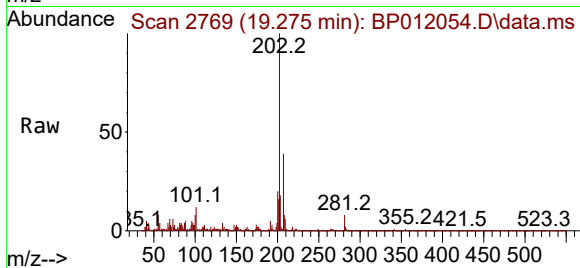

#82

Pyrene

Concen: 1.017 ng/ul

RT: 19.628 min Scan# 2829

Delta R.T. 0.000 min

Lab File: BP012054.D

Acq: 11 Oct 2022 23:09

Tgt Ion:202 Resp: 101724

Ion Ratio Lower Upper

202 100

101 14.2 10.4 15.6

100 11.0 8.5 12.7

