




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012087.D
Acq On : 12 Oct 2022 18:38
Operator : CG/JU
Sample : N4976-08
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8Y5

Manual IntegrationsAPPROVED

Quant Time: Oct 12 23:09:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 12 23:03:21 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

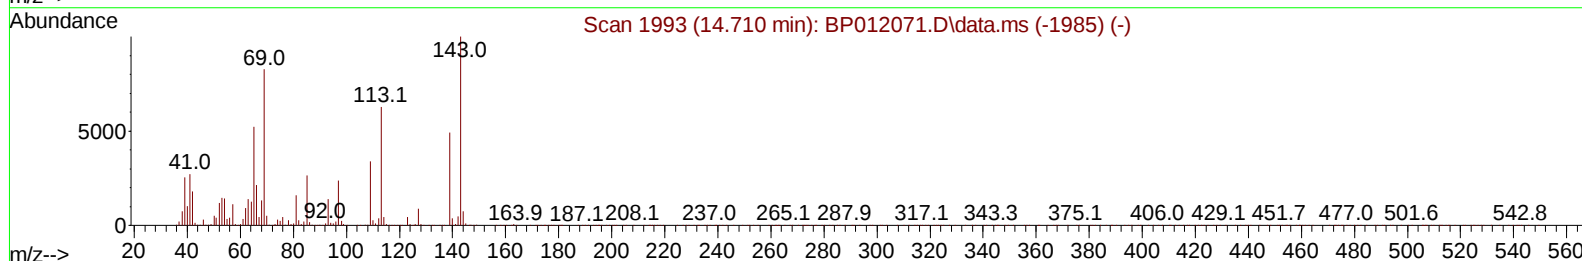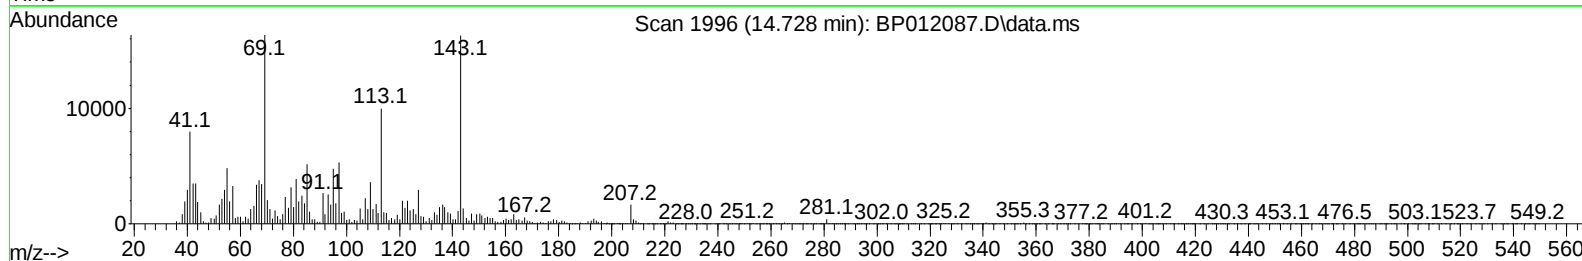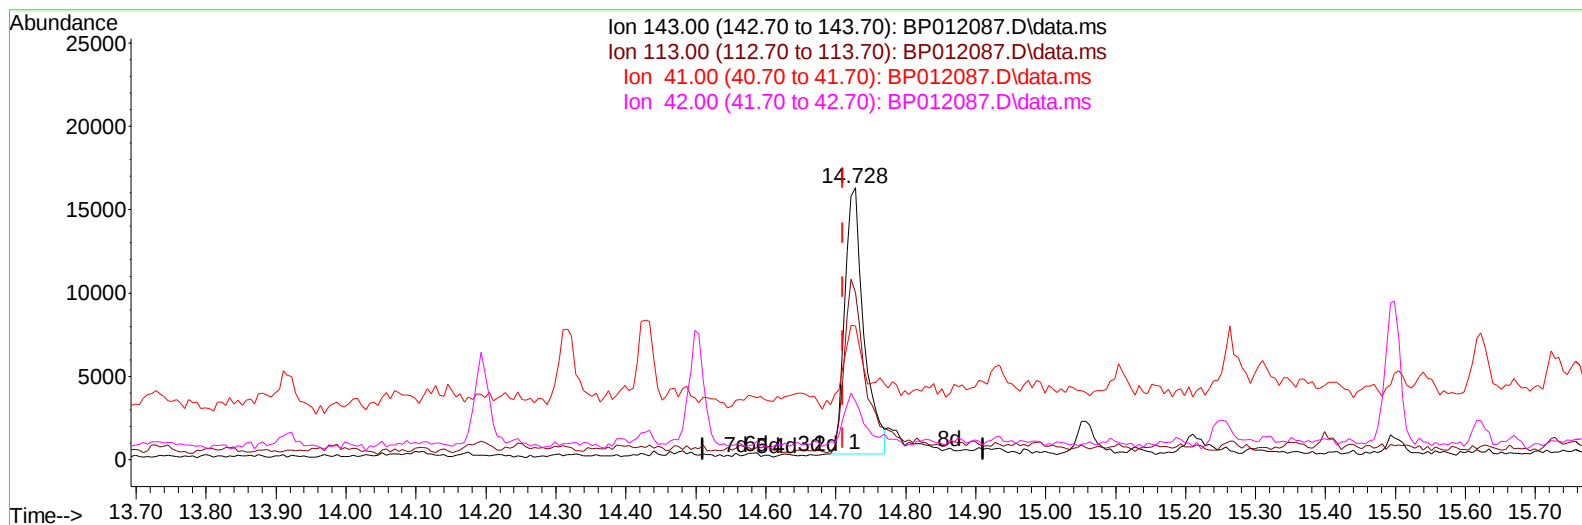

TIC: BP012087.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.728min (+ 0.018) 4.42 ng/ul

response 30251

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	60.80	61.33
41.00	26.60	49.10#
42.00	17.60	21.36#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012087.D
 Acq On : 12 Oct 2022 18:38
 Operator : CG/JU
 Sample : N4976-08
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8Y5

Manual IntegrationsAPPROVED

Quant Time: Oct 12 23:09:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 12 23:03:21 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/13/2022
 Supervised By :mohammad ahmed 10/14/2022

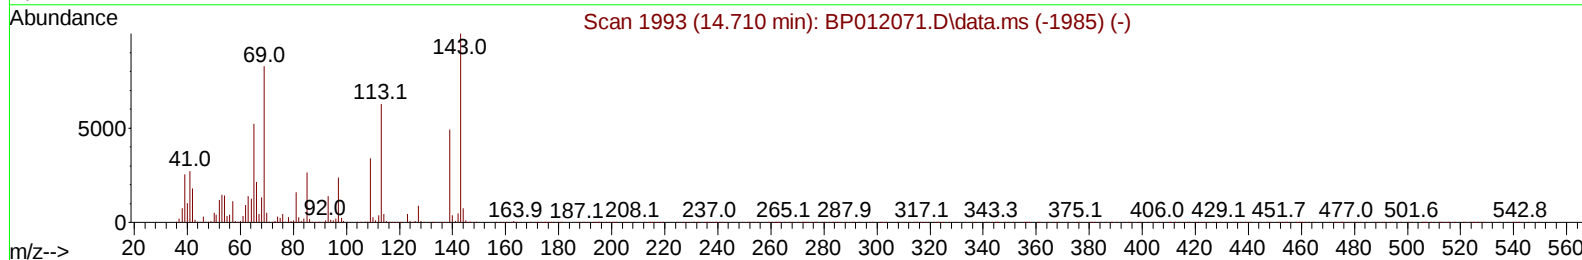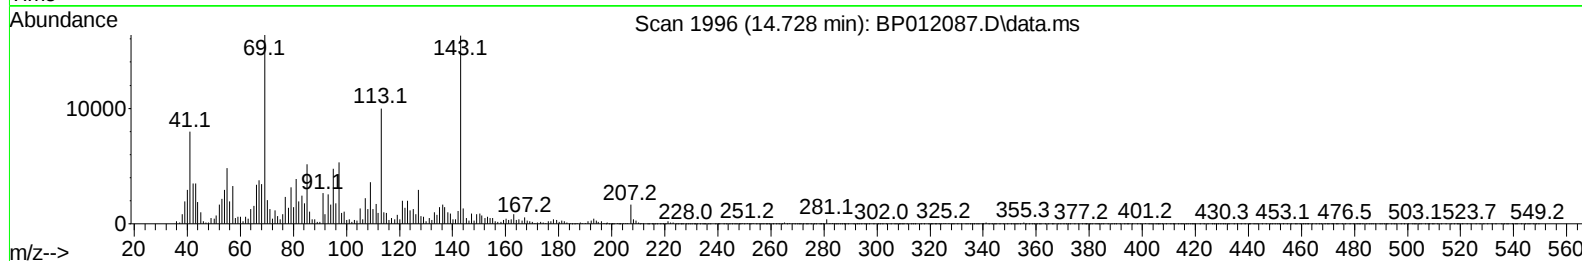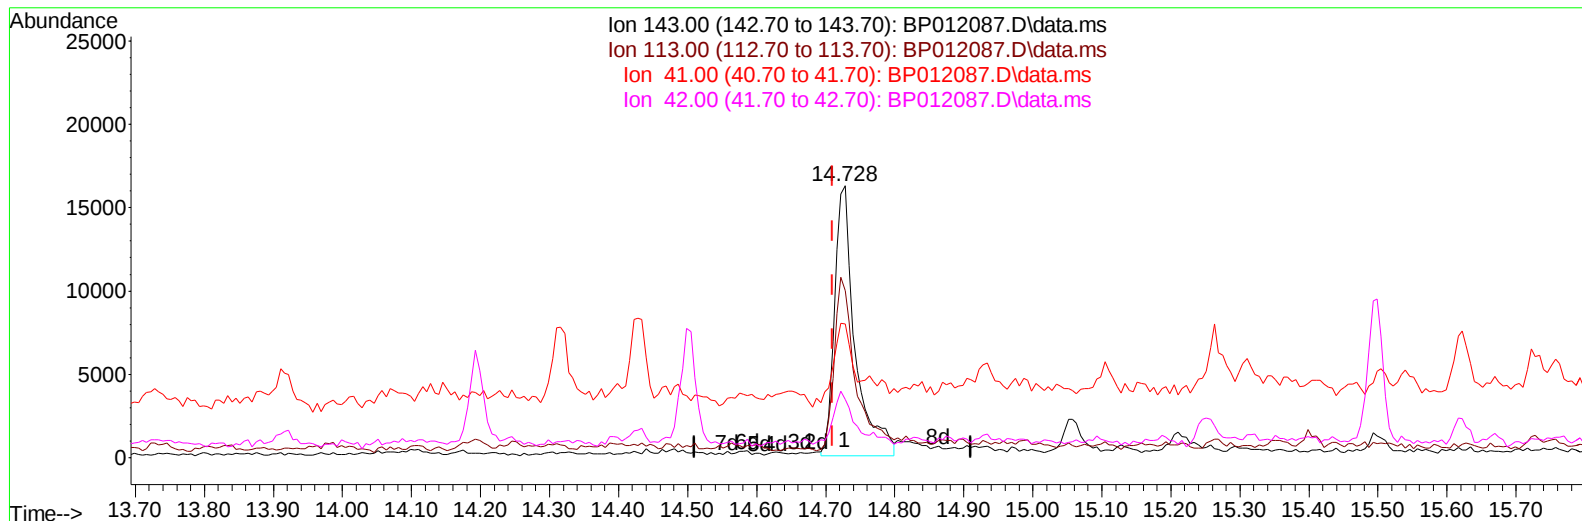

TIC: BP012087.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.728min (+ 0.018) 4.93 ng/ul m

response 33768

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	60.80	61.33
41.00	26.60	49.10#
42.00	17.60	21.36#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012087.D
 Acq On : 12 Oct 2022 18:38
 Operator : CG/JU
 Sample : N4976-08
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8Y5

Manual IntegrationsAPPROVED

Quant Time: Oct 12 23:09:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 12 23:03:21 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/13/2022
 Supervised By :mohammad ahmed 10/14/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	269760	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	1052298	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.499	164	550990	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.257	188	1076895	20.000	ng/ul	0.00
79) Chrysene-d12	21.351	240	1184756	20.000	ng/ul	0.00
88) Perylene-d12	23.769	264	1321381	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.276	96	23717	3.466	ng/uL	0.00
4) Pyridine-d5	3.705	84	197302	10.843	ng/ul	0.00
7) Phenol-d5	7.022	99	117048	5.395	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	262461	21.313	ng/ul	0.00
11) 2-Chlorophenol-d4	7.387	132	309013	17.943	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	215161	12.911	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	176790	23.788	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143	181053	24.026	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	335640	22.982	ng/ul	0.00
31) 4-Chloroaniline-d4	10.805	131	406200	18.874	ng/ul	0.00
46) Dimethylphthalate-d6	13.916	166	997736	28.592	ng/ul	0.00
49) Acenaphthylene-d8	14.193	160	1097785	25.441	ng/ul	0.00
54) 4-Nitrophenol-d4	14.728	143	33768m	4.929	ng/ul	0.02
60) Fluorene-d10	15.498	176	837952	26.541	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.622	200	80620	14.178	ng/ul	0.00
73) Anthracene-d10	17.357	188	1351427	28.900	ng/ul	0.00
81) Pyrene-d10	19.598	212	1658279	27.321	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.616	264	1861449	28.979	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.311	88	174667	24.260	ng/uL	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012087.D
Acq On : 12 Oct 2022 18:38
Operator : CG/JU
Sample : N4976-08
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8Y5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

Quant Time: Oct 12 23:09:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 12 23:03:21 2022
Response via : Initial Calibration

