

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012074.D
 Acq On : 12 Oct 2022 11:07
 Operator : CG/JU
 Sample : N5024-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BE6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 10/13/2022
 Supervised By :mohammad ahmed 10/14/2022

Quant Time: Oct 12 23:06:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 12 23:03:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.858	152	239550	20.000	ng/u1	0.00
20) Naphthalene-d8	10.663	136	930451	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.504	164	498732	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.263	188	1044080	20.000	ng/u1	0.00
79) Chrysene-d12	21.351	240	1149902	20.000	ng/u1	0.00
88) Perylene-d12	23.774	264	1262758	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	23872	3.929	ng/uL	0.00
4) Pyridine-d5	3.711	84	66169	4.095	ng/u1	0.01
7) Phenol-d5	7.022	99	343298	17.819	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	224126	20.495	ng/u1	0.00
11) 2-Chlorophenol-d4	7.387	132	320320	20.946	ng/u1	0.00
15) 4-Methylphenol-d8	8.569	113	197818	13.368	ng/u1	0.00
21) Nitrobenzene-d5	9.022	128	144378	21.971	ng/u1	0.00
24) 2-Nitrophenol-d4	9.746	143	148951	22.354	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	266064	20.604	ng/u1	0.00
31) 4-Chloroaniline-d4	10.805	131	267534	14.059	ng/u1	0.00
46) Dimethylphthalate-d6	13.916	166	722317	22.869	ng/u1	0.00
49) Acenaphthylene-d8	14.198	160	874943	22.401	ng/u1	0.00
54) 4-Nitrophenol-d4	14.716	143	78547	12.667	ng/u1	0.00
60) Fluorene-d10	15.498	176	689094	24.114	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.622	200	42920	7.785	ng/u1	0.00
73) Anthracene-d10	17.363	188	1046805	23.089	ng/u1	0.00
81) Pyrene-d10	19.598	212	1422935	24.154	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.616	264	1515340	24.686	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.687	105	39009	1.710	ng/u1	98
50) Acenaphthylene	14.222	152	48480	1.097	ng/u1	98
72) Phenanthrene	17.304	178	249137	4.388	ng/u1	100
80) Fluoranthene	19.275	202	365101	5.058	ng/u1	99
82) Pyrene	19.628	202	326875	4.279	ng/u1	99
85) Benzo(a)anthracene	21.333	228	137071	1.894	ng/u1	96
87) Chrysene	21.386	228	173470	2.490	ng/u1	96
90) Benzo(b)fluoranthene	23.033	252	234277	2.931	ng/u1#	93
91) Benzo(k)fluoranthene	23.074	252	87984m	1.119	ng/u1	
93) Benzo(a)pyrene	23.663	252	148092	2.077	ng/u1#	91
94) Indeno(1,2,3-cd)pyrene	26.280	276	123031	1.364	ng/u1	99
96) Benzo(g,h,i)perylene	27.062	276	114598	1.410	ng/u1#	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012074.D
Acq On : 12 Oct 2022 11:07
Operator : CG/JU
Sample : N5024-01
Misc :
ALS Vial : 43 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
C0BE6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022


Quant Time: Oct 12 23:06:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 12 23:03:21 2022
Response via : Initial Calibration

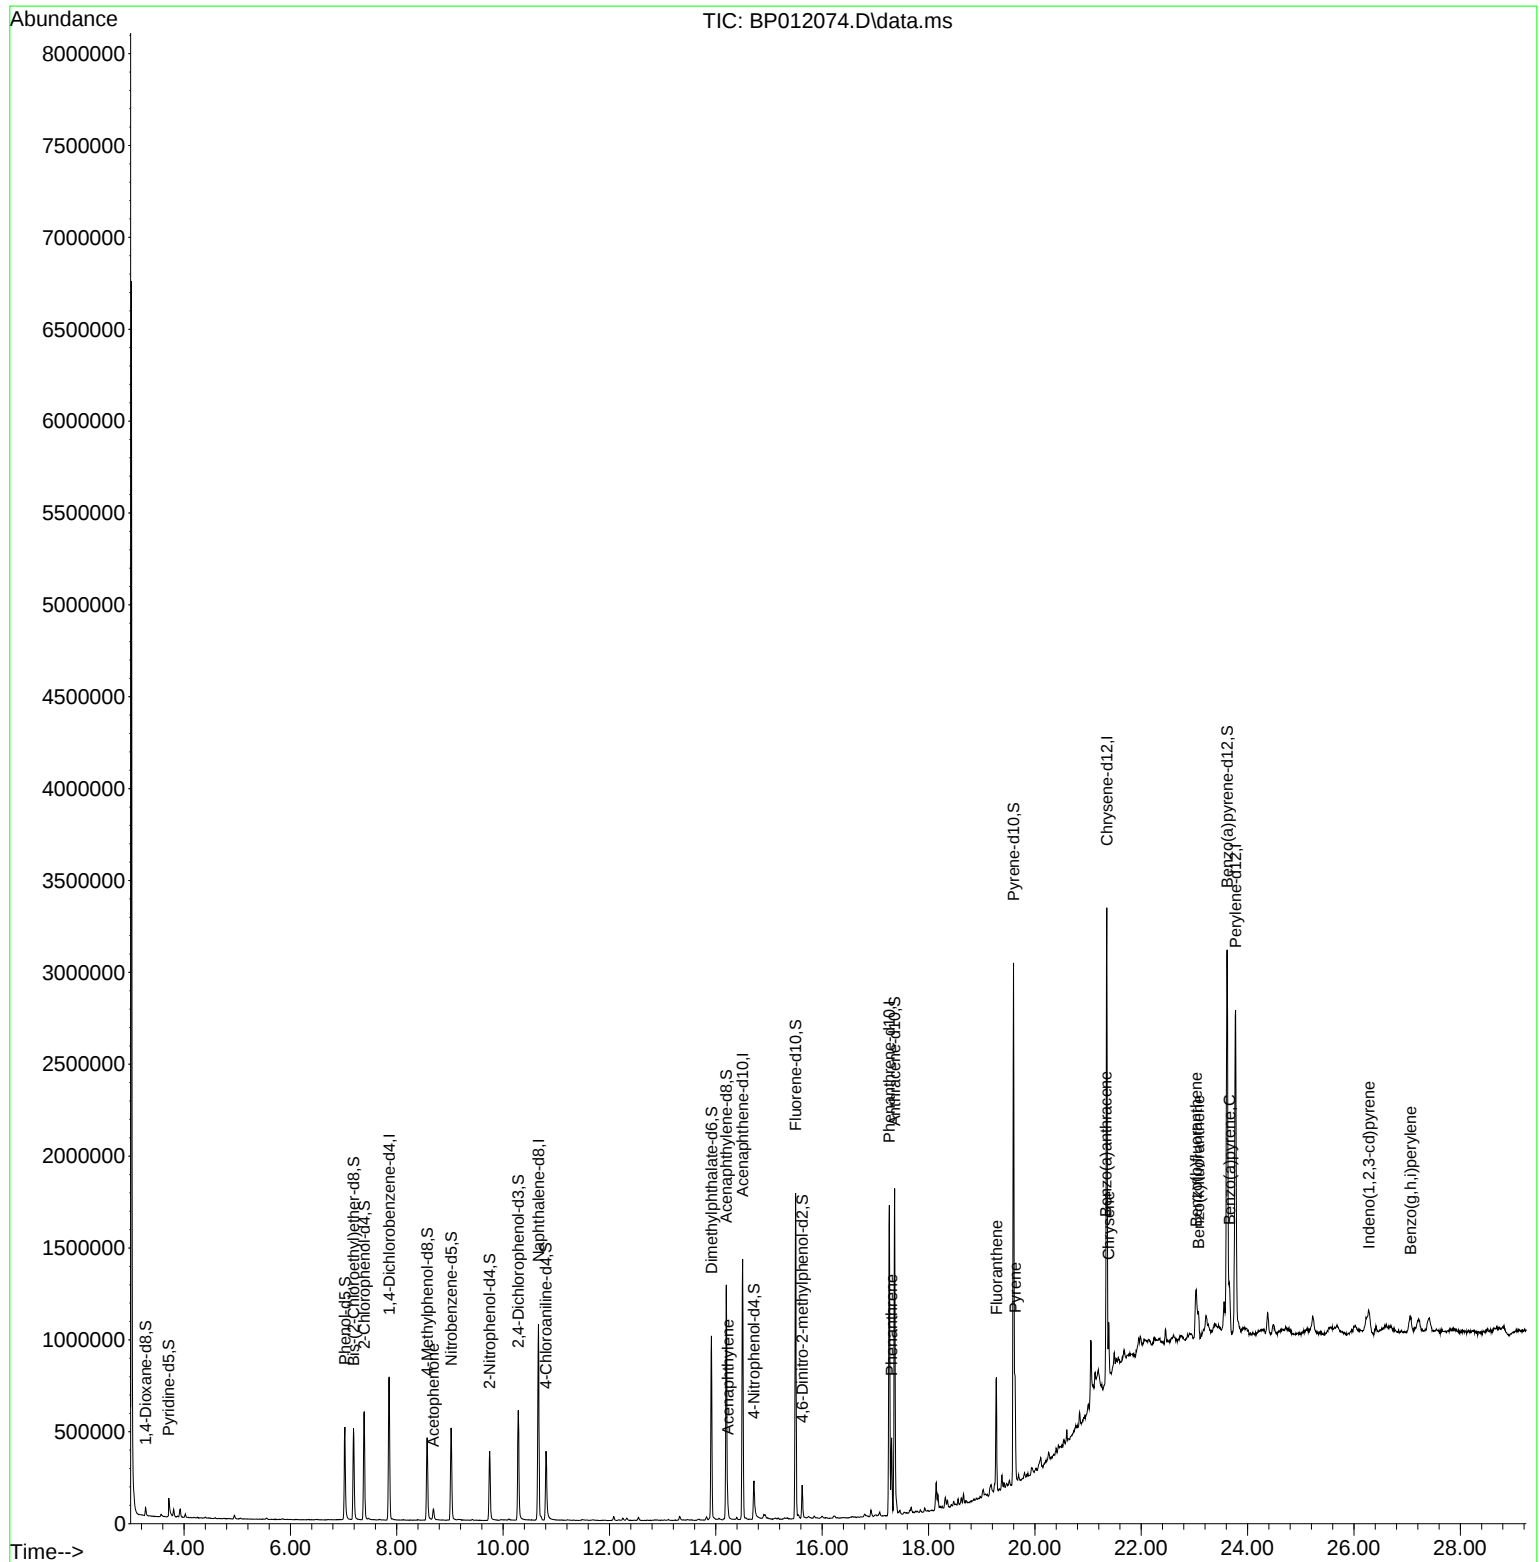

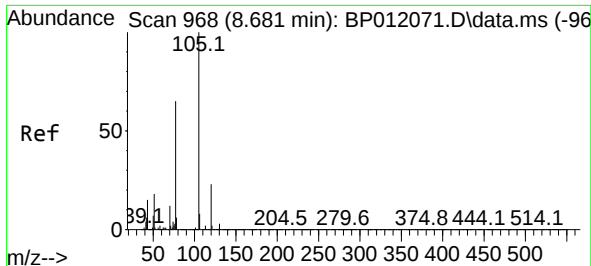

#16
Acetophenone
Concen: 1.710 ng/ul
RT: 8.687 min Scan# 968
Delta R.T. 0.006 min
Lab File: BP012074.D
Acq: 12 Oct 2022 11:07




Instrument :
BNA_P
ClientSampleId :
C0BE6

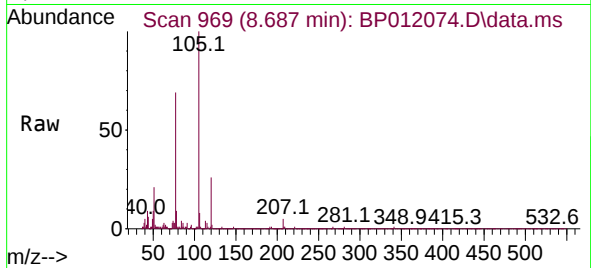

Tgt Ion:105 Resp: 39009
Ion Ratio Lower Upper
105 100
77 69.0 57.0 85.4
51 20.6 16.4 24.6




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

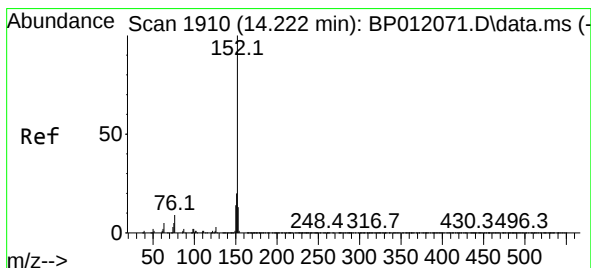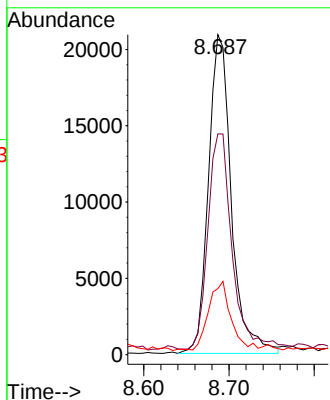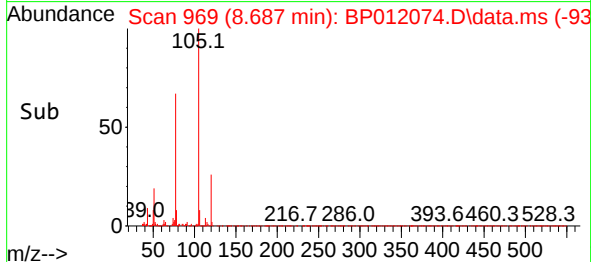

#50
Acenaphthylene
Concen: 1.097 ng/ul
RT: 14.222 min Scan# 1910
Delta R.T. 0.000 min
Lab File: BP012074.D
Acq: 12 Oct 2022 11:07


Tgt Ion:152 Resp: 48480
Ion Ratio Lower Upper
152 100
151 18.3 15.7 23.5
153 12.9 10.4 15.6

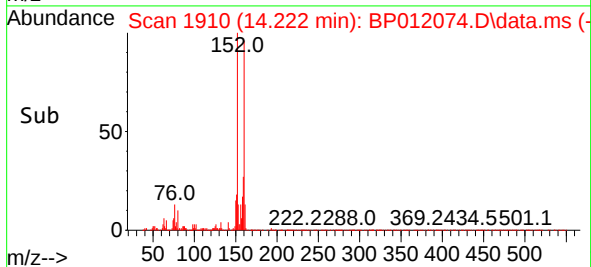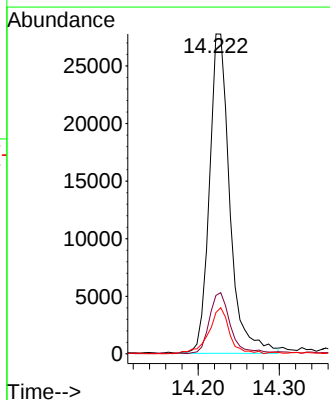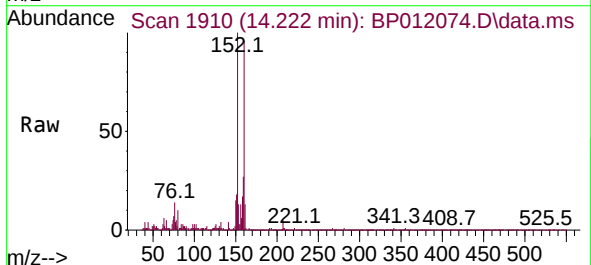

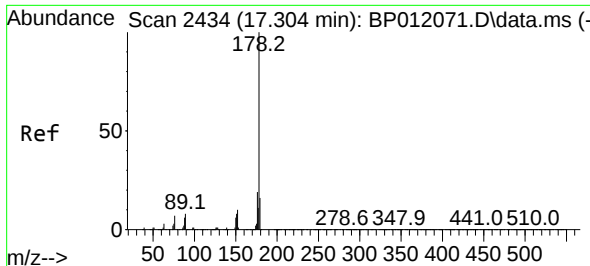

#72
Phenanthrene
Concen: 4.388 ng/ul
RT: 17.304 min Scan# 2434
Delta R.T. 0.000 min
Lab File: BP012074.D
Acq: 12 Oct 2022 11:07




Instrument :
BNA_P
ClientSampleId :
C0BE6

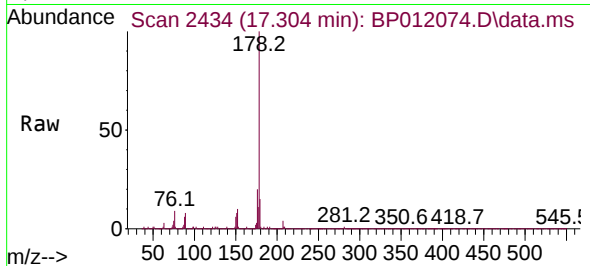

Tgt Ion:178 Resp: 249137
Ion Ratio Lower Upper
178 100
179 15.0 12.2 18.4
176 19.7 15.8 23.6




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

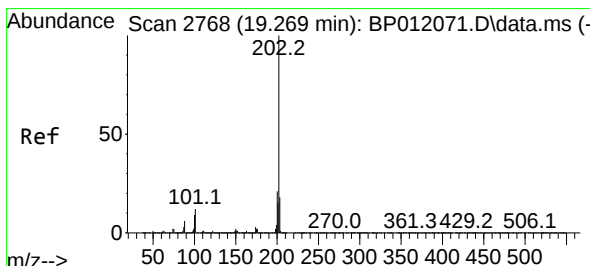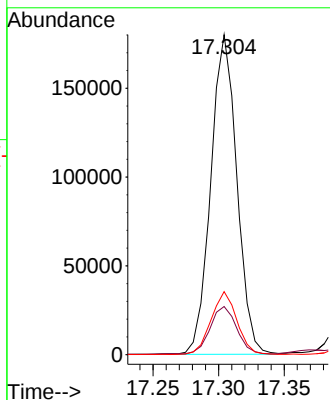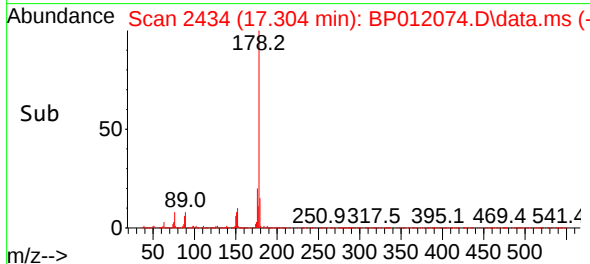

#80
Fluoranthene
Concen: 5.058 ng/ul
RT: 19.275 min Scan# 2769
Delta R.T. 0.006 min
Lab File: BP012074.D
Acq: 12 Oct 2022 11:07

Tgt Ion:202 Resp: 365101
Ion Ratio Lower Upper
202 100
101 11.6 9.0 13.6
100 8.8 7.0 10.6

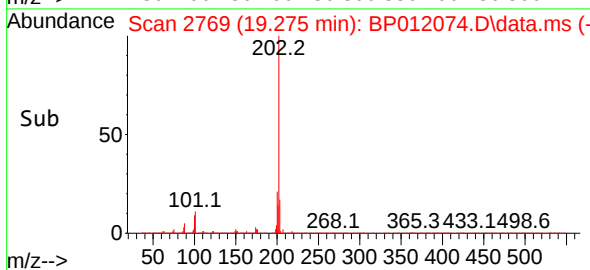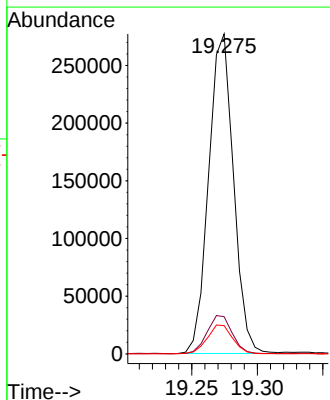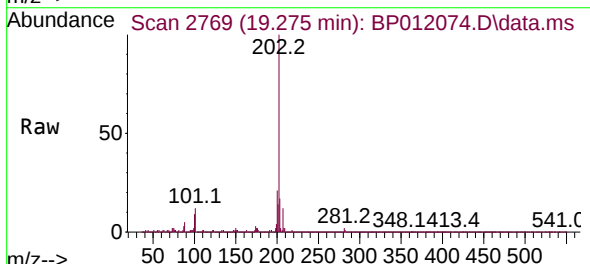

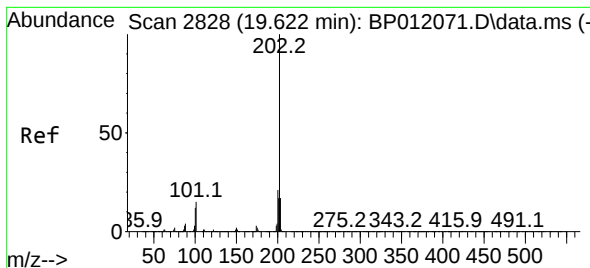

#82

Pyrene

Concen: 4.279 ng/ul

RT: 19.628 min Scan# 2828

Delta R.T. 0.006 min

Lab File: BP012074.D

Acq: 12 Oct 2022 11:07

Instrument :

BNA_P

ClientSampleId :





C0BE6

Tgt Ion:	202	Resp:	326875
Ion Ratio	Lower	Upper	
202	100		
101	13.2	10.4	15.6
100	10.8	8.5	12.7

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

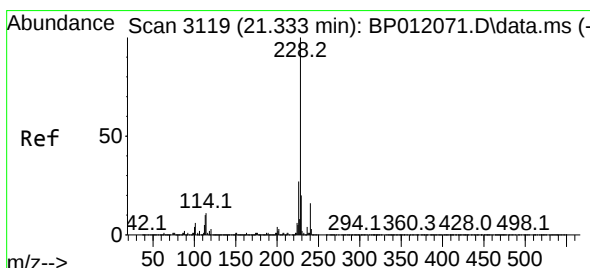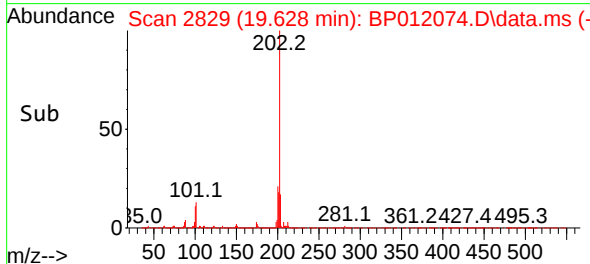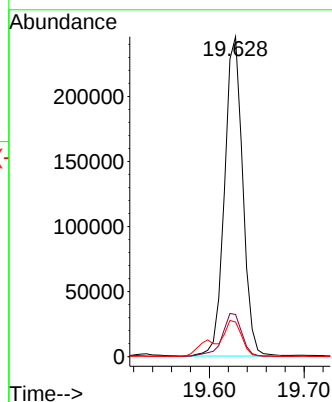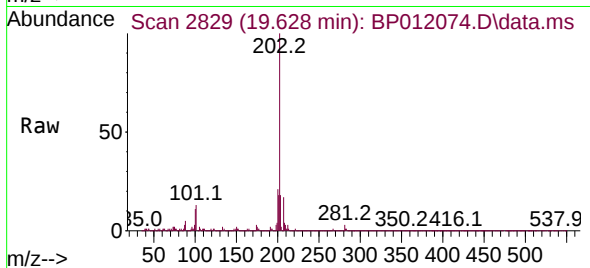

#85

Benzo(a)anthracene

Concen: 1.894 ng/ul




RT: 21.333 min Scan# 3119


Delta R.T. 0.000 min

Lab File: BP012074.D

Acq: 12 Oct 2022 11:07


Tgt Ion:	228	Resp:	137071
Ion Ratio	Lower	Upper	
228	100		
229	21.4	15.7	23.5
226	29.4	21.9	32.9

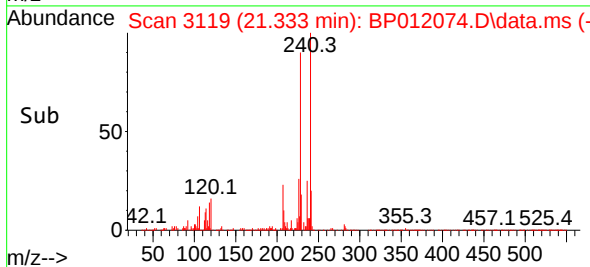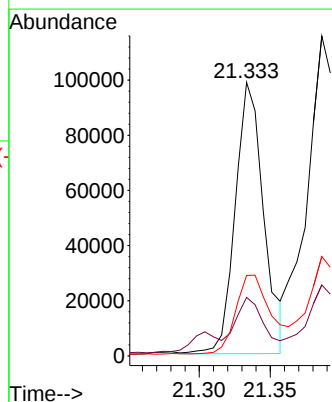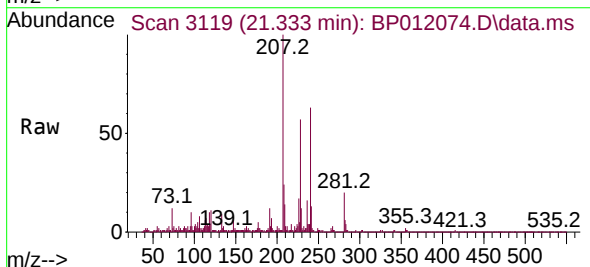

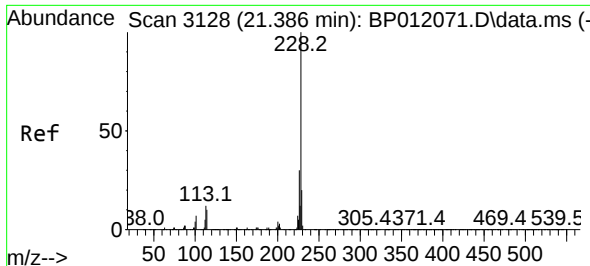

#87
Chrysene
Concen: 2.490 ng/ul
RT: 21.386 min Scan# 3128
Delta R.T. 0.000 min
Lab File: BP012074.D
Acq: 12 Oct 2022 11:07




Instrument :
BNA_P
ClientSampleId :
C0BE6

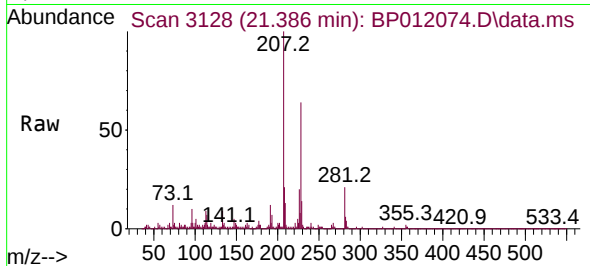


Tgt Ion:228 Resp: 173476
Ion Ratio Lower Upper
228 100
226 31.1 24.0 36.0
229 22.2 15.5 23.3

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

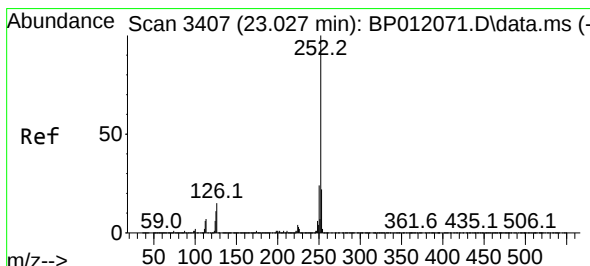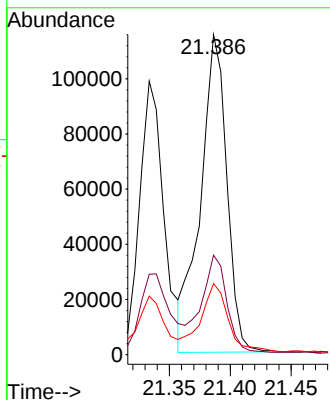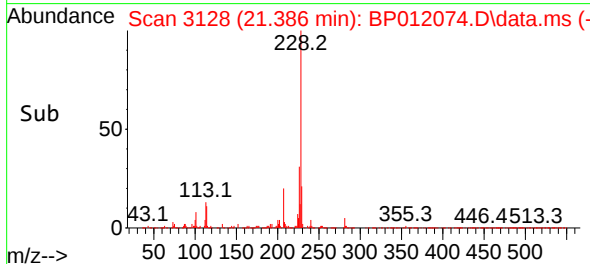


#90
Benzo(b)fluoranthene
Concen: 2.931 ng/ul
RT: 23.033 min Scan# 3408
Delta R.T. 0.006 min
Lab File: BP012074.D
Acq: 12 Oct 2022 11:07

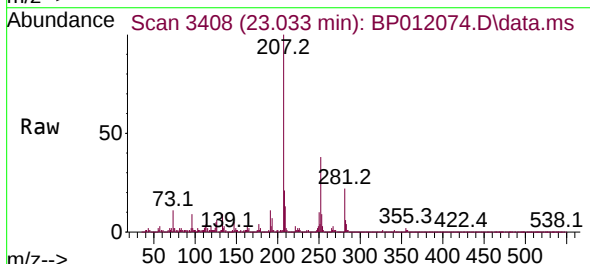


Tgt Ion:252 Resp: 234277
Ion Ratio Lower Upper
252 100
253 24.0 17.6 26.4
125 14.2 7.8 11.8#

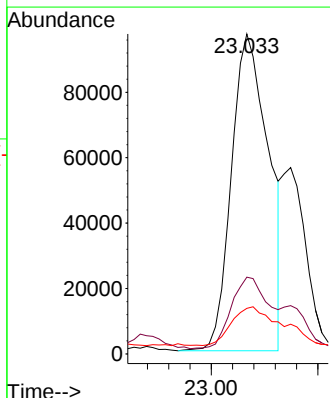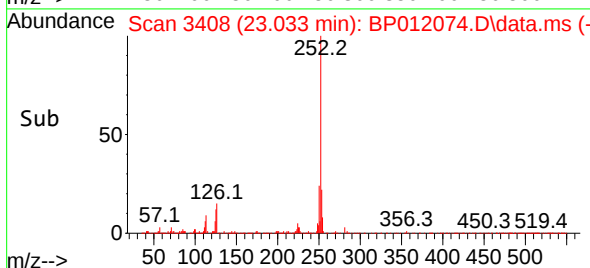

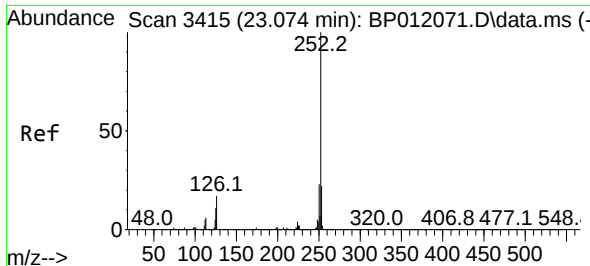

#91
Benzo(k)fluoranthene
Concen: 1.119 ng/ul m
RT: 23.074 min Scan# 3415
Delta R.T. 0.000 min
Lab File: BP012074.D
Acq: 12 Oct 2022 11:07




Instrument :
BNA_P
ClientSampleId :
C0BE6

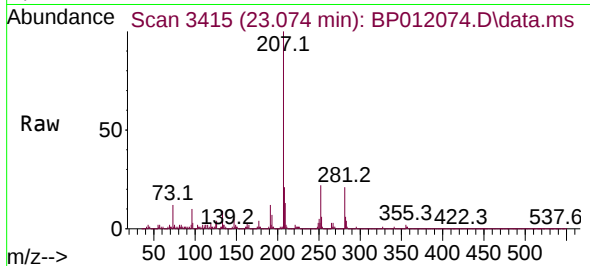

Tgt Ion:252 Resp: 87984
Ion Ratio Lower Upper
252 100
253 25.9 17.6 26.4
125 15.9 8.2 12.2




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

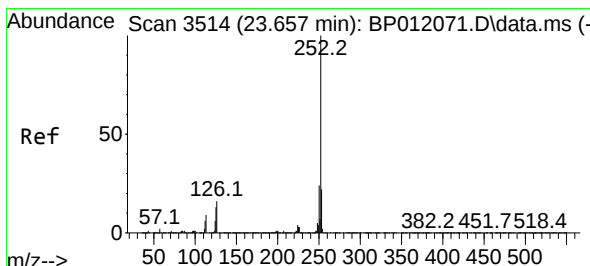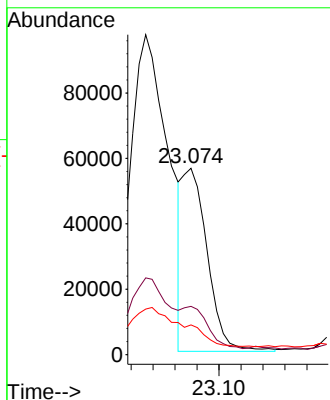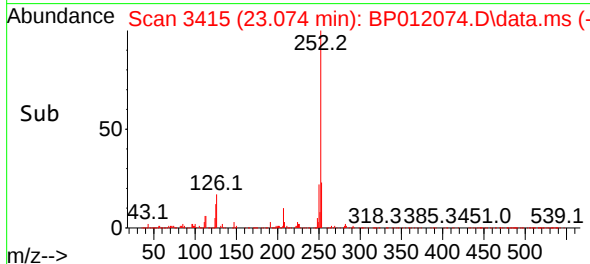

#93
Benzo(a)pyrene
Concen: 2.077 ng/ul
RT: 23.663 min Scan# 3515
Delta R.T. 0.006 min
Lab File: BP012074.D
Acq: 12 Oct 2022 11:07

Tgt Ion:252 Resp: 148092
Ion Ratio Lower Upper
252 100
253 25.4 17.6 26.4
125 15.5 8.9 13.3

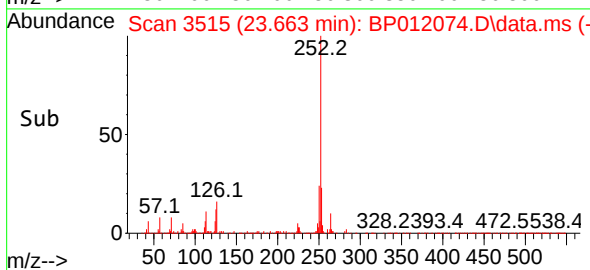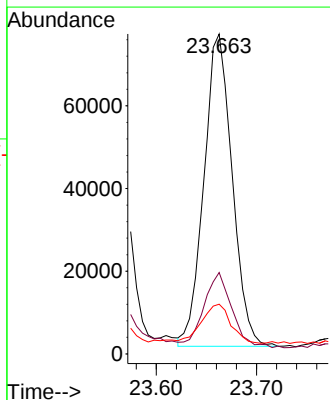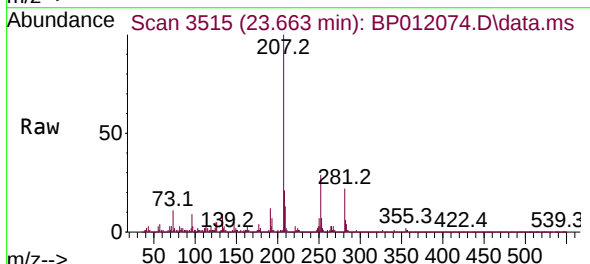

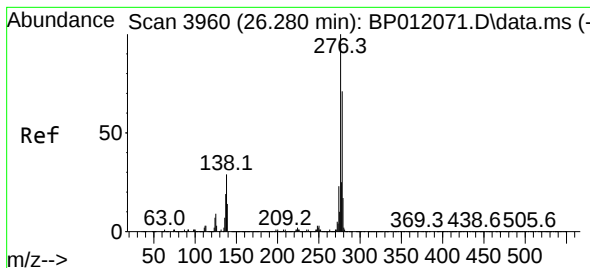

#94

Indeno(1,2,3-cd)pyrene

Concen: 1.364 ng/ul

RT: 26.280 min Scan# 3960

Delta R.T. 0.000 min

Lab File: BP012074.D

Acq: 12 Oct 2022 11:07

Instrument :

BNA_P

ClientSampleId :





C0BE6

Tgt Ion:	276	Resp:	12303
Ion Ratio	Lower	Upper	
276	100		
138	24.0	19.1	28.7
277	24.5	19.9	29.9

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

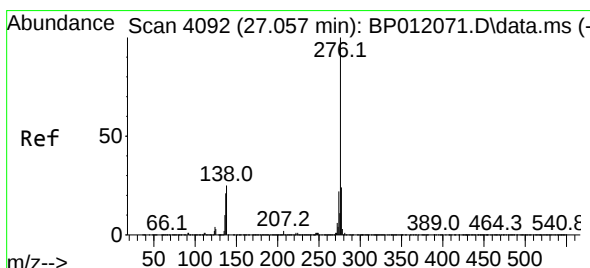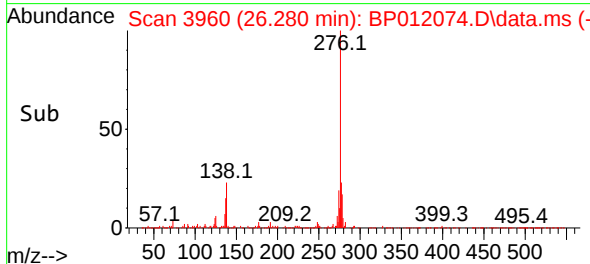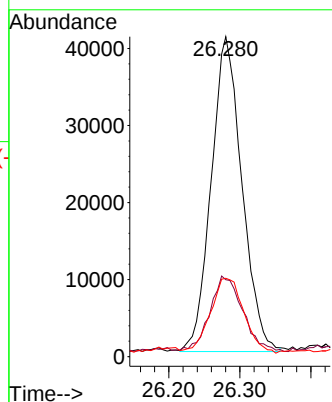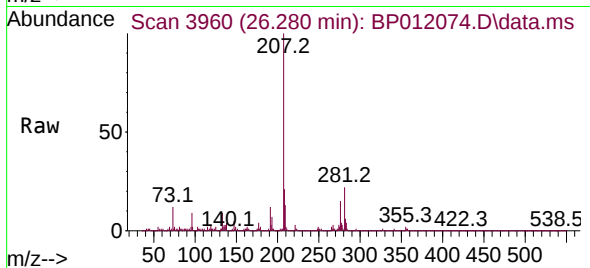

#96

Benzo(g,h,i)perylene

Concen: 1.410 ng/ul

RT: 27.062 min Scan# 4093

Delta R.T. 0.006 min

Lab File: BP012074.D

Acq: 12 Oct 2022 11:07

Tgt Ion:	276	Resp:	114598
Ion Ratio	Lower	Upper	
276	100		
138	26.7	16.5	24.7#
277	24.5	19.0	28.4

