

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012093.D
 Acq On : 12 Oct 2022 22:41
 Operator : CG/JU
 Sample : N4976-11
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8Y7

Quant Time: Oct 13 00:34:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 12 23:03:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	281014	20.000	ng/u1	0.00
20) Naphthalene-d8	10.657	136	1112396	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.498	164	646351	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.257	188	1365259	20.000	ng/u1	0.00
79) Chrysene-d12	21.351	240	1418834	20.000	ng/u1	0.00
88) Perylene-d12	23.768	264	1551342	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	26203	3.676	ng/uL	0.00
4) Pyridine-d5	3.704	84	291011	15.353	ng/u1	0.00
7) Phenol-d5	7.022	99	166802	7.380	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	332877	25.948	ng/u1	0.00
11) 2-Chlorophenol-d4	7.381	132	426137	23.754	ng/u1	0.00
15) 4-Methylphenol-d8	8.569	113	284207	16.372	ng/u1	0.00
21) Nitrobenzene-d5	9.022	128	235358	29.958	ng/u1	0.00
24) 2-Nitrophenol-d4	9.739	143	248965	31.253	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	435969	28.239	ng/u1	0.00
31) 4-Chloroaniline-d4	10.804	131	485204	21.327	ng/u1	0.00
46) Dimethylphthalate-d6	13.916	166	1277912	31.218	ng/u1	0.00
49) Acenaphthylene-d8	14.192	160	1479465	29.228	ng/u1	0.00
54) 4-Nitrophenol-d4	14.727	143	48846	6.078	ng/u1	0.02
60) Fluorene-d10	15.498	176	1119750	30.234	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.621	200	102978	14.285	ng/u1	0.00
73) Anthracene-d10	17.357	188	1852122	31.241	ng/u1	0.00
81) Pyrene-d10	19.592	212	2162516	29.751	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.609	264	2301949	30.524	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.310	88	216192	28.824	ng/uL	98
52) Acenaphthene	14.563	153	251592	6.171	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012093.D
Acq On : 12 Oct 2022 22:41
Operator : CG/JU
Sample : N4976-11
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8Y7

Quant Time: Oct 13 00:34:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 12 23:03:21 2022
Response via : Initial Calibration




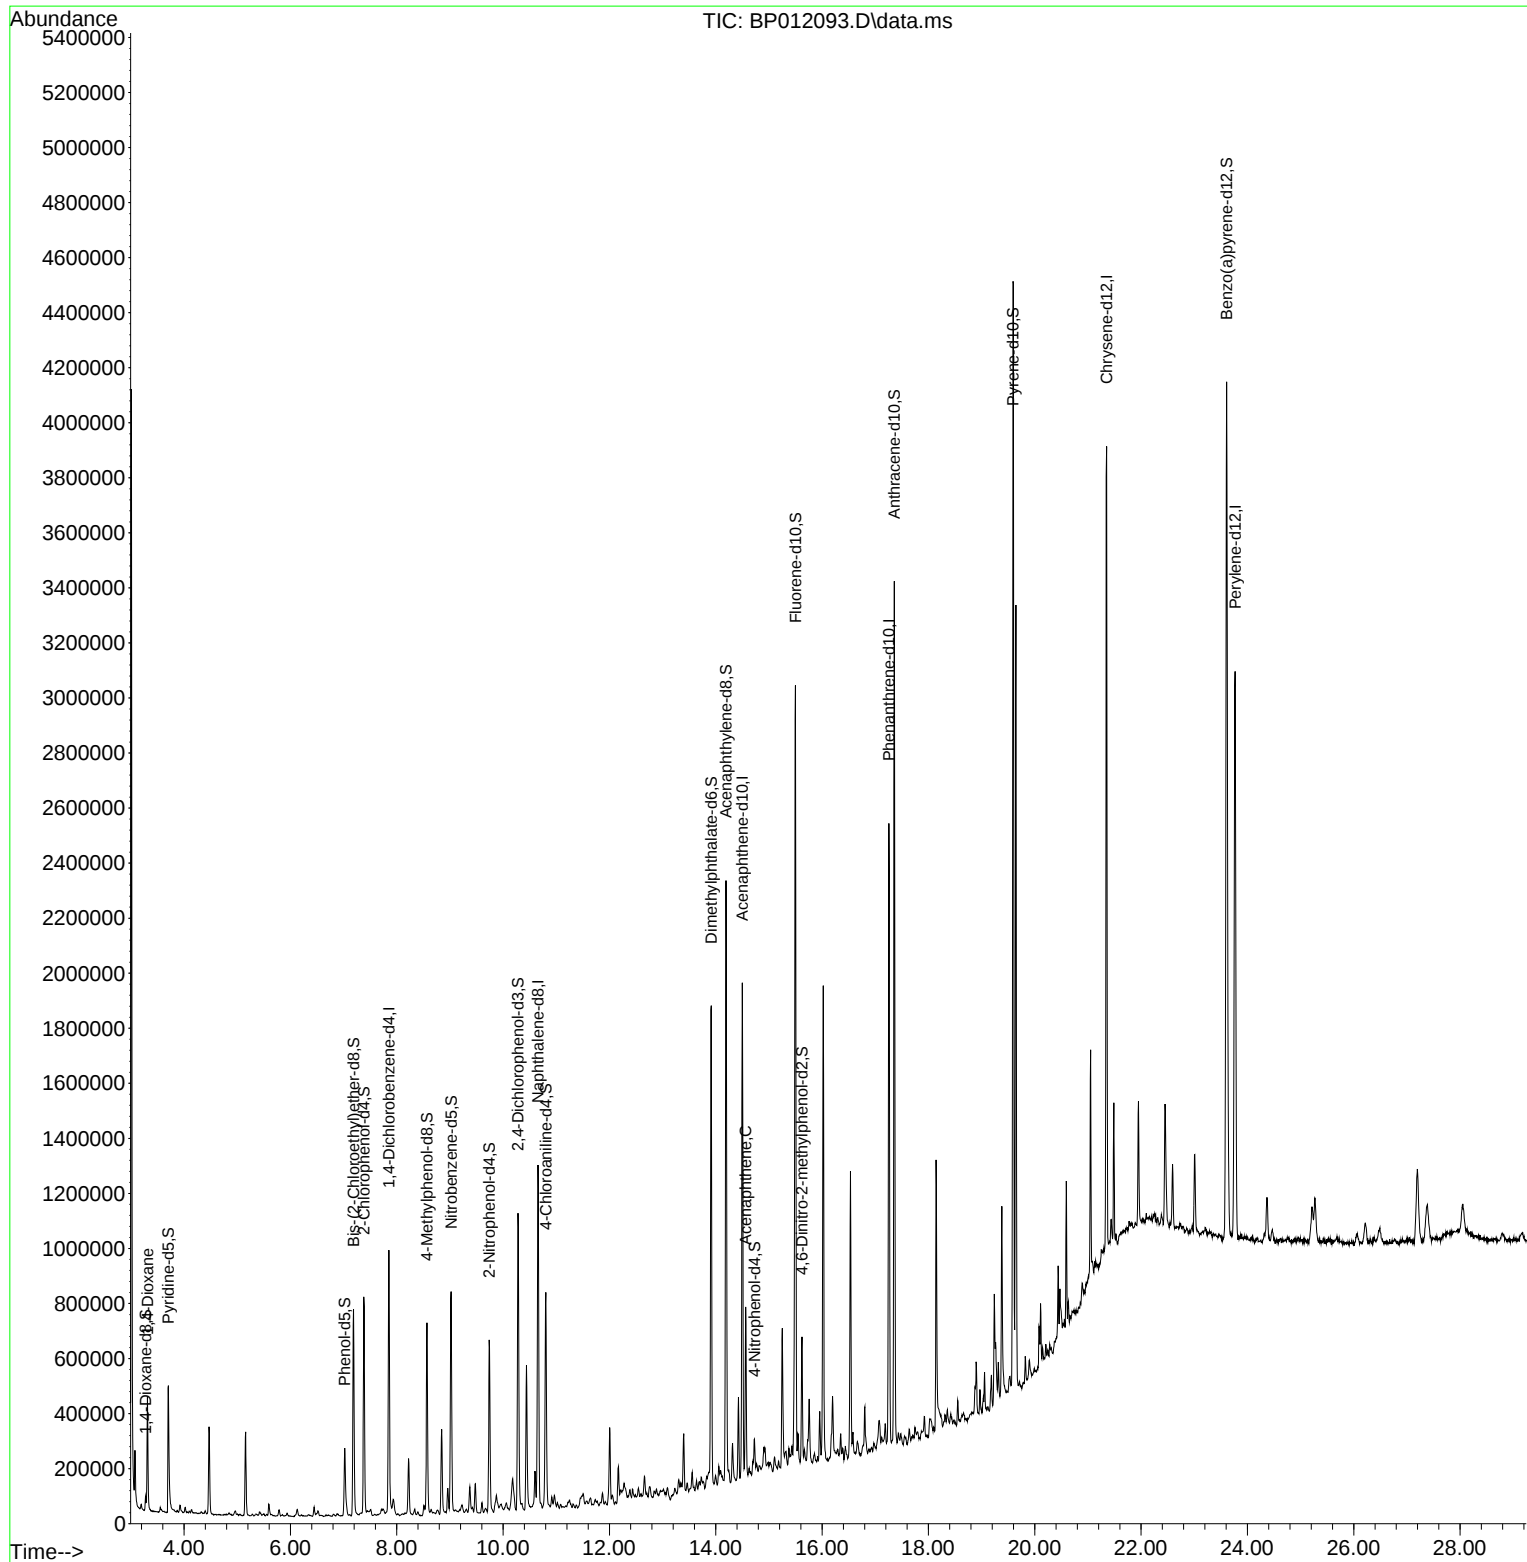


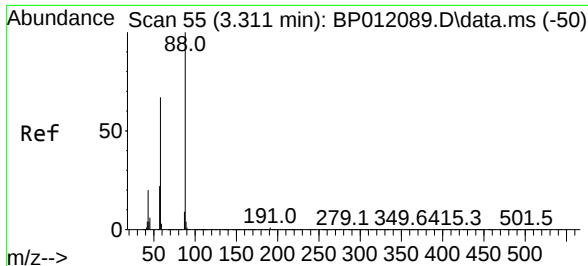

#2
1,4-Dioxane
Concen: 28.824 ng/uL
RT: 3.310 min Scan# 51
Delta R.T. -0.000 min
Lab File: BP012093.D
Acq: 12 Oct 2022 22:41

Instrument :
BNA_P
ClientSampleId :
CB8Y7

Tgt Ion: 88 Resp: 216192
Ion Ratio Lower Upper
88 100
43 20.1 16.6 25.0
58 64.4 52.6 79.0

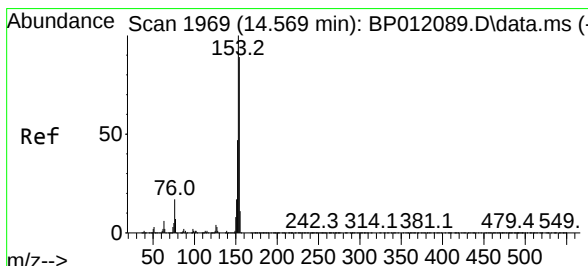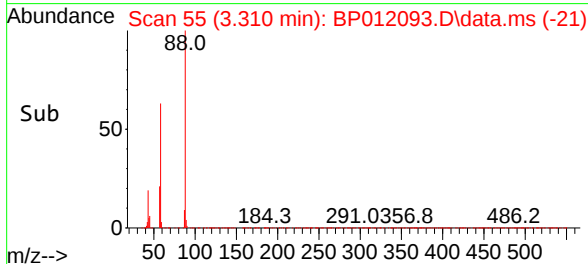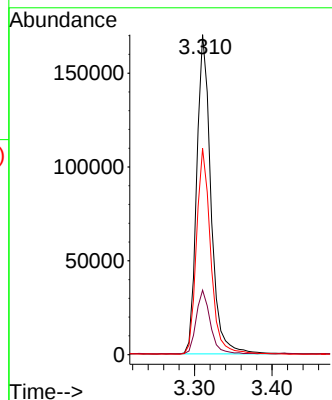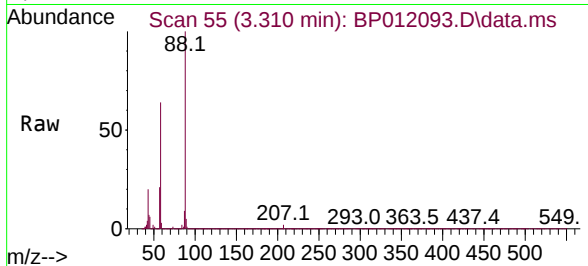

#52
Acenaphthene
Concen: 6.171 ng/uL
RT: 14.563 min Scan# 1968
Delta R.T. -0.000 min
Lab File: BP012093.D
Acq: 12 Oct 2022 22:41

Tgt Ion:153 Resp: 251592
Ion Ratio Lower Upper
153 100
152 47.1 38.2 57.2
154 90.1 70.6 105.8

