

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012041.D
 Acq On : 11 Oct 2022 15:38
 Operator : CG/JU
 Sample : PB148209BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK209

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012041.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	45	50	59	rVB	54838	74465	1.80%	0.166%
2	3.705	119	122	145	rBV	575533	931640	22.58%	2.081%
3	4.022	172	176	183	rVB	14278	20955	0.51%	0.047%
4	4.258	212	216	220	rVB7	3457	5464	0.13%	0.012%
5	7.028	679	687	701	rBV	692599	1171146	28.38%	2.616%
6	7.193	708	715	728	rBV	636457	1013735	24.56%	2.264%
7	7.387	741	748	762	rBV	747987	1227944	29.76%	2.742%
8	7.858	819	828	841	rBV	734236	1219788	29.56%	2.724%
9	8.575	943	950	968	rBV	857834	1463787	35.47%	3.269%
10	9.028	1020	1027	1043	rBV	665174	1105998	26.80%	2.470%
11	9.752	1142	1150	1168	rBV	490426	855923	20.74%	1.912%
12	10.287	1233	1241	1262	rBV	794470	1418439	34.37%	3.168%
13	10.669	1297	1306	1317	rBV	1001092	1765951	42.79%	3.944%
14	10.810	1323	1330	1351	rBV	805530	1509191	36.57%	3.371%
15	12.269	1572	1578	1587	rBV2	10600	28485	0.69%	0.064%
16	13.481	1780	1784	1790	rVB8	3176	5803	0.14%	0.013%
17	13.922	1852	1859	1874	rBV	1343056	1941500	47.05%	4.336%
18	14.198	1898	1906	1920	rBV	1633445	2532329	61.36%	5.656%
19	14.510	1950	1959	1967	rBV	1455907	2192992	53.14%	4.898%
20	14.716	1987	1994	2015	rBV	429751	831676	20.15%	1.857%
21	15.504	2120	2128	2139	rBV	2204564	3198047	77.49%	7.142%
22	15.628	2143	2149	2164	rVV	472680	719968	17.45%	1.608%
23	15.745	2165	2169	2176	rVB4	10685	20695	0.50%	0.046%
24	17.051	2389	2391	2398	rBV7	4186	4788	0.12%	0.011%
25	17.269	2420	2428	2438	rBV	1667976	2474408	59.96%	5.526%
26	17.363	2438	2444	2462	rVV	2250910	3350056	81.18%	7.482%
27	18.163	2575	2580	2586	rBV9	13227	30216	0.73%	0.067%
28	19.181	2749	2753	2758	rBV3	27327	39124	0.95%	0.087%
29	19.251	2762	2765	2770	rVV2	22157	31871	0.77%	0.071%
30	19.598	2819	2824	2836	rBV	2746792	3860005	93.53%	8.621%
31	21.351	3117	3122	3130	rBV	2134042	2725130	66.03%	6.086%
32	23.616	3500	3507	3519	rVB2	2022182	4126823	100.00%	9.217%
33	23.774	3528	3534	3545	rVB2	1400785	2877160	69.72%	6.426%




Sum of corrected areas: 44775502

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012041.D
Acq On : 11 Oct 2022 15:38
Operator : CG/JU
Sample : PB148209BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK209

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

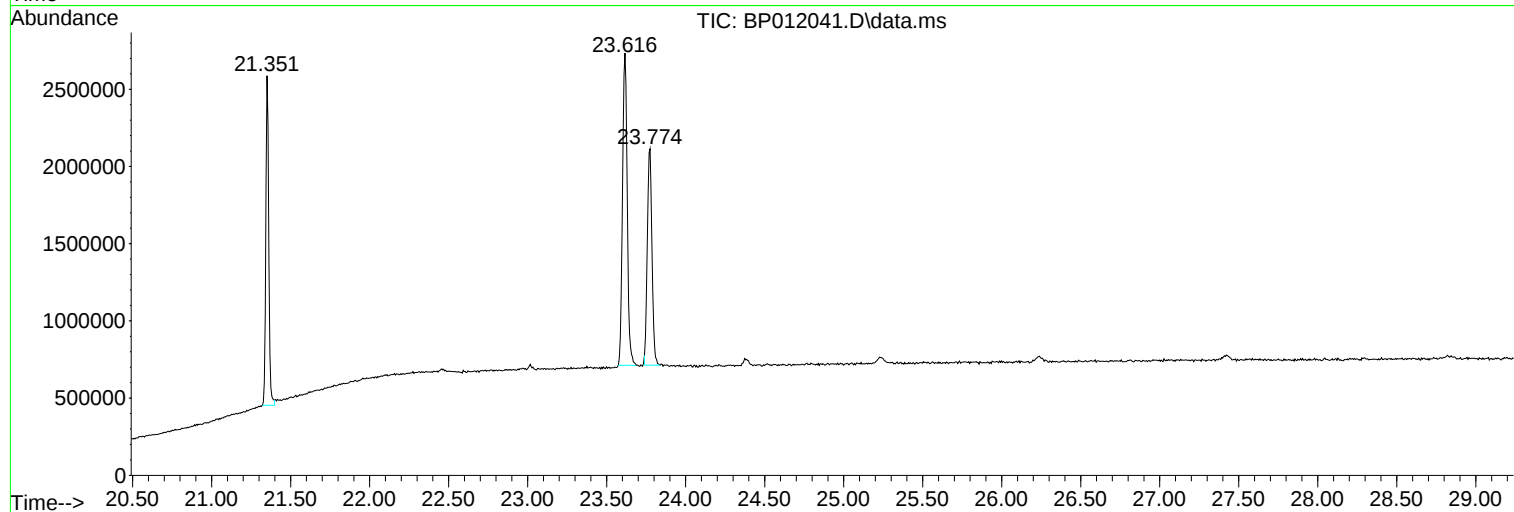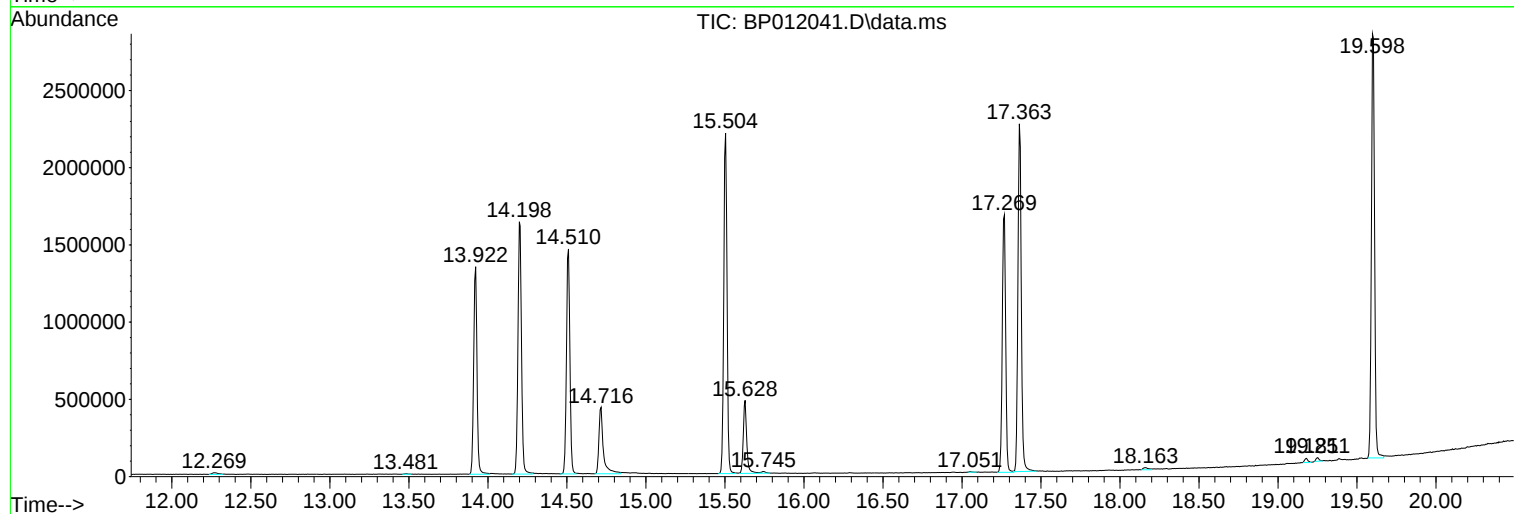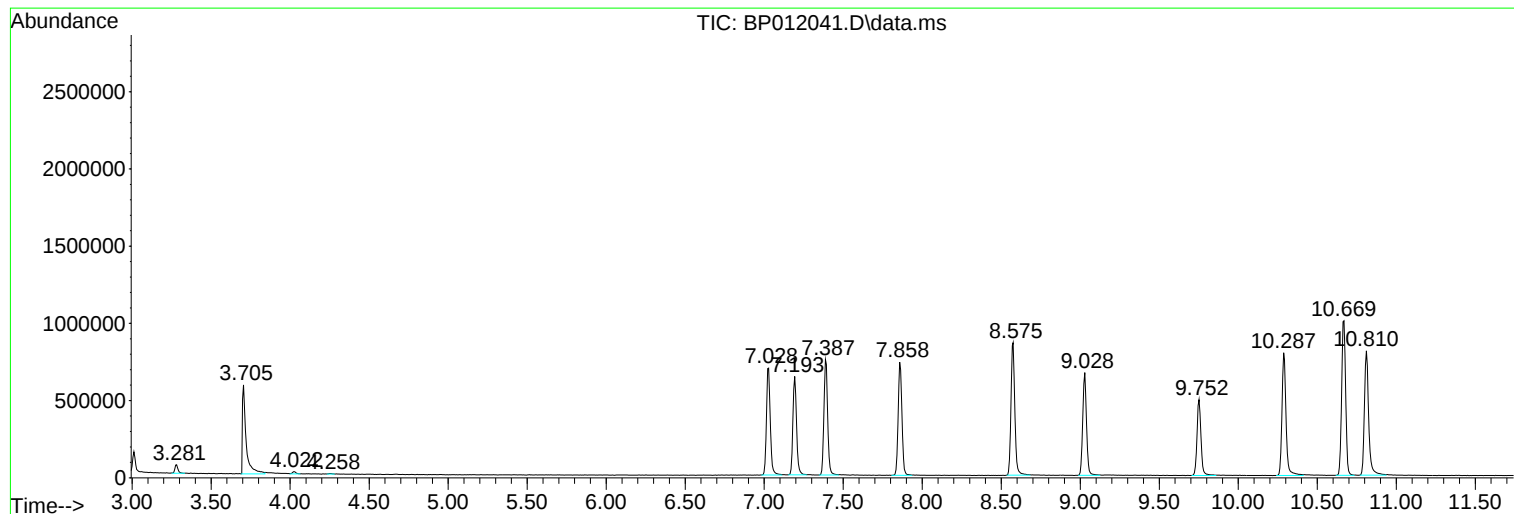

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012041.D
Acq On : 11 Oct 2022 15:38
Operator : CG/JU
Sample : PB148209BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK209

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012041.D
Acq On : 11 Oct 2022 15:38
Operator : CG/JU
Sample : PB148209BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK209

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc