

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012044.D
 Acq On : 11 Oct 2022 17:22
 Operator : CG/JU
 Sample : PB148209BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK209

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012044.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	45	49	59	rVB	57529	78165	1.83%	0.169%
2	3.705	119	122	148	rBV	609845	981466	23.01%	2.122%
3	4.023	172	176	182	rVB	15506	21241	0.50%	0.046%
4	4.252	213	215	221	rVB7	4663	6302	0.15%	0.014%
5	7.022	680	686	704	rBV	744058	1236981	29.01%	2.674%
6	7.193	708	715	733	rVB	669692	1076888	25.25%	2.328%
7	7.387	741	748	764	rVB	804074	1292674	30.31%	2.795%
8	7.858	821	828	844	rVB	790226	1273093	29.85%	2.752%
9	8.569	942	949	966	rBV	906479	1555005	36.46%	3.362%
10	9.028	1019	1027	1040	rBV	673538	1165629	27.33%	2.520%
11	9.752	1142	1150	1164	rBV	512259	897348	21.04%	1.940%
12	10.287	1234	1241	1265	rBV	832975	1497443	35.11%	3.237%
13	10.663	1297	1305	1321	rVB	1085437	1856467	43.53%	4.013%
14	10.810	1322	1330	1353	rBV	845388	1597467	37.46%	3.453%
15	12.269	1572	1578	1584	rBV2	11135	26789	0.63%	0.058%
16	13.487	1781	1785	1790	rVB7	3582	5704	0.13%	0.012%
17	13.916	1852	1858	1870	rBV	1398922	2000359	46.91%	4.324%
18	14.198	1899	1906	1923	rBV	1779229	2625636	61.57%	5.676%
19	14.504	1951	1958	1973	rBV	1528652	2279905	53.46%	4.929%
20	14.710	1986	1993	2019	rBV	455713	886200	20.78%	1.916%
21	15.498	2121	2127	2142	rBV	2240196	3316111	77.76%	7.169%
22	15.622	2142	2148	2164	rVV	488265	741429	17.39%	1.603%
23	15.740	2164	2168	2177	rVB3	11462	22294	0.52%	0.048%
24	17.057	2388	2392	2398	rBV7	4604	8655	0.20%	0.019%
25	17.263	2421	2427	2437	rBV	1808323	2517546	59.03%	5.443%
26	17.363	2438	2444	2463	rVV	2445828	3401845	79.77%	7.354%
27	18.157	2575	2579	2585	rBV4	15196	26141	0.61%	0.057%
28	19.175	2749	2752	2757	rVB3	24472	33916	0.80%	0.073%
29	19.245	2761	2764	2768	rBV3	24411	38743	0.91%	0.084%
30	19.598	2819	2824	2834	rBV	2980960	3857040	90.44%	8.338%
31	21.351	3117	3122	3131	rBV	2164010	2748325	64.44%	5.941%
32	23.610	3500	3506	3521	rVB2	2107489	4264663	100.00%	9.219%
33	23.769	3527	3533	3544	rVB	1495202	2919661	68.46%	6.312%




Sum of corrected areas: 46257131

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012044.D
Acq On : 11 Oct 2022 17:22
Operator : CG/JU
Sample : PB148209BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK209

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

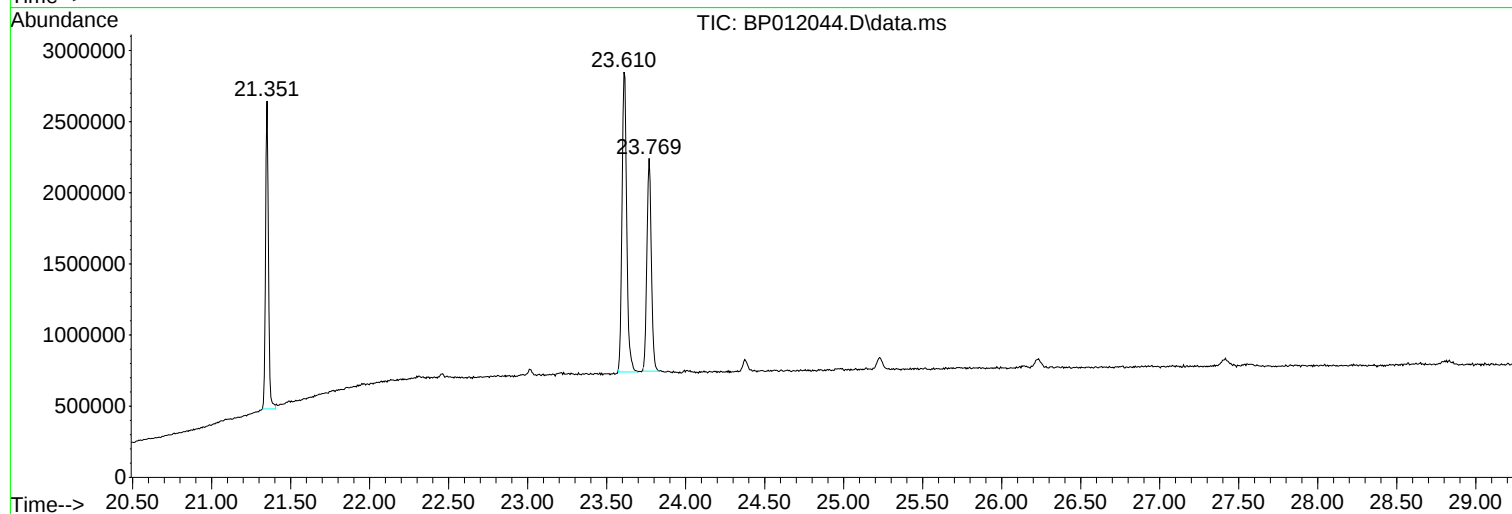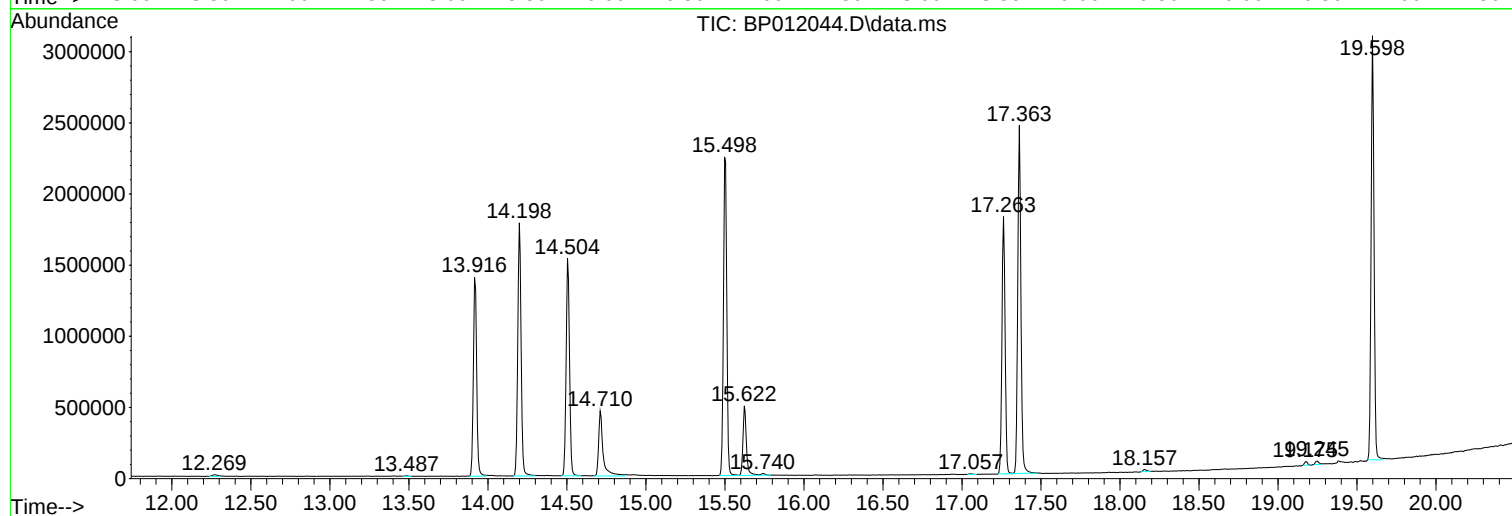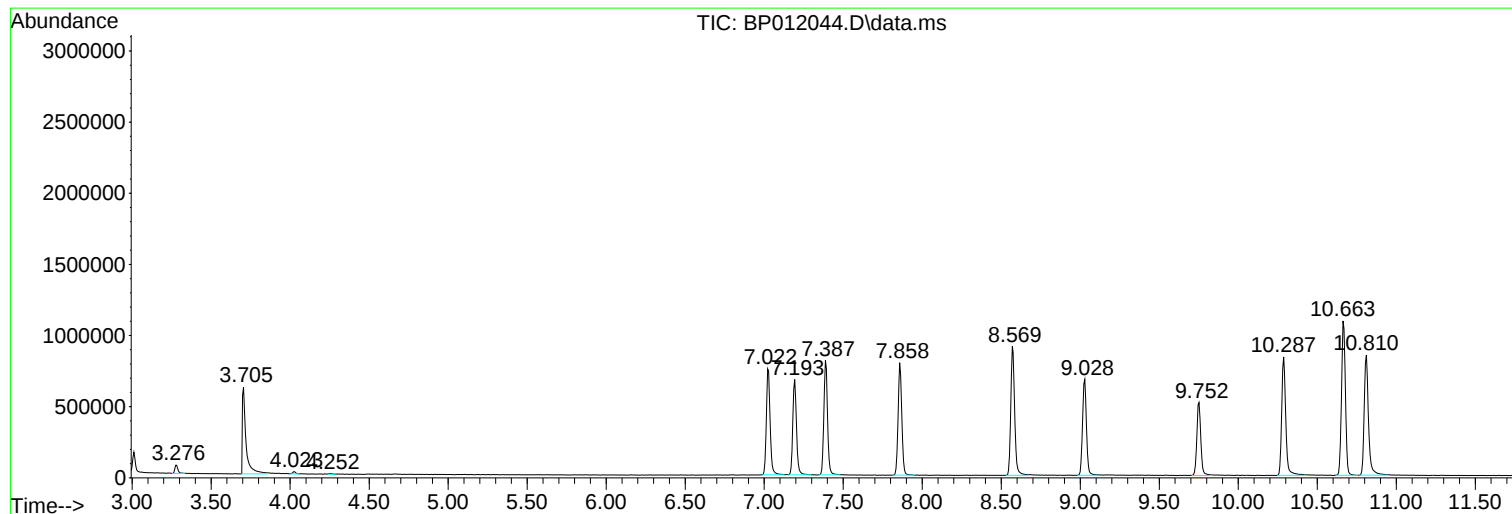

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012044.D
Acq On : 11 Oct 2022 17:22
Operator : CG/JU
Sample : PB148209BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK209

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012044.D
Acq On : 11 Oct 2022 17:22
Operator : CG/JU
Sample : PB148209BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK209

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc