

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012048.D
 Acq On : 11 Oct 2022 19:41
 Operator : CG/JU
 Sample : N4950-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8T0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012048.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	46	50	59	rVB	28706	40964	1.07%	0.119%
2	3.710	116	123	125	rBV2	9747	14618	0.38%	0.042%
3	3.734	125	127	135	rVV	36467	74704	1.96%	0.217%
4	3.804	135	139	146	rVB	52553	75008	1.97%	0.217%
5	3.928	156	160	165	rVB	35010	50377	1.32%	0.146%
6	4.022	172	176	182	rBV	44386	59652	1.56%	0.173%
7	4.399	238	240	245	rVB5	6803	8546	0.22%	0.025%
8	4.587	268	272	280	rVB5	9027	14009	0.37%	0.041%
9	4.963	328	336	343	rBV2	56568	107887	2.83%	0.313%
10	5.057	349	352	358	rBV5	5795	9030	0.24%	0.026%
11	5.857	482	488	493	rBV9	5813	11123	0.29%	0.032%
12	6.716	629	634	638	rBV5	5663	10087	0.26%	0.029%
13	6.934	668	671	676	rBV4	5047	8529	0.22%	0.025%
14	7.028	676	687	702	rVV	334049	618287	16.22%	1.792%
15	7.192	706	715	728	rVV	311779	522906	13.71%	1.516%
16	7.387	742	748	759	rBV	381981	615003	16.13%	1.783%
17	7.475	759	763	765	rVV3	9282	15083	0.40%	0.044%
18	7.498	765	767	776	rVB2	9498	15151	0.40%	0.044%
19	7.857	821	828	839	rBV	687508	1128586	29.60%	3.271%
20	8.492	933	936	941	rBV6	4410	7778	0.20%	0.023%
21	8.575	943	950	965	rVV	276064	513260	13.46%	1.488%
22	8.692	965	970	979	rVB	20942	41120	1.08%	0.119%
23	8.963	1010	1016	1019	rBV8	3800	6176	0.16%	0.018%
24	9.028	1019	1027	1043	rBV	297102	541735	14.21%	1.570%
25	9.163	1045	1050	1052	rBV6	3369	5725	0.15%	0.017%
26	9.428	1089	1095	1100	rBV2	7240	13013	0.34%	0.038%
27	9.751	1142	1150	1162	rBV	216170	392712	10.30%	1.138%
28	10.286	1233	1241	1261	rBV	384396	707552	18.56%	2.051%
29	10.475	1266	1273	1279	rBV6	9114	23843	0.63%	0.069%
30	10.663	1297	1305	1312	rBV	932529	1591909	41.75%	4.614%
31	10.810	1324	1330	1351	rBV	223004	468934	12.30%	1.359%
32	12.092	1543	1548	1552	rBV8	3593	6026	0.16%	0.017%
33	12.251	1571	1575	1585	rVB2	7262	14708	0.39%	0.043%
34	12.333	1585	1589	1597	rBV3	6524	13014	0.34%	0.038%
35	13.327	1754	1758	1764	rBV6	5664	9455	0.25%	0.027%
36	13.404	1766	1771	1776	rVB6	4098	7255	0.19%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012048.D
 Acq On : 11 Oct 2022 19:41
 Operator : CG/JU
 Sample : N4950-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8T0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

37	13.675	1812	1817	1818	rBV5	4004	5898	0.15%	0.017%
38	13.827	1837	1843	1848	rBV10	7151	12346	0.32%	0.036%
39	13.916	1852	1858	1874	rVB	730484	1039171	27.25%	3.012%
40	14.198	1899	1906	1924	rBV	844651	1290967	33.86%	3.742%
41	14.398	1938	1940	1945	rVB6	5134	6266	0.16%	0.018%
42	14.504	1950	1958	1965	rVV	1347319	1988442	52.15%	5.764%
43	14.569	1966	1969	1978	rVB2	14927	26786	0.70%	0.078%
44	14.716	1988	1994	2008	rBV	117946	270370	7.09%	0.784%
45	14.904	2022	2026	2029	rBV2	9811	18149	0.48%	0.053%
46	14.933	2029	2031	2036	rVB4	13356	15631	0.41%	0.045%
47	15.292	2085	2092	2096	rBV9	5931	12012	0.32%	0.035%
48	15.498	2121	2127	2134	rBV	1214016	1802911	47.28%	5.226%
49	15.557	2134	2137	2142	rVB	22820	31135	0.82%	0.090%
50	15.621	2143	2148	2156	rBV	137589	217900	5.71%	0.632%
51	15.851	2184	2187	2195	rVB5	8475	13823	0.36%	0.040%
52	15.998	2209	2212	2220	rVB4	7349	13430	0.35%	0.039%
53	16.804	2344	2349	2352	rBV5	13508	23622	0.62%	0.068%
54	17.080	2392	2396	2402	rVB	14541	26405	0.69%	0.077%
55	17.263	2421	2427	2431	rBV	1679617	2336384	61.28%	6.772%
56	17.304	2431	2434	2439	rVV	272692	382545	10.03%	1.109%
57	17.363	2439	2444	2456	rVB	1285866	1911563	50.13%	5.541%
58	18.145	2571	2577	2580	rBV2	77648	150716	3.95%	0.437%
59	18.174	2580	2582	2587	rVB	58822	77888	2.04%	0.226%
60	18.321	2602	2607	2611	rBV2	75774	132578	3.48%	0.384%
61	18.615	2654	2657	2660	rBV	32743	39833	1.04%	0.115%
62	19.015	2722	2725	2731	rBV4	36888	66641	1.75%	0.193%
63	19.274	2764	2769	2775	rVB	888046	1107637	29.05%	3.211%
64	19.598	2819	2824	2827	rBV	2057331	2852402	74.81%	8.268%
65	19.627	2827	2829	2837	rVB	776777	876693	22.99%	2.541%
66	20.109	2908	2911	2917	rVB	133414	174245	4.57%	0.505%
67	20.204	2924	2927	2931	rBV	108815	139529	3.66%	0.404%
68	21.351	3115	3122	3126	rBV2	2431527	3812887	100.00%	11.052%
69	21.386	3126	3128	3136	rVB	516679	584317	15.32%	1.694%
70	23.609	3501	3506	3511	rBV2	1273558	2331223	61.14%	6.757%
71	23.768	3527	3533	3540	rBV2	1487213	2943261	77.19%	8.531%




Sum of corrected areas: 34499371

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012048.D
Acq On : 11 Oct 2022 19:41
Operator : CG/JU
Sample : N4950-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8T0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

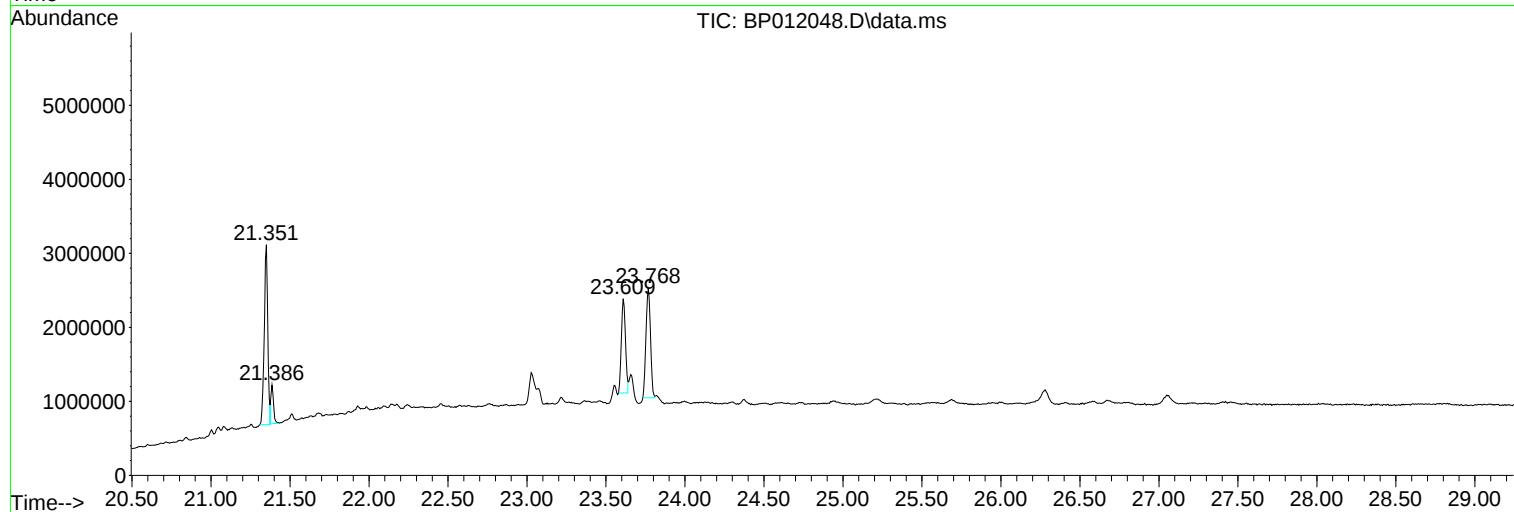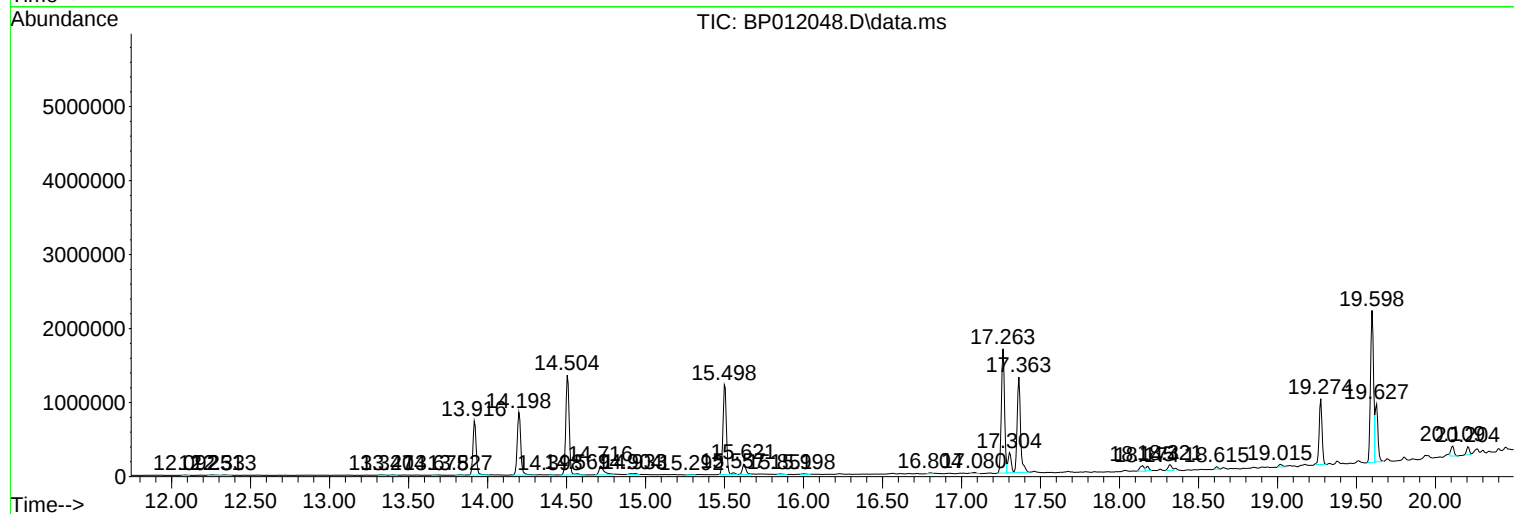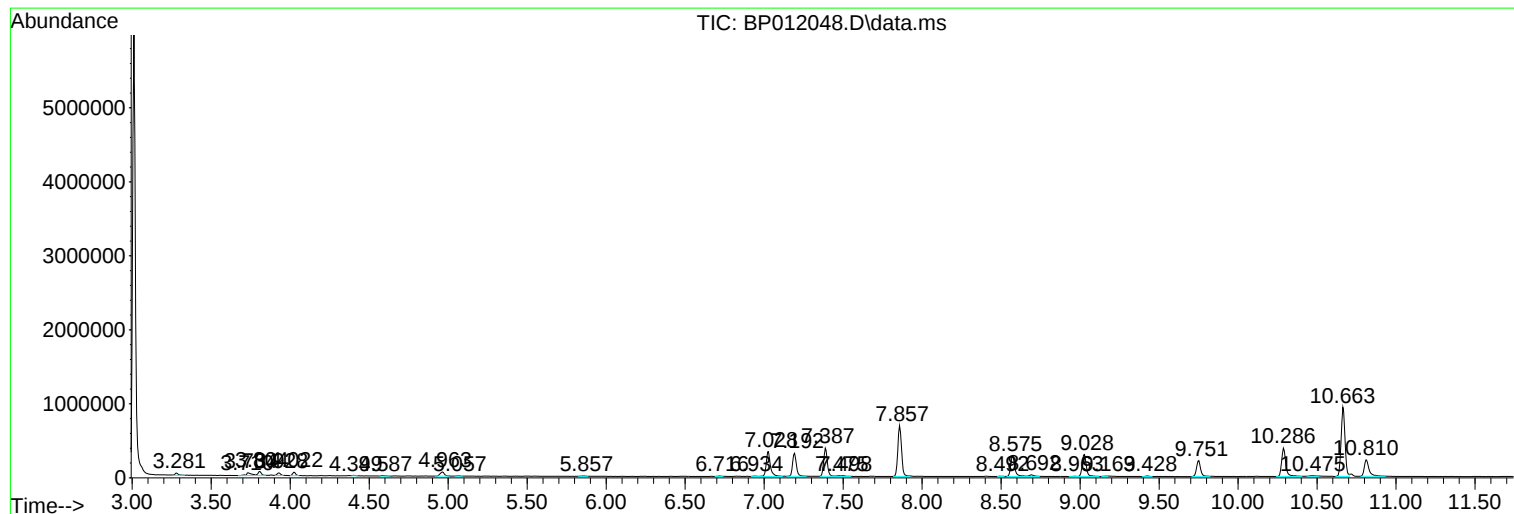

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012048.D
Acq On : 11 Oct 2022 19:41
Operator : CG/JU
Sample : N4950-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8T0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012048.D
Acq On : 11 Oct 2022 19:41
Operator : CG/JU
Sample : N4950-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8T0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
