

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012057.D
 Acq On : 12 Oct 2022 00:52
 Operator : CG/JU
 Sample : N4991-09
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012057.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	45	49	56	rBV	62730	83344	2.03%	0.201%
2	3.575	98	100	105	rBV	6800	10108	0.25%	0.024%
3	3.728	124	126	137	rBV	42135	76051	1.85%	0.183%
4	3.928	155	160	166	rVB	15492	21825	0.53%	0.053%
5	4.022	172	176	182	rVB	21655	27181	0.66%	0.065%
6	4.199	202	206	209	rBV6	3812	5096	0.12%	0.012%
7	4.958	331	335	343	rVB4	5504	11410	0.28%	0.027%
8	5.163	366	370	375	rVB3	5304	8427	0.21%	0.020%
9	7.022	679	686	699	rBV	329064	529129	12.91%	1.275%
10	7.187	708	714	733	rBV	700265	1150799	28.07%	2.773%
11	7.387	741	748	760	rBV	610095	998509	24.35%	2.406%
12	7.740	803	808	809	rBV5	3556	4224	0.10%	0.010%
13	7.857	819	828	836	rBV	770477	1274373	31.08%	3.071%
14	8.204	881	887	890	rBV7	2845	4277	0.10%	0.010%
15	8.569	941	949	964	rBV	297113	519154	12.66%	1.251%
16	9.022	1019	1026	1047	rBV	731752	1242188	30.30%	2.993%
17	9.434	1089	1096	1107	rVB3	23149	42401	1.03%	0.102%
18	9.746	1142	1149	1161	rBV	529876	899190	21.93%	2.167%
19	10.287	1233	1241	1261	rBV	675356	1226988	29.93%	2.956%
20	10.522	1275	1281	1288	rVB	3834	9429	0.23%	0.023%
21	10.663	1297	1305	1320	rBV	1036609	1780049	43.41%	4.289%
22	10.810	1321	1330	1349	rBV	356462	723315	17.64%	1.743%
23	12.263	1569	1577	1583	rBV3	14891	31858	0.78%	0.077%
24	12.581	1622	1631	1633	rBV10	3977	8882	0.22%	0.021%
25	12.857	1676	1678	1687	rVB9	3659	8592	0.21%	0.021%
26	13.110	1715	1721	1726	rVB10	3749	5811	0.14%	0.014%
27	13.234	1739	1742	1747	rVB7	2717	4436	0.11%	0.011%
28	13.475	1779	1783	1789	rVB8	4095	7660	0.19%	0.018%
29	13.916	1850	1858	1872	rBV	1402607	1942706	47.38%	4.681%
30	14.198	1899	1906	1918	rBV	1803475	2609136	63.64%	6.287%
31	14.504	1951	1958	1967	rBV	1461594	2179354	53.15%	5.251%
32	14.728	1990	1996	2009	rBV	29874	91526	2.23%	0.221%
33	15.345	2096	2101	2105	rVB7	3320	5886	0.14%	0.014%
34	15.498	2119	2127	2140	rBV	2352512	3372705	82.26%	8.126%
35	15.622	2142	2148	2160	rVV	268821	402465	9.82%	0.970%
36	15.739	2165	2168	2174	rVB3	10961	18864	0.46%	0.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012057.D
 Acq On : 12 Oct 2022 00:52
 Operator : CG/JU
 Sample : N4991-09
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

37	16.798	2344	2348	2353	rBV4	9286	15345	0.37%	0.037%
38	17.004	2382	2383	2387	rBV4	2783	4182	0.10%	0.010%
39	17.110	2398	2401	2409	rVB7	9085	15278	0.37%	0.037%
40	17.263	2420	2427	2437	rBV	1783083	2562971	62.51%	6.175%
41	17.363	2437	2444	2456	rVV	2287689	3348531	81.67%	8.068%
42	17.457	2457	2460	2469	rVB7	21950	37893	0.92%	0.091%
43	17.927	2537	2540	2546	rVB6	12567	15176	0.37%	0.037%
44	18.145	2573	2577	2583	rBV3	51291	78715	1.92%	0.190%
45	18.557	2644	2647	2651	rVB6	12376	14439	0.35%	0.035%
46	19.174	2749	2752	2758	rVB3	30603	39740	0.97%	0.096%
47	19.239	2760	2763	2770	rBV	33355	54513	1.33%	0.131%
48	19.374	2784	2786	2794	rBV5	31151	44491	1.09%	0.107%
49	19.598	2818	2824	2832	rBV	3109664	4100088	100.00%	9.879%
50	21.051	3068	3071	3078	rBV2	192380	260262	6.35%	0.627%
51	21.345	3117	3121	3127	rBV	2490772	3241078	79.05%	7.809%
52	23.610	3500	3506	3517	rVB	1326825	2667041	65.05%	6.426%
53	23.762	3526	3532	3546	rVB2	1821662	3666077	89.41%	8.833%




Sum of corrected areas: 41503168

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012057.D
Acq On : 12 Oct 2022 00:52
Operator : CG/JU
Sample : N4991-09
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

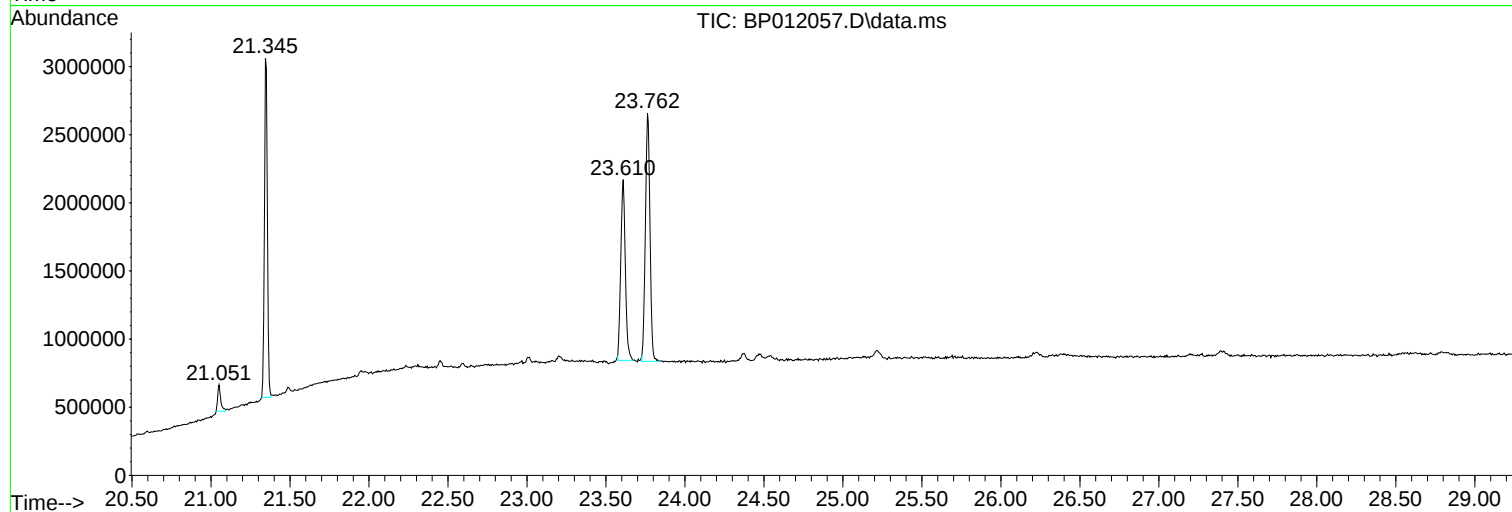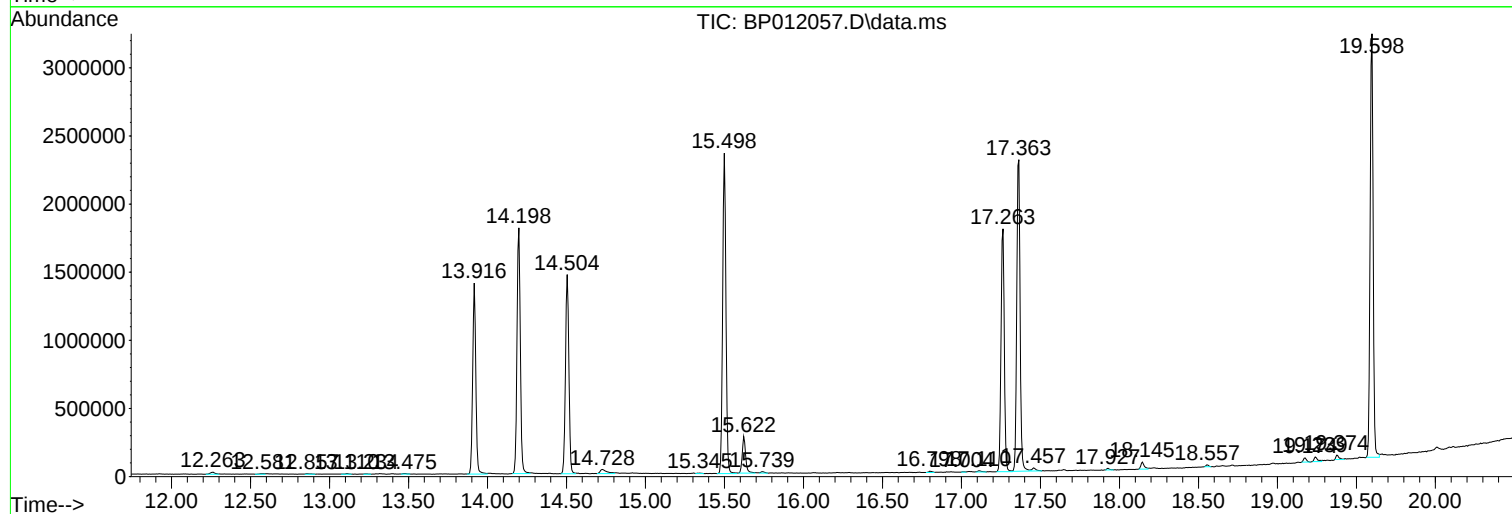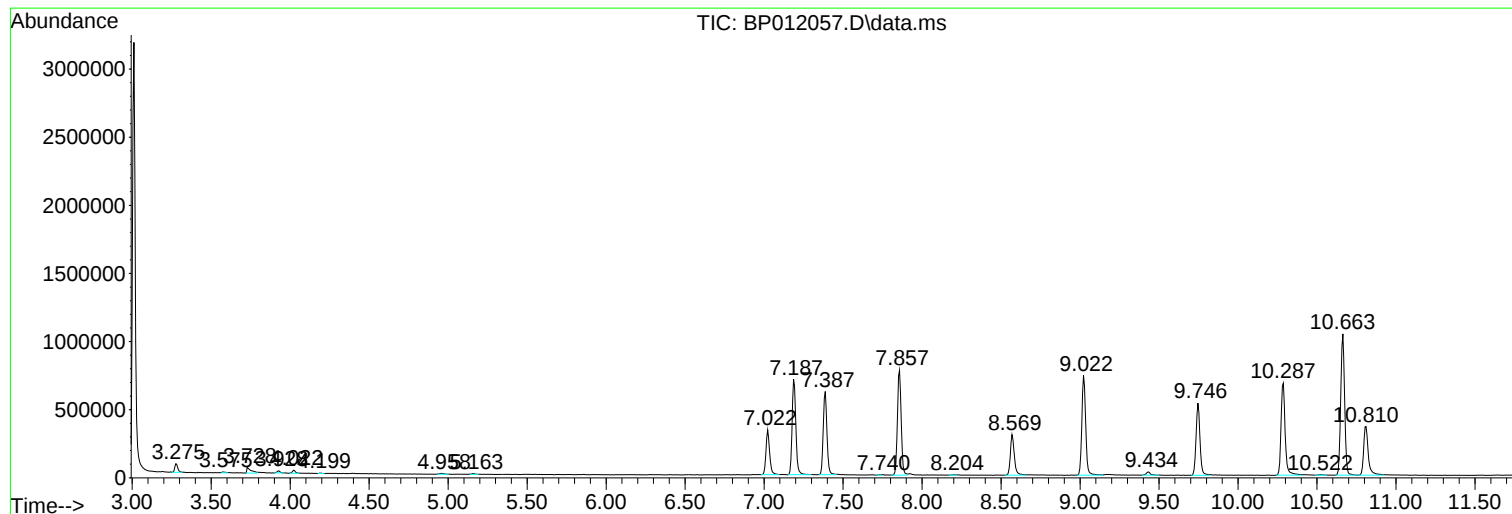

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012057.D
Acq On : 12 Oct 2022 00:52
Operator : CG/JU
Sample : N4991-09
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012057.D
Acq On : 12 Oct 2022 00:52
Operator : CG/JU
Sample : N4991-09
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
