

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012058.D
 Acq On : 12 Oct 2022 01:26
 Operator : CG/JU
 Sample : N4991-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012058.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	45	49	59	rVB	79662	105191	1.66%	0.187%
2	3.569	95	99	106	rBV	17300	28416	0.45%	0.051%
3	3.705	119	122	135	rBV	548155	833407	13.19%	1.483%
4	3.928	156	160	165	rVB	14021	21295	0.34%	0.038%
5	4.022	172	176	183	rVB	18912	26902	0.43%	0.048%
6	7.022	677	686	703	rBV	646463	1062693	16.82%	1.892%
7	7.187	708	714	727	rBV	845860	1375113	21.76%	2.448%
8	7.387	740	748	763	rBV	901417	1481326	23.44%	2.637%
9	7.857	819	828	837	rBV	732045	1213702	19.21%	2.160%
10	7.922	837	839	846	rVB4	7027	9980	0.16%	0.018%
11	8.569	940	949	974	rBV	703004	1213094	19.20%	2.159%
12	9.022	1018	1026	1044	rBV	903676	1523183	24.11%	2.711%
13	9.181	1052	1053	1060	rVB7	4568	7184	0.11%	0.013%
14	9.434	1088	1096	1103	rBV3	14176	25664	0.41%	0.046%
15	9.746	1142	1149	1162	rBV	692407	1191430	18.86%	2.121%
16	10.281	1232	1240	1258	rBV	1003216	1819454	28.79%	3.239%
17	10.663	1297	1305	1319	rVB	1022630	1726325	27.32%	3.073%
18	10.804	1322	1329	1351	rVV	814826	1492215	23.62%	2.656%
19	12.257	1568	1576	1583	rBV	19172	38722	0.61%	0.069%
20	13.110	1716	1721	1729	rVB	3879	8341	0.13%	0.015%
21	13.316	1753	1756	1764	rVB9	3394	6912	0.11%	0.012%
22	13.475	1778	1783	1788	rVB4	5089	8156	0.13%	0.015%
23	13.916	1851	1858	1872	rBV	1843047	2567549	40.63%	4.570%
24	14.198	1898	1906	1923	rBV	2329051	3453086	54.65%	6.146%
25	14.504	1951	1958	1972	rVB	1456410	2142721	33.91%	3.814%
26	14.710	1987	1993	2010	rBV	293934	582205	9.21%	1.036%
27	14.928	2024	2030	2036	rVB	6849	16329	0.26%	0.029%
28	15.498	2120	2127	2139	rBV	3091441	4353023	68.89%	7.748%
29	15.622	2142	2148	2161	rVV	597904	849088	13.44%	1.511%
30	15.739	2164	2168	2177	rVB3	14238	26978	0.43%	0.048%
31	16.216	2246	2249	2257	rVV10	4712	9334	0.15%	0.017%
32	16.798	2345	2348	2355	rVB4	12119	16760	0.27%	0.030%
33	17.110	2397	2401	2405	rBV	18290	24315	0.38%	0.043%
34	17.263	2420	2427	2436	rBV	1772538	2577061	40.78%	4.587%
35	17.363	2437	2444	2457	rVV	3126060	4687741	74.19%	8.344%
36	17.457	2457	2460	2468	rVB5	26534	45854	0.73%	0.082%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012058.D
 Acq On : 12 Oct 2022 01:26
 Operator : CG/JU
 Sample : N4991-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

37	17.928	2537	2540	2545	rVB2	30675	35151	0.56%	0.063%
38	18.145	2573	2577	2585	rBV	96074	151112	2.39%	0.269%
39	19.175	2748	2752	2757	rBV2	43685	64033	1.01%	0.114%
40	19.239	2760	2763	2770	rBV	48136	77847	1.23%	0.139%
41	19.374	2783	2786	2793	rBV2	52534	83912	1.33%	0.149%
42	19.598	2818	2824	2833	rBV	4436077	5910929	93.55%	10.521%
43	21.051	3068	3071	3076	rBV2	176431	229040	3.62%	0.408%
44	21.345	3117	3121	3129	rBV	2433708	3203080	50.69%	5.701%
45	23.610	3499	3506	3519	rVB2	3214522	6318764	100.00%	11.247%
46	23.763	3526	3532	3542	rVB2	1815879	3536263	55.96%	6.294%




Sum of corrected areas: 56180880

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012058.D
Acq On : 12 Oct 2022 01:26
Operator : CG/JU
Sample : N4991-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

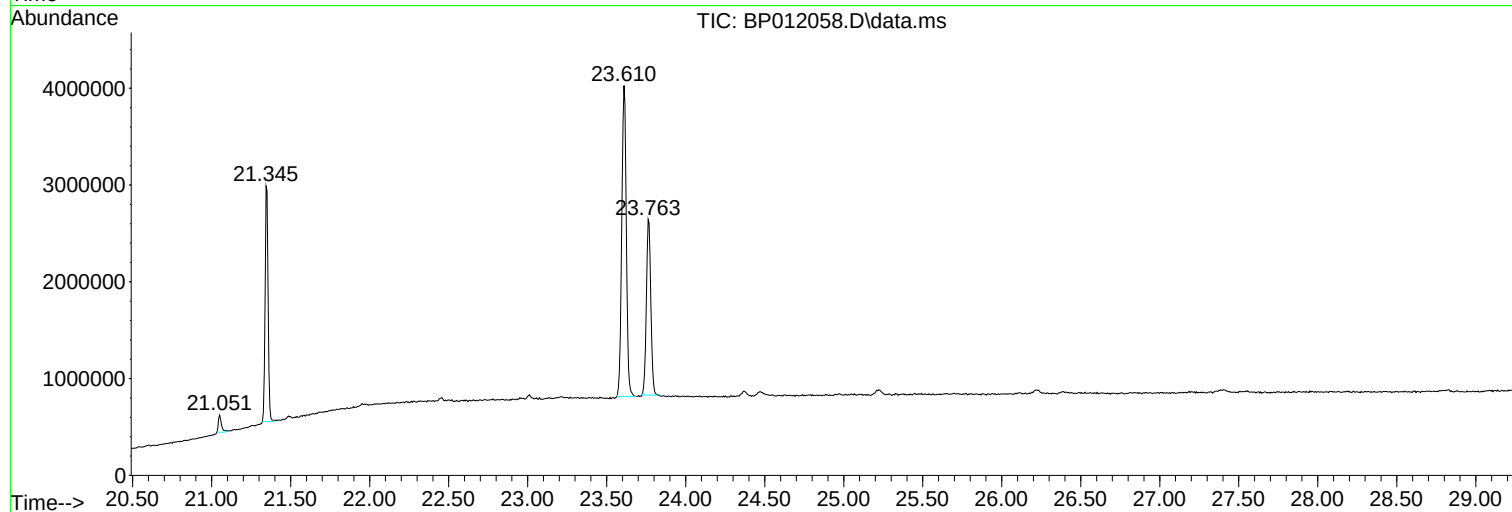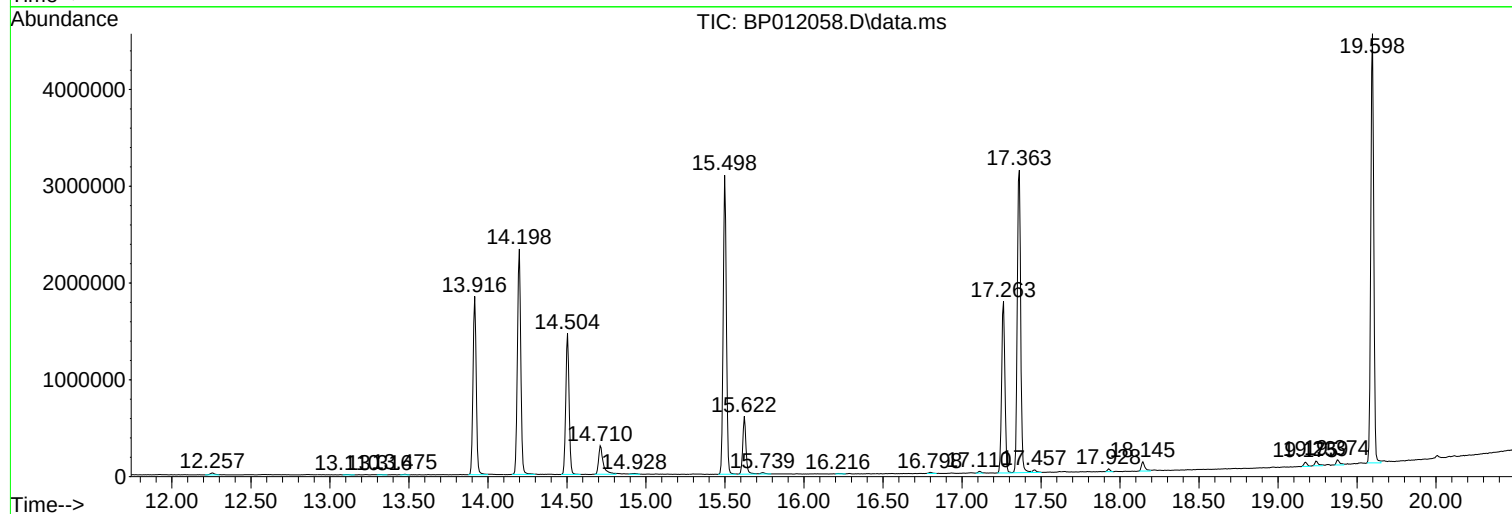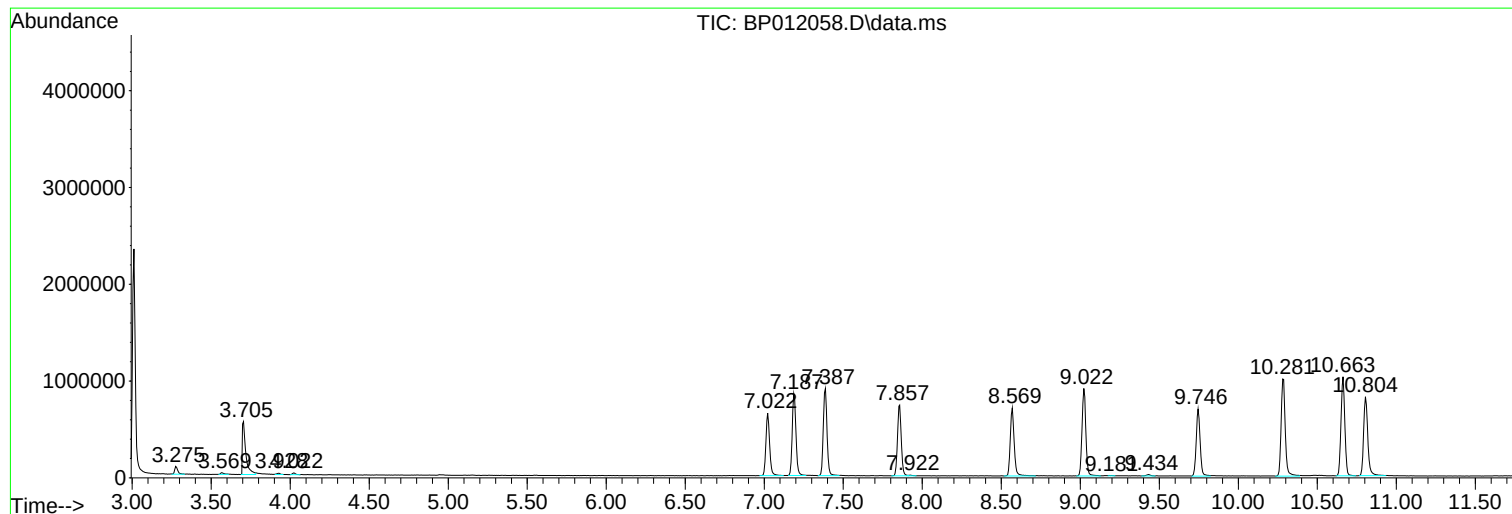

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012058.D
Acq On : 12 Oct 2022 01:26
Operator : CG/JU
Sample : N4991-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012058.D
Acq On : 12 Oct 2022 01:26
Operator : CG/JU
Sample : N4991-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
