

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012062.D
 Acq On : 12 Oct 2022 04:17
 Operator : CG/JU
 Sample : PB148150BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK150

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012062.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	45	49	56	rVB	63549	80874	1.40%	0.155%
2	3.699	118	121	146	rBV	691676	1103709	19.08%	2.121%
3	4.022	172	176	183	rVB	17620	25135	0.43%	0.048%
4	7.022	679	686	707	rBV	851776	1396566	24.14%	2.684%
5	7.187	708	714	731	rVB	737659	1176538	20.34%	2.261%
6	7.387	740	748	762	rBV	876913	1461536	25.27%	2.809%
7	7.851	820	827	842	rBV	778241	1293326	22.36%	2.486%
8	8.569	941	949	962	rBV	1018749	1719259	29.72%	3.305%
9	9.022	1017	1026	1044	rBV	759490	1290851	22.32%	2.481%
10	9.745	1141	1149	1163	rBV	589284	1006062	17.39%	1.934%
11	10.281	1232	1240	1261	rBV	941771	1670737	28.88%	3.211%
12	10.663	1296	1305	1316	rBV	1090549	1848171	31.95%	3.552%
13	10.804	1321	1329	1346	rBV	906961	1657261	28.65%	3.185%
14	12.257	1571	1576	1586	rBV2	12543	30237	0.52%	0.058%
15	12.481	1606	1614	1621	rBV2	2540	5938	0.10%	0.011%
16	13.475	1778	1783	1788	rBV7	3367	6607	0.11%	0.013%
17	13.916	1851	1858	1871	rBV	1460172	2100753	36.32%	4.038%
18	14.192	1898	1905	1925	rBV	1826619	2831042	48.94%	5.441%
19	14.504	1951	1958	1968	rBV	1483983	2231377	38.58%	4.289%
20	14.710	1987	1993	2013	rBV	543339	989419	17.11%	1.902%
21	15.498	2120	2127	2139	rBV	2524184	3514828	60.76%	6.756%
22	15.622	2142	2148	2163	rVV	590028	862125	14.90%	1.657%
23	15.739	2164	2168	2173	rVB3	12361	20127	0.35%	0.039%
24	17.257	2420	2426	2436	rBV	1737587	2517903	43.53%	4.840%
25	17.363	2437	2444	2458	rVV	2587394	3848238	66.53%	7.397%
26	19.245	2760	2764	2767	rBV	32283	44281	0.77%	0.085%
27	19.598	2818	2824	2837	rBV	3576826	4837885	83.64%	9.299%
28	21.345	3117	3121	3131	rBV	2436807	3158408	54.60%	6.071%
29	23.609	3499	3506	3521	rVB2	2945812	5784380	100.00%	11.118%
30	23.768	3526	3533	3542	rVB	1778449	3514123	60.75%	6.754%




Sum of corrected areas: 52027696

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012062.D
Acq On : 12 Oct 2022 04:17
Operator : CG/JU
Sample : PB148150BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK150

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

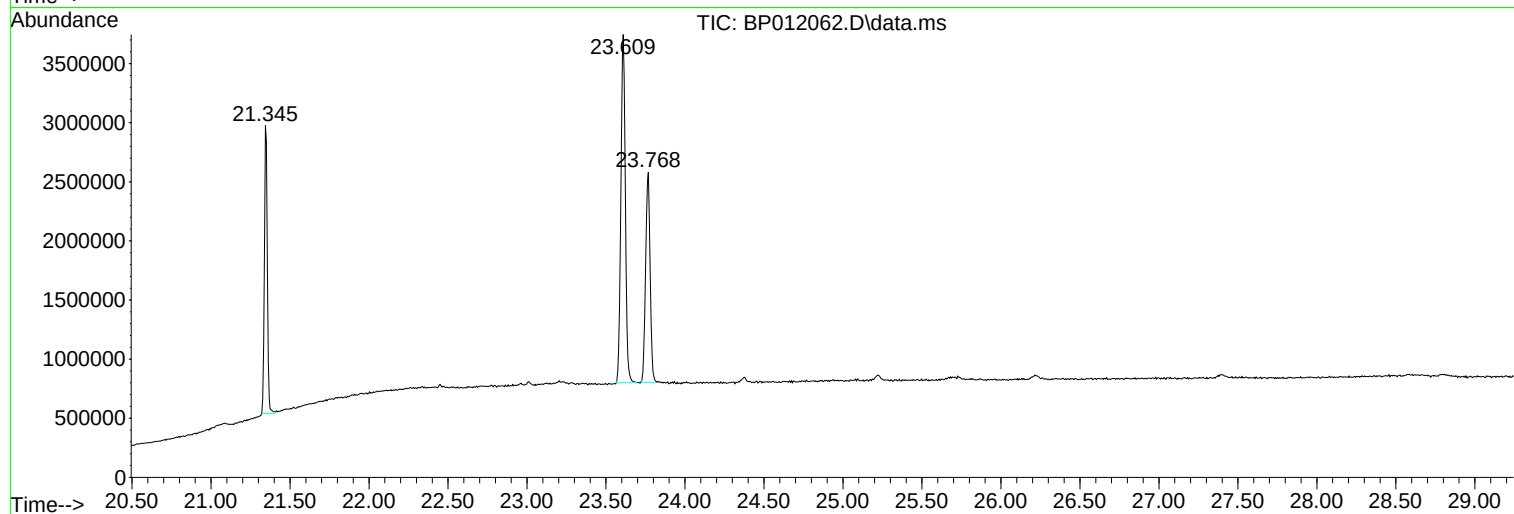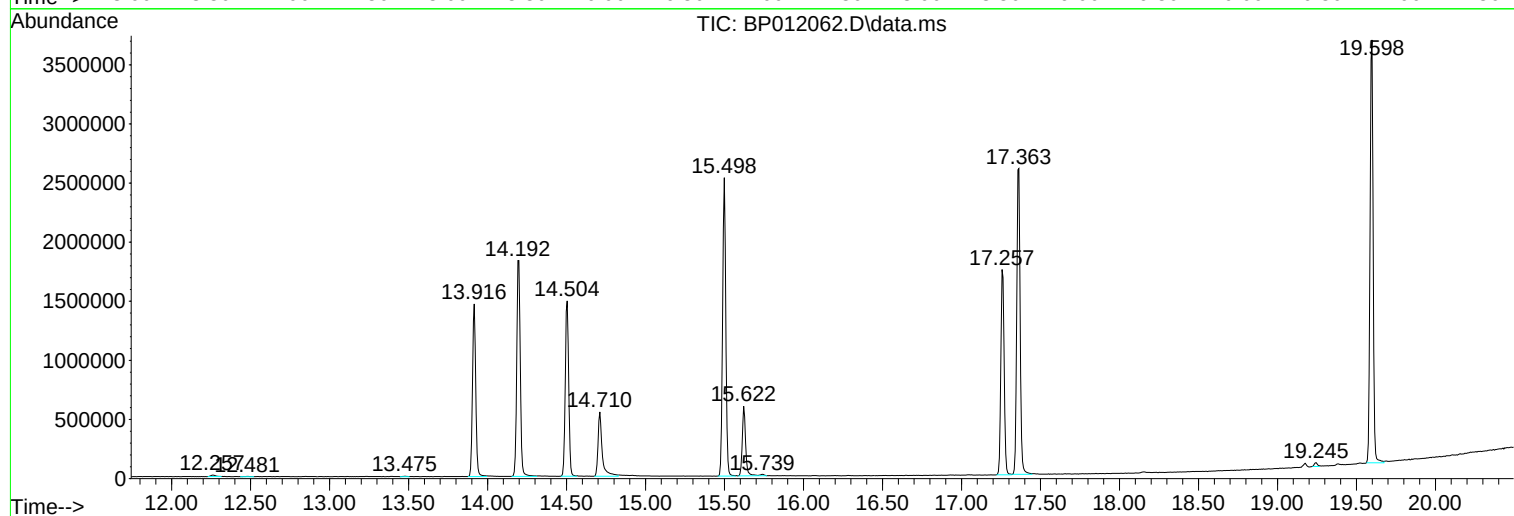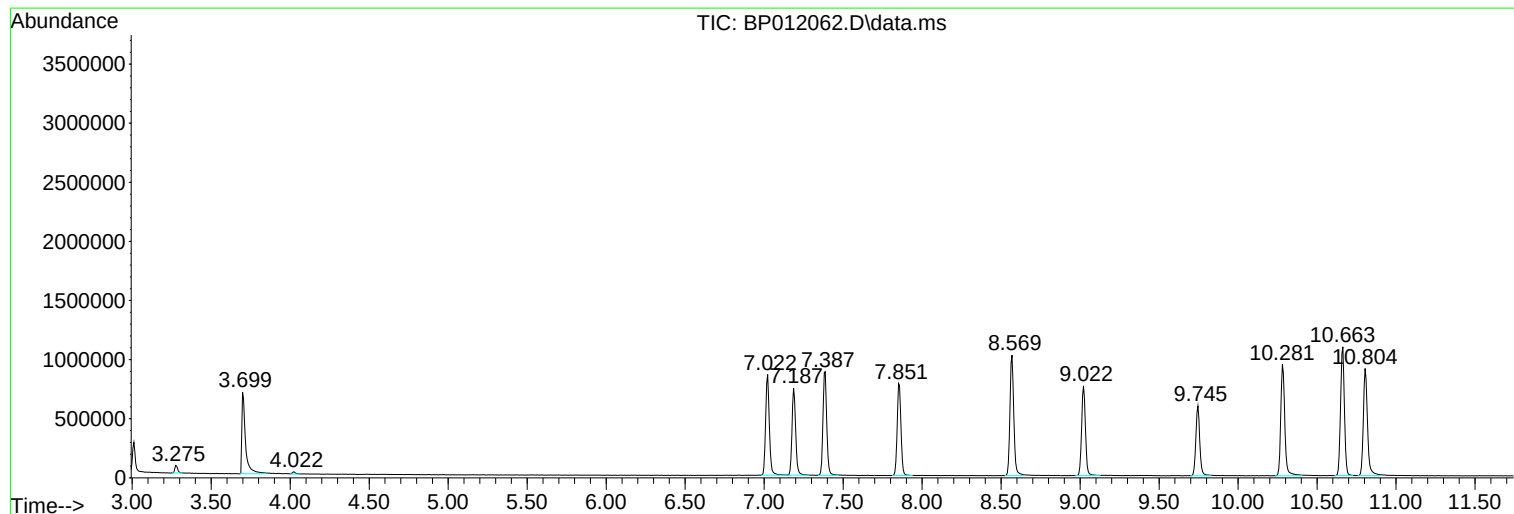

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012062.D
Acq On : 12 Oct 2022 04:17
Operator : CG/JU
Sample : PB148150BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK150

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012062.D
Acq On : 12 Oct 2022 04:17
Operator : CG/JU
Sample : PB148150BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK150

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc