

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012065.D
 Acq On : 12 Oct 2022 06:00
 Operator : CG/JU
 Sample : N4991-08
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COBG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012065.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	45	49	59	rVB	65273	87703	1.11%	0.135%
2	3.564	96	98	109	rBV	20107	33352	0.42%	0.051%
3	3.699	119	121	143	rBV	581992	944977	11.98%	1.455%
4	3.928	157	160	165	rVB2	9515	12506	0.16%	0.019%
5	4.022	172	176	183	rVB	19122	27189	0.34%	0.042%
6	7.022	679	686	702	rBV	653101	1078073	13.67%	1.660%
7	7.187	707	714	727	rBV	794894	1260116	15.98%	1.940%
8	7.381	740	747	763	rBV	842707	1376273	17.45%	2.119%
9	7.852	818	827	836	rBV	794615	1277705	16.20%	1.967%
10	7.916	836	838	844	rVB4	6341	8970	0.11%	0.014%
11	8.563	941	948	964	rBV	799179	1392041	17.65%	2.143%
12	9.022	1018	1026	1043	rBV	884542	1498958	19.01%	2.308%
13	9.428	1090	1095	1099	rBV3	9972	15393	0.20%	0.024%
14	9.746	1141	1149	1161	rBV	694641	1208373	15.32%	1.861%
15	10.281	1232	1240	1256	rBV	1113942	1930444	24.48%	2.973%
16	10.657	1296	1304	1319	rVB	1060833	1848003	23.44%	2.846%
17	10.804	1321	1329	1347	rBV	901274	1676065	21.26%	2.581%
18	12.251	1569	1575	1583	rBV	23078	39123	0.50%	0.060%
19	12.328	1583	1588	1594	rVB2	5535	10010	0.13%	0.015%
20	13.322	1751	1757	1764	rVB10	5312	10439	0.13%	0.016%
21	13.828	1837	1843	1847	rVB6	4948	9350	0.12%	0.014%
22	13.916	1847	1858	1871	rBV	2147944	3070242	38.94%	4.728%
23	14.198	1899	1906	1920	rBV	2684608	4042326	51.26%	6.224%
24	14.504	1950	1958	1973	rBV	1536564	2354754	29.86%	3.626%
25	14.710	1987	1993	2015	rBV	484505	864568	10.96%	1.331%
26	14.922	2022	2029	2035	rVB	11987	26316	0.33%	0.041%
27	15.069	2048	2054	2061	rBV2	11125	26259	0.33%	0.040%
28	15.292	2087	2092	2096	rBV7	5733	9262	0.12%	0.014%
29	15.498	2120	2127	2138	rBV	3675433	5185855	65.77%	7.985%
30	15.622	2141	2148	2161	rVV	789746	1149721	14.58%	1.770%
31	15.739	2164	2168	2174	rVB2	16678	28254	0.36%	0.044%
32	16.210	2243	2248	2258	rBV3	21978	46071	0.58%	0.071%
33	16.798	2344	2348	2352	rBV3	12157	19021	0.24%	0.029%
34	17.257	2420	2426	2437	rBV	1974137	2911168	36.92%	4.483%
35	17.357	2437	2443	2455	rVV2	3944445	5691926	72.18%	8.765%
36	17.457	2456	2460	2470	rVB5	34064	64365	0.82%	0.099%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012065.D
 Acq On : 12 Oct 2022 06:00
 Operator : CG/JU
 Sample : N4991-08
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

37	17.622	2484	2488	2489	rBV3	5760	8168	0.10%	0.013%
38	17.927	2535	2540	2545	rBV	69055	88586	1.12%	0.136%
39	18.145	2572	2577	2586	rBV	150352	253356	3.21%	0.390%
40	19.174	2748	2752	2758	rBV3	53652	79012	1.00%	0.122%
41	19.239	2760	2763	2766	rBV	59563	75193	0.95%	0.116%
42	19.374	2783	2786	2793	rBV2	104312	141842	1.80%	0.218%
43	19.598	2818	2824	2841	rBV	5487450	7234669	91.75%	11.140%
44	21.051	3067	3071	3079	rBV	247875	389088	4.93%	0.599%
45	21.345	3116	3121	3128	rBV	2897153	3653808	46.34%	5.626%
46	23.610	3499	3506	3518	rVB2	3968422	7885231	100.00%	12.142%
47	23.762	3526	3532	3544	rVB2	1879161	3898401	49.44%	6.003%




Sum of corrected areas: 64942525

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012065.D
Acq On : 12 Oct 2022 06:00
Operator : CG/JU
Sample : N4991-08
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

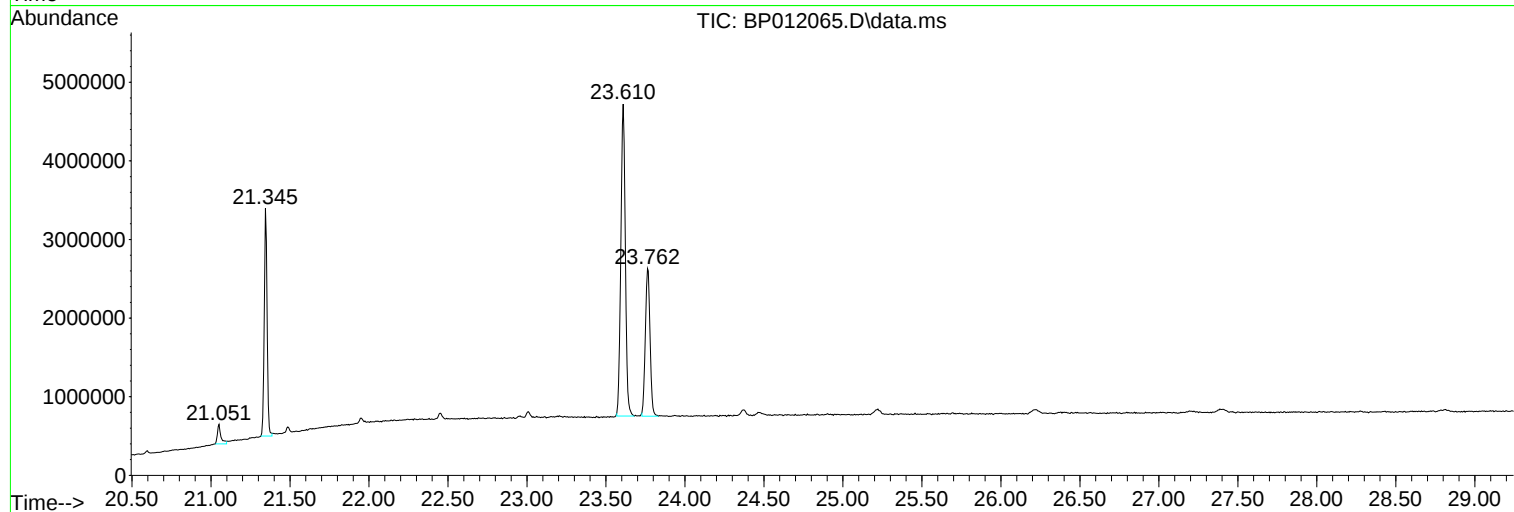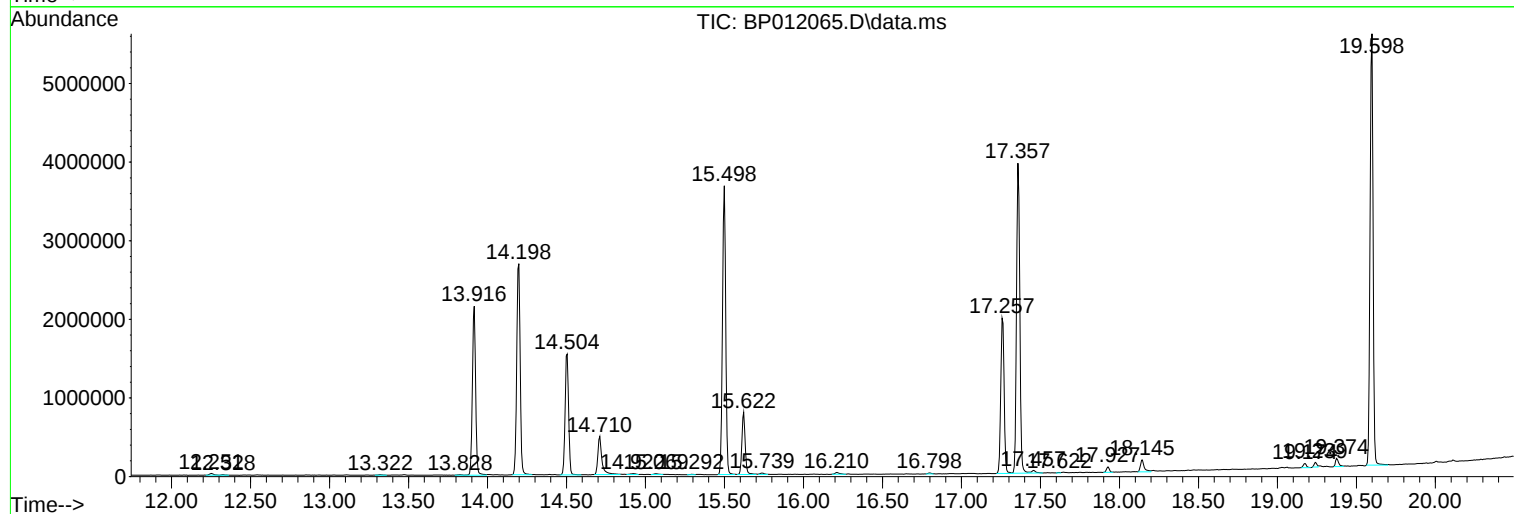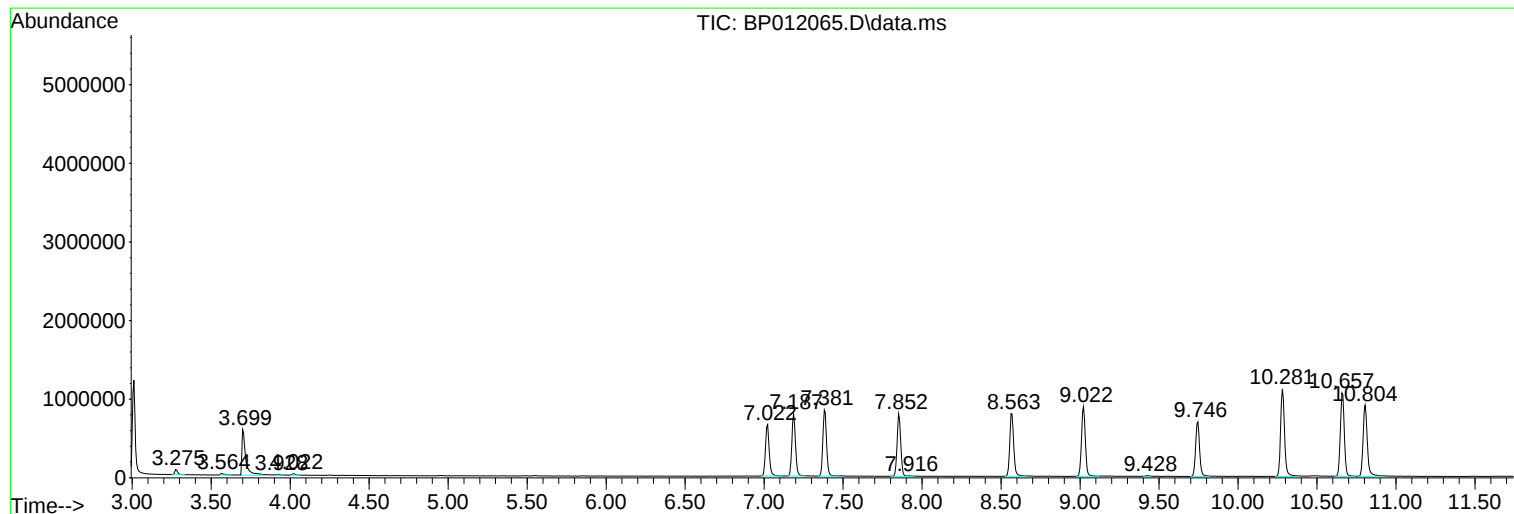

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012065.D
Acq On : 12 Oct 2022 06:00
Operator : CG/JU
Sample : N4991-08
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BG0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2- Chloropropionic acid, oc... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.051	2.13 ng/ul	389088	Chrysene-d12	21.345

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-	Chloropropionic acid, octadec...	360	C21H41ClO2	088104-31-8	94	
2	Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	91		
3	1-Hexadecanesulfonyl chloride	324	C16H33ClO2S	038775-38-1	91		
4	Ethanol, 2-(tetradecyloxy)-	258	C16H34O2	002136-70-1	91		
5	2- Chloropropionic acid, hexadec...	332	C19H37ClO2	086711-81-1	89		

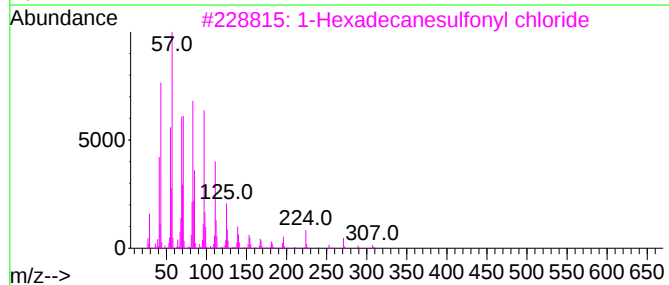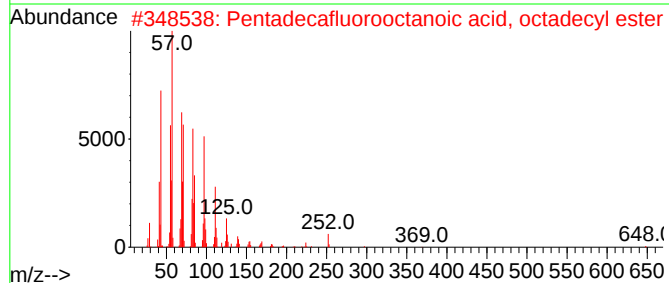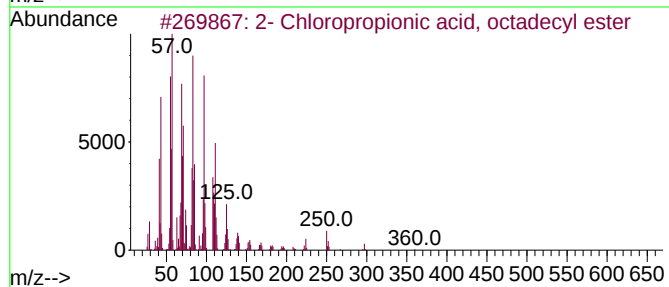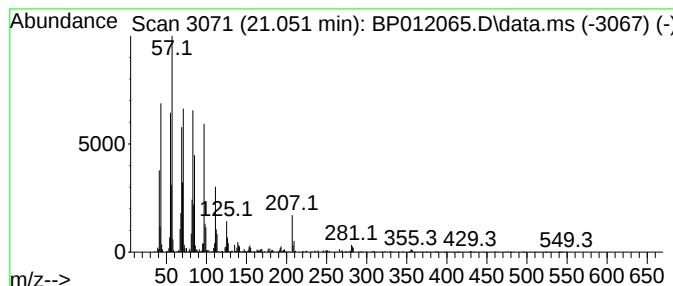

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012065.D
Acq On : 12 Oct 2022 06:00
Operator : CG/JU
Sample : N4991-08
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2- Chloropropio...	21.051	2.1	ng/u1	389088	5	21.345	3653810	20.0