

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012072.D
 Acq On : 12 Oct 2022 09:59
 Operator : CG/JU
 Sample : PB148184BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK184

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012072.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	45	49	63	rVB	63827	90439	1.92%	0.189%
2	3.699	119	121	148	rBV	658457	1035288	21.93%	2.167%
3	4.023	171	176	183	rVB	16137	27264	0.58%	0.057%
4	7.016	679	685	699	rBV	770388	1270349	26.91%	2.659%
5	7.187	707	714	729	rVB	669429	1098741	23.27%	2.300%
6	7.381	740	747	760	rBV	836743	1342936	28.44%	2.811%
7	7.852	820	827	846	rVB	803298	1304569	27.63%	2.730%
8	8.563	941	948	973	rBV	927557	1600604	33.90%	3.350%
9	9.022	1017	1026	1047	rBV	692958	1200799	25.43%	2.513%
10	9.740	1141	1148	1159	rBV	510600	905888	19.19%	1.896%
11	10.281	1232	1240	1262	rBV	875554	1548303	32.79%	3.241%
12	10.657	1297	1304	1320	rVB	1085264	1869351	39.59%	3.912%
13	10.805	1320	1329	1356	rBV	862596	1617999	34.27%	3.386%
14	12.257	1571	1576	1585	rBV2	11495	27515	0.58%	0.058%
15	13.910	1851	1857	1869	rBV	1296832	1923917	40.75%	4.027%
16	14.193	1897	1905	1928	rBV	1669280	2615745	55.40%	5.475%
17	14.498	1950	1957	1971	rBV	1519229	2278258	48.26%	4.768%
18	14.704	1985	1992	2015	rBV	431455	856245	18.14%	1.792%
19	15.498	2120	2127	2140	rBV	2270678	3281410	69.50%	6.868%
20	15.622	2142	2148	2160	rVV	469026	707631	14.99%	1.481%
21	15.740	2164	2168	2173	rVB2	11174	18511	0.39%	0.039%
22	17.051	2387	2391	2393	rBV4	5170	5270	0.11%	0.011%
23	17.257	2420	2426	2437	rBV	1735248	2506028	53.08%	5.245%
24	17.357	2437	2443	2461	rVV	2350519	3411328	72.26%	7.140%
25	18.151	2576	2578	2583	rBV6	6177	9659	0.20%	0.020%
26	19.175	2749	2752	2757	rVB2	23739	30744	0.65%	0.064%
27	19.245	2761	2764	2768	rVB	25682	31102	0.66%	0.065%
28	19.598	2818	2824	2833	rBV	3025087	4140431	87.70%	8.666%
29	21.351	3117	3122	3132	rBV	2238923	3031212	64.20%	6.344%
30	23.610	3499	3506	3517	rVB2	2354032	4721197	100.00%	9.881%
31	23.769	3527	3533	3542	rVB2	1666028	3270230	69.27%	6.844%




Sum of corrected areas: 47778963

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012072.D
Acq On : 12 Oct 2022 09:59
Operator : CG/JU
Sample : PB148184BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK184

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

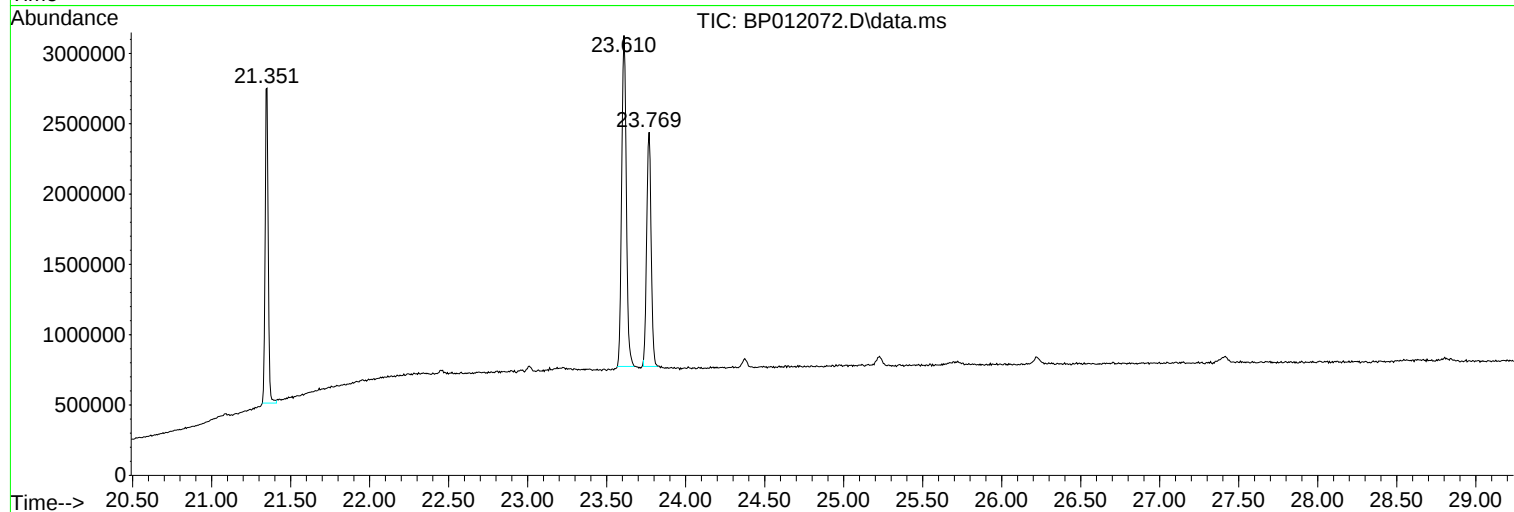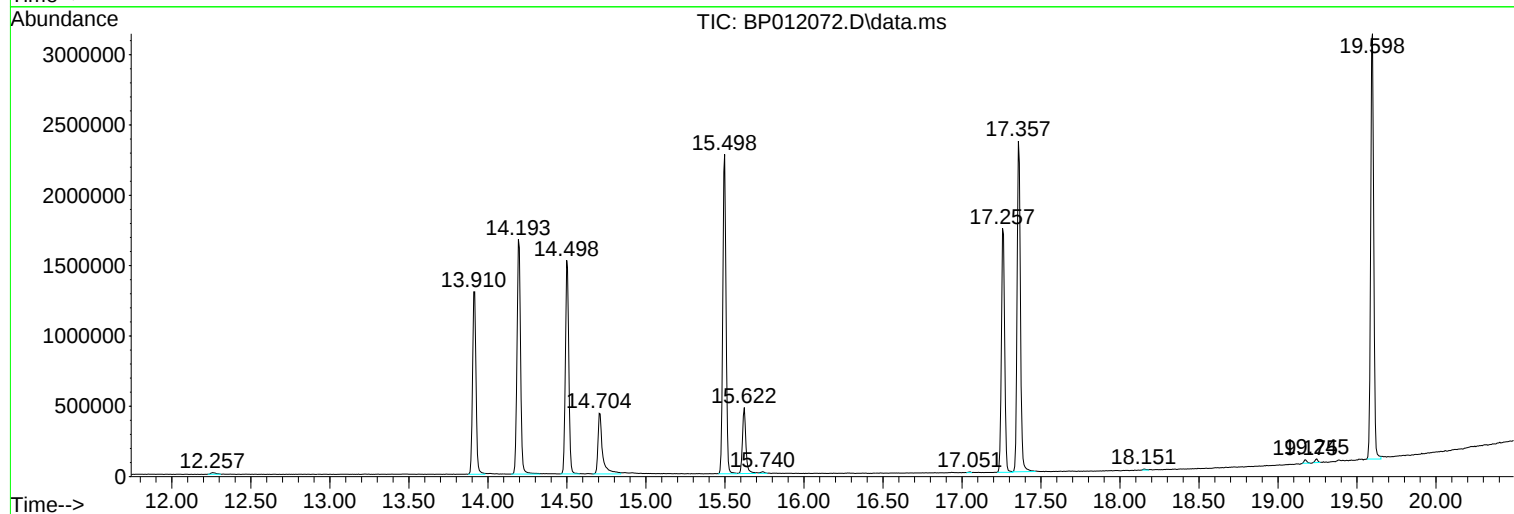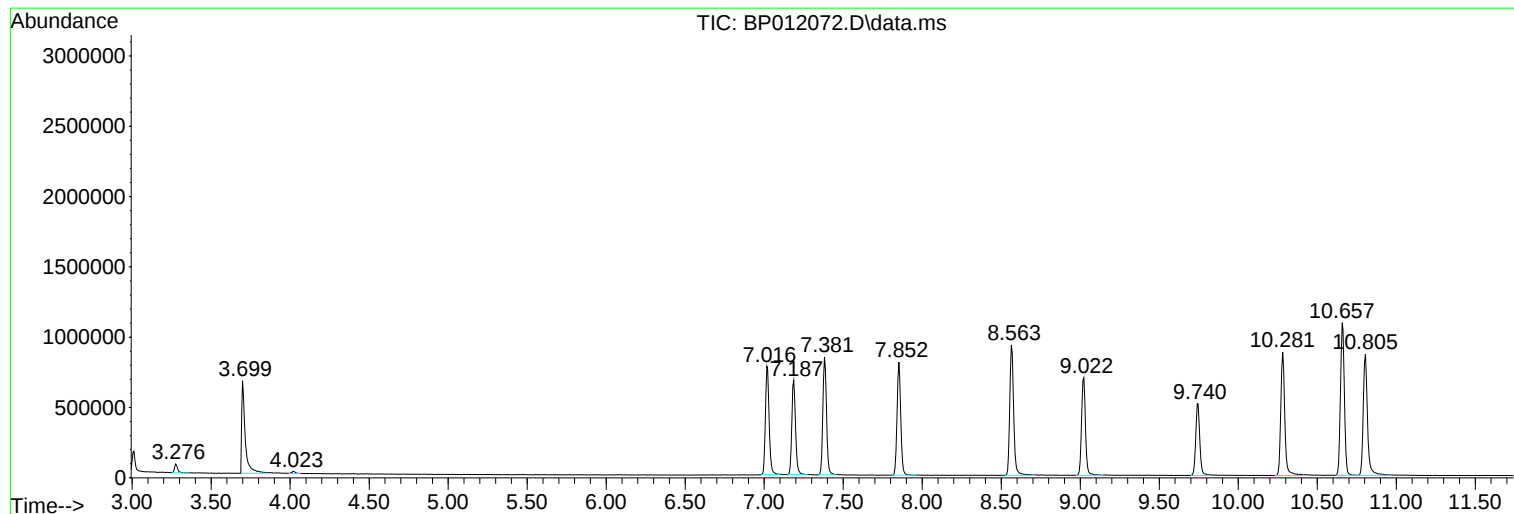

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012072.D
Acq On : 12 Oct 2022 09:59
Operator : CG/JU
Sample : PB148184BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK184

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012072.D
Acq On : 12 Oct 2022 09:59
Operator : CG/JU
Sample : PB148184BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK184

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc