

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012080.D
 Acq On : 12 Oct 2022 14:35
 Operator : CG/JU
 Sample : N5024-02
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012080.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	46	49	54	rVB	33366	42122	1.08%	0.106%
2	3.717	121	124	136	rBV	81121	140390	3.60%	0.354%
3	3.805	136	139	145	rVB	21317	29282	0.75%	0.074%
4	3.922	155	159	165	rVB	37142	57032	1.46%	0.144%
5	4.022	172	176	183	rVB	24153	32860	0.84%	0.083%
6	4.399	238	240	245	rVB6	7687	10379	0.27%	0.026%
7	4.964	328	336	343	rBV2	49125	105132	2.70%	0.265%
8	5.481	419	424	432	rBV	13058	25407	0.65%	0.064%
9	5.546	432	435	447	rVB9	5308	11750	0.30%	0.030%
10	5.858	483	488	493	rVB	22463	33091	0.85%	0.084%
11	6.334	563	569	576	rBV8	5861	15658	0.40%	0.040%
12	6.481	589	594	596	rVV6	7495	13028	0.33%	0.033%
13	6.505	596	598	606	rVB4	6702	11855	0.30%	0.030%
14	6.828	649	653	660	rVB6	5824	10684	0.27%	0.027%
15	7.022	676	686	701	rVV	436001	757128	19.42%	1.911%
16	7.187	708	714	732	rVB	403058	664458	17.04%	1.677%
17	7.387	741	748	758	rBV	494525	809123	20.75%	2.042%
18	7.469	758	762	764	rVV	17189	25524	0.65%	0.064%
19	7.499	764	767	773	rVB2	12999	20691	0.53%	0.052%
20	7.858	816	828	838	rBV	681139	1135148	29.11%	2.865%
21	7.969	842	847	853	rVB3	7977	14186	0.36%	0.036%
22	8.569	942	949	964	rVV	447525	770033	19.75%	1.944%
23	8.687	964	969	978	rVB	52974	89626	2.30%	0.226%
24	9.022	1019	1026	1033	rBV	425765	708993	18.18%	1.790%
25	9.081	1033	1036	1040	rVB	16888	23564	0.60%	0.059%
26	9.422	1090	1094	1099	rBV4	6596	10063	0.26%	0.025%
27	9.746	1140	1149	1160	rBV	323124	572902	14.69%	1.446%
28	10.104	1207	1210	1217	rVB7	5523	10783	0.28%	0.027%
29	10.287	1234	1241	1263	rVB	502431	925881	23.74%	2.337%
30	10.446	1263	1268	1281	rBV	59743	138971	3.56%	0.351%
31	10.663	1294	1305	1311	rBV	928272	1590910	40.80%	4.016%
32	10.710	1311	1313	1320	rVB	43878	63045	1.62%	0.159%
33	10.804	1322	1329	1340	rBV	337471	644869	16.54%	1.628%
34	11.575	1455	1460	1467	rVB	7308	14605	0.37%	0.037%
35	11.681	1473	1478	1485	rBV2	14982	25974	0.67%	0.066%
36	12.081	1540	1546	1551	rBV	27227	41754	1.07%	0.105%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012080.D
 Acq On : 12 Oct 2022 14:35
 Operator : CG/JU
 Sample : N5024-02
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

37	12.251	1571	1575	1580	rBV	9639	14194	0.36%	0.036%
38	12.322	1580	1587	1594	rVB	57848	97711	2.51%	0.247%
39	12.546	1617	1625	1633	rVV	52284	87196	2.24%	0.220%
40	13.028	1703	1707	1713	rVV3	11220	17525	0.45%	0.044%

41	13.104	1715	1720	1725	rVB9	5059	9822	0.25%	0.025%
42	13.322	1749	1757	1765	rBV3	29334	60978	1.56%	0.154%
43	13.398	1765	1770	1775	rVB8	5997	10904	0.28%	0.028%
44	13.534	1789	1793	1795	rBV3	7993	12010	0.31%	0.030%
45	13.663	1809	1815	1816	rBV2	23389	30116	0.77%	0.076%

46	13.822	1836	1842	1847	rBV	51832	92807	2.38%	0.234%
47	13.875	1847	1851	1853	rVV	45492	64230	1.65%	0.162%
48	13.916	1853	1858	1865	rVV	880354	1213719	31.13%	3.064%
49	13.975	1865	1868	1872	rVB	20891	30049	0.77%	0.076%
50	14.063	1878	1883	1886	rBV	28392	42338	1.09%	0.107%

51	14.093	1886	1888	1893	rVB3	17756	22240	0.57%	0.056%
52	14.198	1899	1906	1921	rVB	1074954	1699207	43.58%	4.289%
53	14.392	1935	1939	1944	rVB	26265	35516	0.91%	0.090%
54	14.504	1948	1958	1965	rBV	1293914	1971090	50.55%	4.975%
55	14.563	1965	1968	1977	rVB4	21598	44176	1.13%	0.112%

56	14.716	1988	1994	2004	rBV	211124	439272	11.27%	1.109%
57	14.904	2020	2026	2034	rBV3	52172	112246	2.88%	0.283%
58	14.975	2035	2038	2043	rVB	23114	31107	0.80%	0.079%
59	15.122	2058	2063	2068	rBV2	25592	44301	1.14%	0.112%
60	15.175	2068	2072	2077	rVB	24908	34083	0.87%	0.086%

61	15.292	2085	2092	2095	rBV4	32754	60470	1.55%	0.153%
62	15.328	2095	2098	2099	rVV3	19299	25173	0.65%	0.064%
63	15.351	2099	2102	2107	rVB	30649	39728	1.02%	0.100%
64	15.498	2121	2127	2132	rBV	1464198	2097996	53.80%	5.296%
65	15.545	2132	2135	2141	rVB2	61634	90508	2.32%	0.228%

66	15.622	2143	2148	2156	rBV	205052	297639	7.63%	0.751%
67	15.851	2180	2187	2194	rVB	42416	78144	2.00%	0.197%
68	15.963	2203	2206	2208	rVV4	16512	24087	0.62%	0.061%
69	15.992	2208	2211	2220	rVV2	45771	98157	2.52%	0.248%
70	16.087	2220	2227	2234	rVB2	19652	45473	1.17%	0.115%

71	16.234	2244	2252	2258	rBV2	73876	162368	4.16%	0.410%
72	16.369	2270	2275	2278	rBV2	11209	19325	0.50%	0.049%
73	16.404	2278	2281	2285	rVB	10692	13800	0.35%	0.035%
74	16.657	2321	2324	2329	rBV6	7854	13434	0.34%	0.034%
75	16.792	2342	2347	2351	rBV2	43877	82359	2.11%	0.208%

76	16.916	2364	2368	2376	rBV3	25559	51757	1.33%	0.131%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012080.D
 Acq On : 12 Oct 2022 14:35
 Operator : CG/JU
 Sample : N5024-02
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

77	16.986	2376	2380	2381	rBV2	30073	33249	0.85%	0.084%
78	17.010	2381	2384	2388	rVB	40596	56861	1.46%	0.144%
79	17.263	2421	2427	2431	rBV	1617722	2294194	58.84%	5.791%
80	17.304	2431	2434	2438	rVV	312044	410400	10.52%	1.036%
81	17.363	2438	2444	2454	rVV	1540640	2273953	58.32%	5.740%
82	17.457	2456	2460	2464	rVB4	25092	41171	1.06%	0.104%
83	17.669	2494	2496	2500	rBV3	18797	23276	0.60%	0.059%
84	17.751	2507	2510	2514	rVB	49509	59146	1.52%	0.149%
85	18.139	2571	2576	2579	rBV3	129001	228241	5.85%	0.576%
86	18.175	2579	2582	2588	rVB	133788	191307	4.91%	0.483%
87	18.310	2601	2605	2610	rBV2	86415	157063	4.03%	0.396%
88	18.351	2610	2612	2617	rVB2	66493	85376	2.19%	0.216%
89	18.428	2621	2625	2629	rVV	68914	81676	2.09%	0.206%
90	18.616	2654	2657	2661	rBV2	38876	46241	1.19%	0.117%
91	19.016	2721	2725	2726	rBV	84524	101082	2.59%	0.255%
92	19.275	2764	2769	2774	rVB	382468	528222	13.55%	1.333%
93	19.375	2783	2786	2791	rBV4	73848	110968	2.85%	0.280%
94	19.598	2819	2824	2836	rVB2	2417587	3570355	91.56%	9.012%
95	20.116	2909	2912	2916	rVB2	127269	153255	3.93%	0.387%
96	20.598	2992	2994	2999	rVB2	114970	118840	3.05%	0.300%
97	21.051	3068	3071	3077	rBV2	352074	501501	12.86%	1.266%
98	21.351	3117	3122	3126	rBV	2113388	2835296	72.71%	7.157%
99	23.616	3501	3507	3524	rVB	1754323	3899328	100.00%	9.842%
100	23.774	3528	3534	3541	rVB2	1436464	2802392	71.87%	7.074%



Sum of corrected areas: 39617549

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012080.D
Acq On : 12 Oct 2022 14:35
Operator : CG/JU
Sample : N5024-02
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

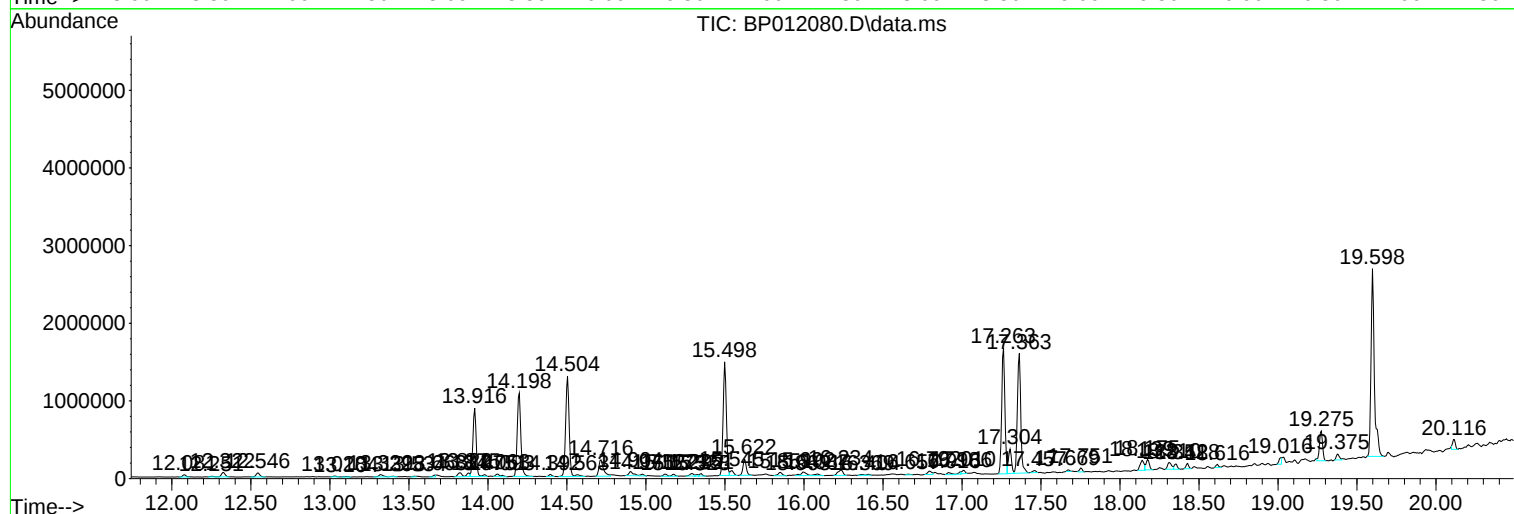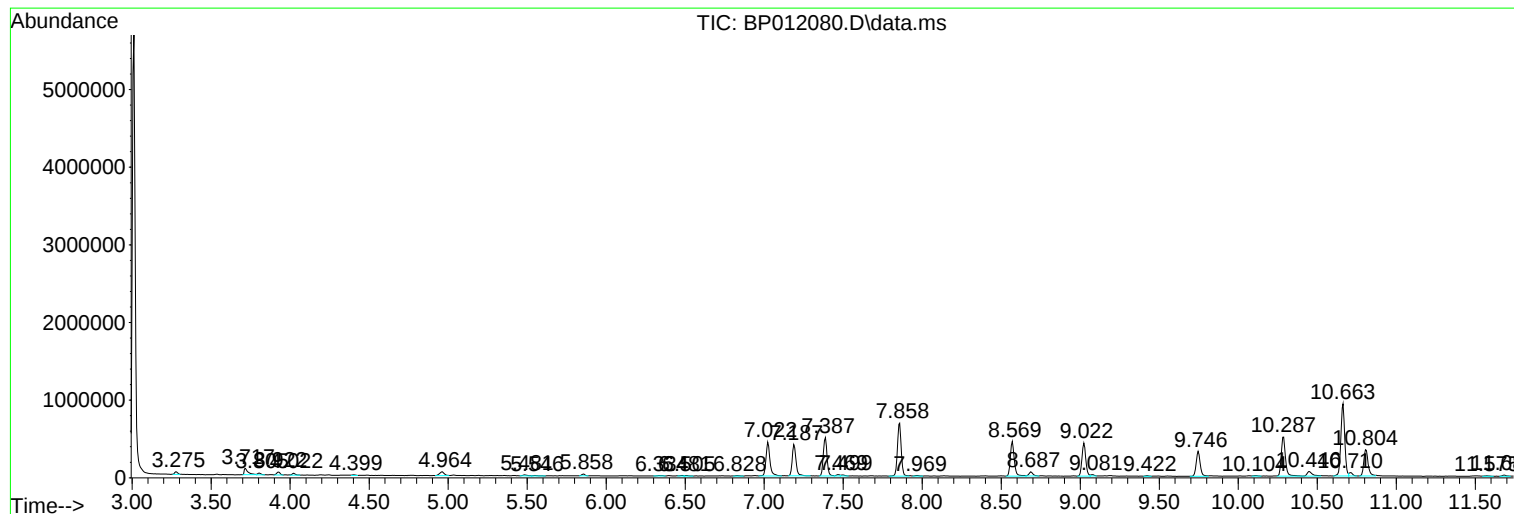

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012080.D
Acq On : 12 Oct 2022 14:35
Operator : CG/JU
Sample : N5024-02
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BE8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Oxalic acid, isobutyl hexadec... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.051	3.54 ng/ul	501501	Chrysene-d12	21.351

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Oxalic acid, isobutyl hexadecyl ...	370	C22H42O4	1000309-38-1	91
2			Oxalic acid, isobutyl heptadecyl...	384	C23H44O4	1000309-38-2	91
3			Oxalic acid, hexadecyl propyl ester	356	C21H40O4	1000309-26-9	91
4			Oxalic acid, isobutyl octadecyl ...	398	C24H46O4	1000309-38-3	91
5			2- Chloropropionic acid, hexadec...	332	C19H37ClO2	086711-81-1	78

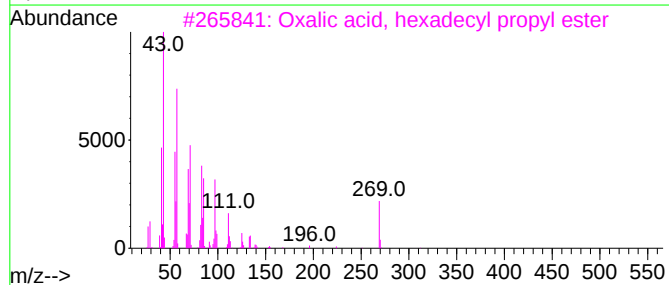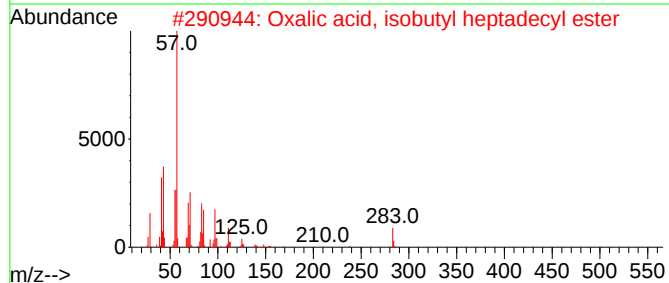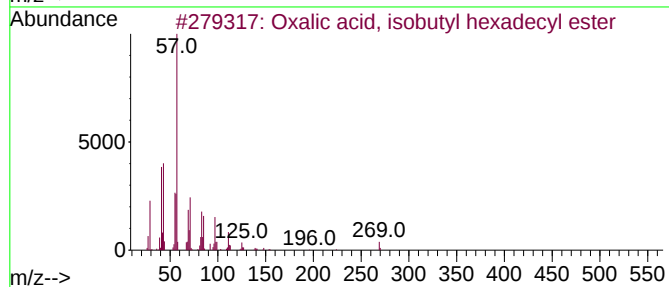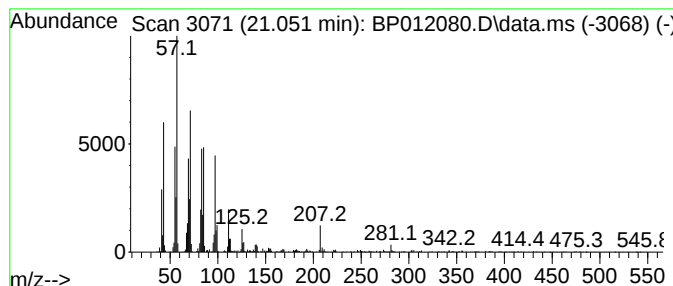

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012080.D
Acq On : 12 Oct 2022 14:35
Operator : CG/JU
Sample : N5024-02
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Oxalic acid, is...	21.051	3.5	ng/u1	501501	5	21.351	2835300	20.0