

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012082.D
 Acq On : 12 Oct 2022 15:44
 Operator : CG/JU
 Sample : N5024-05
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012082.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	45	49	56	rVB	45392	58388	1.29%	0.155%
2	3.575	97	100	105	rVB	5326	7966	0.18%	0.021%
3	3.746	127	129	135	rBV4	9031	15468	0.34%	0.041%
4	3.805	136	139	146	rVB	16925	22982	0.51%	0.061%
5	3.928	154	160	168	rVB	47482	75753	1.67%	0.201%
6	4.022	172	176	183	rVB	16009	22386	0.49%	0.059%
7	4.399	237	240	247	rVB7	7532	12805	0.28%	0.034%
8	4.946	329	333	340	rVB	22507	35078	0.77%	0.093%
9	6.893	658	664	670	rBV10	2937	7945	0.17%	0.021%
10	7.022	680	686	706	rVB	465406	783305	17.24%	2.074%
11	7.187	708	714	732	rVB	508759	820410	18.06%	2.172%
12	7.387	741	748	758	rBV	578321	954141	21.00%	2.526%
13	7.463	758	761	772	rVB8	7962	18648	0.41%	0.049%
14	7.852	820	827	836	rBV	687576	1128370	24.84%	2.987%
15	8.569	942	949	960	rBV	404664	691169	15.21%	1.830%
16	8.687	965	969	980	rVB	23221	45272	1.00%	0.120%
17	9.022	1017	1026	1041	rBV	521035	881839	19.41%	2.335%
18	9.422	1088	1094	1099	rVB	7462	12912	0.28%	0.034%
19	9.746	1141	1149	1158	rBV	399449	681255	15.00%	1.804%
20	10.110	1206	1211	1215	rVB6	5214	7825	0.17%	0.021%
21	10.281	1232	1240	1262	rBV	571221	1065280	23.45%	2.820%
22	10.469	1265	1272	1279	rBV6	8888	25354	0.56%	0.067%
23	10.663	1294	1305	1319	rBV	899070	1565240	34.45%	4.144%
24	10.804	1322	1329	1350	rBV	312958	626589	13.79%	1.659%
25	12.081	1540	1546	1551	rBV8	4005	6986	0.15%	0.018%
26	12.251	1571	1575	1583	rVV2	9868	17361	0.38%	0.046%
27	12.328	1583	1588	1593	rVB4	5535	9282	0.20%	0.025%
28	12.545	1619	1625	1630	rBV	5757	8622	0.19%	0.023%
29	13.110	1717	1721	1726	rBV5	4329	7186	0.16%	0.019%
30	13.322	1747	1757	1765	rBV3	10837	25136	0.55%	0.067%
31	13.828	1836	1843	1849	rBV7	9501	18178	0.40%	0.048%
32	13.916	1852	1858	1873	rVB	921187	1327631	29.22%	3.515%
33	14.192	1897	1905	1918	rBV	1138140	1829597	40.27%	4.844%
34	14.398	1935	1940	1946	rVB7	5935	9720	0.21%	0.026%
35	14.504	1949	1958	1967	rBV	1178063	1779890	39.18%	4.712%
36	14.716	1988	1994	2009	rBV	133787	299942	6.60%	0.794%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012082.D
 Acq On : 12 Oct 2022 15:44
 Operator : CG/JU
 Sample : N5024-05
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

37	14.928	2017	2030	2036	rBV5	22137	53708	1.18%	0.142%
38	15.298	2087	2093	2096	rBV8	3968	7348	0.16%	0.019%
39	15.498	2120	2127	2134	rBV	1508198	2227117	49.02%	5.897%
40	15.622	2143	2148	2160	rBV	216803	326606	7.19%	0.865%
41	15.739	2165	2168	2176	rVB9	7431	13757	0.30%	0.036%
42	16.216	2244	2249	2250	rBV5	6116	8786	0.19%	0.023%
43	16.798	2344	2348	2357	rBV2	16968	28196	0.62%	0.075%
44	16.922	2364	2369	2375	rVB5	9617	17234	0.38%	0.046%
45	17.263	2420	2427	2431	rBV	1366631	1926080	42.40%	5.099%
46	17.304	2431	2434	2438	rVV	115125	156446	3.44%	0.414%
47	17.363	2438	2444	2455	rVB	1428686	2166487	47.69%	5.736%
48	17.457	2456	2460	2468	rVV8	35281	68177	1.50%	0.181%
49	17.651	2490	2493	2494	rBV2	8800	9699	0.21%	0.026%
50	18.145	2572	2577	2581	rBV4	73468	121276	2.67%	0.321%
51	19.275	2765	2769	2774	rVB	242765	317634	6.99%	0.841%
52	19.380	2784	2787	2791	rBV2	43341	61154	1.35%	0.162%
53	19.598	2819	2824	2835	rBV	2717559	3901086	85.87%	10.329%
54	21.051	3068	3071	3080	rBV4	203688	339522	7.47%	0.899%
55	21.351	3117	3122	3127	rBV	2401087	3169806	69.78%	8.392%
56	23.615	3501	3507	3521	rVB2	2134639	4542896	100.00%	12.028%
57	23.774	3528	3534	3542	rVB2	1725573	3401114	74.87%	9.005%




Sum of corrected areas: 37770040

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012082.D
Acq On : 12 Oct 2022 15:44
Operator : CG/JU
Sample : N5024-05
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BF4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

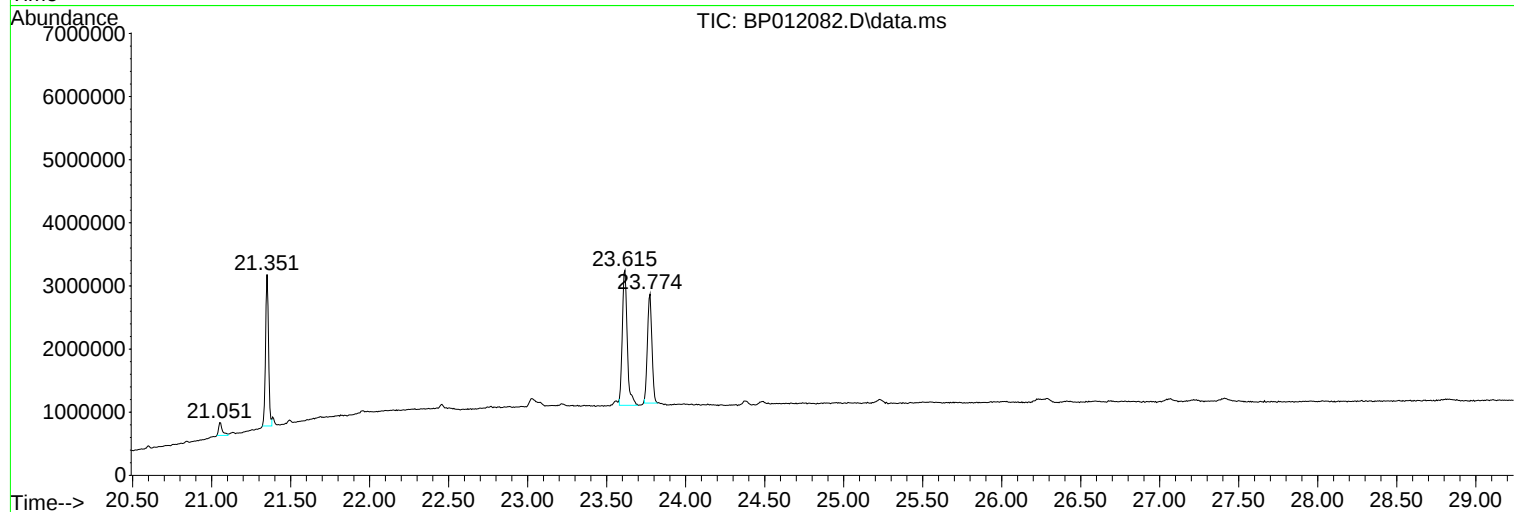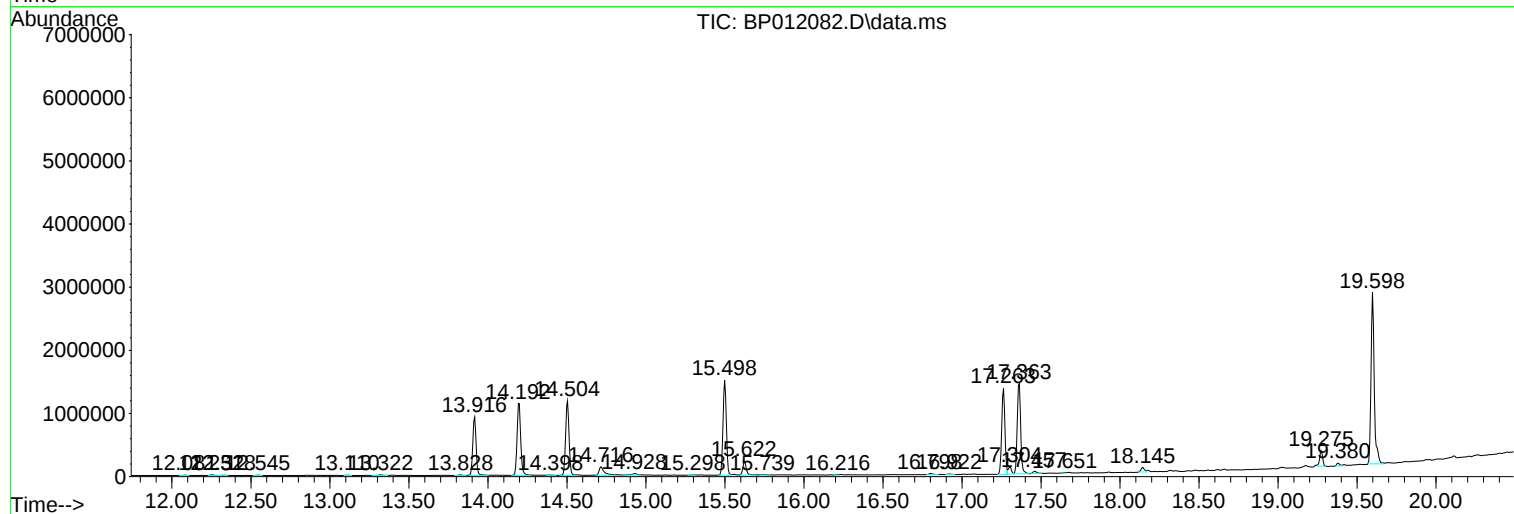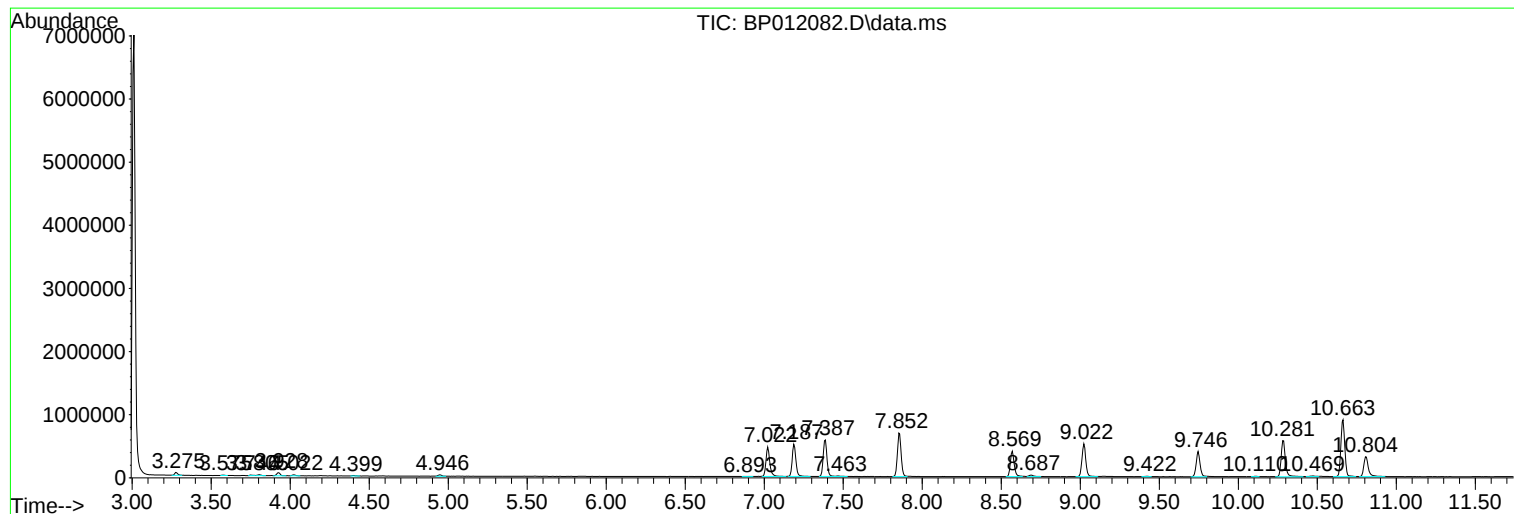

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012082.D
Acq On : 12 Oct 2022 15:44
Operator : CG/JU
Sample : N5024-05
Misc :
ALS Vial : 51 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
C0BF4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Pentadecafluorooctanoic aci... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
21.051	2.14 ng/ul	339522	Chrysene-d12	21.351	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	93
2	Ethanol, 2-(tetradecyloxy)-	258	C16H34O2	002136-70-1	91
3	3-Eicosene, (E)-	280	C20H40	074685-33-9	91
4	9-Eicosene, (E)-	280	C20H40	074685-29-3	83
5	Cyclopentane, (4-octyldodecyl)-	350	C25H50	005638-09-5	83

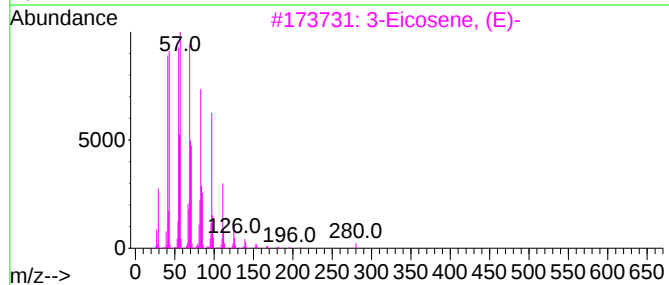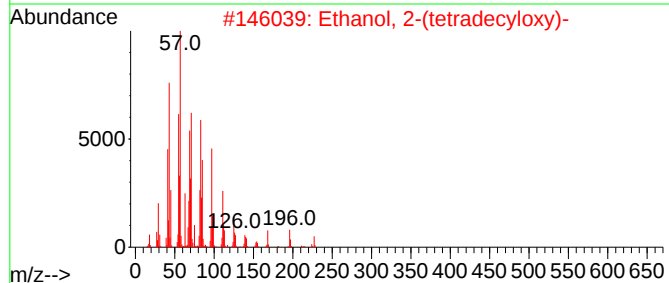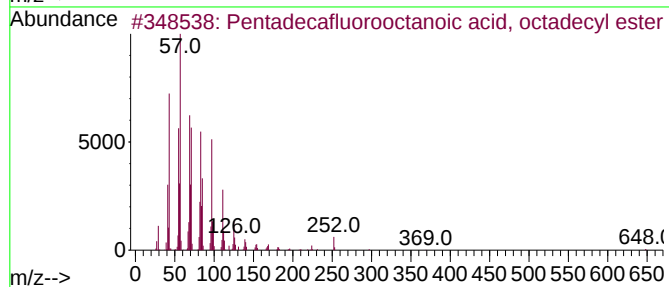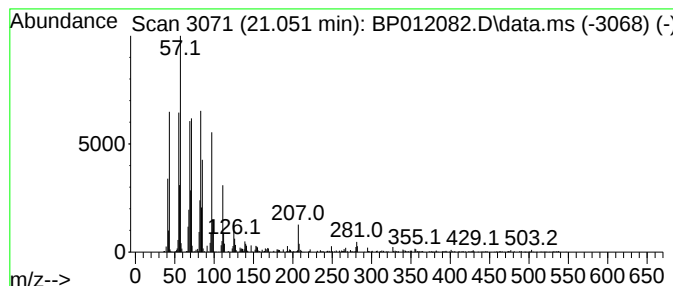

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012082.D
Acq On : 12 Oct 2022 15:44
Operator : CG/JU
Sample : N5024-05
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BF4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Pentadecafluoro...	21.051	2.1	ng/u1	339522	5	21.351	3169810	20.0