

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012090.D
 Acq On : 12 Oct 2022 20:57
 Operator : CG/JU
 Sample : PB148211BL
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK211

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012090.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	46	49	61	rVB	67216	89559	1.66%	0.170%
2	3.699	119	121	140	rBV	741661	1134448	21.00%	2.150%
3	4.022	171	176	180	rBV	18480	26812	0.50%	0.051%
4	7.022	679	686	701	rBV	852302	1391048	25.75%	2.636%
5	7.187	707	714	725	rBV	750239	1185198	21.94%	2.246%
6	7.381	740	747	768	rBV	916173	1500160	27.77%	2.843%
7	7.852	820	827	840	rBV	932127	1491527	27.61%	2.826%
8	8.569	942	949	964	rBV	1033726	1747804	32.35%	3.312%
9	9.022	1018	1026	1044	rBV	767130	1305037	24.16%	2.473%
10	9.746	1140	1149	1163	rBV	594479	1040972	19.27%	1.972%
11	10.281	1233	1240	1262	rBV	942997	1687107	31.23%	3.197%
12	10.657	1296	1304	1317	rBV	1216424	2072043	38.35%	3.926%
13	10.804	1321	1329	1351	rVV	940168	1723889	31.91%	3.266%
14	12.257	1569	1576	1587	rBV2	13756	33503	0.62%	0.063%
15	13.910	1851	1857	1873	rBV	1424317	2064242	38.21%	3.911%
16	14.192	1897	1905	1922	rBV	1882330	2814908	52.10%	5.334%
17	14.498	1950	1957	1972	rBV	1596095	2433779	45.05%	4.612%
18	14.710	1987	1993	2018	rBV	512944	986047	18.25%	1.868%
19	14.916	2024	2028	2033	rVB7	3832	7575	0.14%	0.014%
20	15.492	2118	2126	2141	rBV	2321340	3454594	63.94%	6.546%
21	15.622	2141	2148	2161	rVV	530749	778346	14.41%	1.475%
22	15.739	2164	2168	2172	rVB3	11895	19263	0.36%	0.036%
23	16.286	2257	2261	2266	rBV8	2852	5732	0.11%	0.011%
24	17.257	2420	2426	2435	rBV	1950112	2731690	50.56%	5.176%
25	17.357	2437	2443	2460	rVV	2607234	3707813	68.63%	7.026%
26	19.174	2748	2752	2757	rBV3	33827	51976	0.96%	0.098%
27	19.239	2760	2763	2771	rVV	34840	53948	1.00%	0.102%
28	19.592	2818	2823	2838	rBV	3381880	4646795	86.01%	8.805%
29	21.345	3117	3121	3132	rBV	2618732	3391938	62.78%	6.427%
30	23.610	3499	3506	3517	rBV	2727071	5402526	100.00%	10.237%
31	23.762	3526	3532	3540	rBV2	1891962	3795200	70.25%	7.191%




Sum of corrected areas: 52775479

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012090.D
Acq On : 12 Oct 2022 20:57
Operator : CG/JU
Sample : PB148211BL
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK211

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

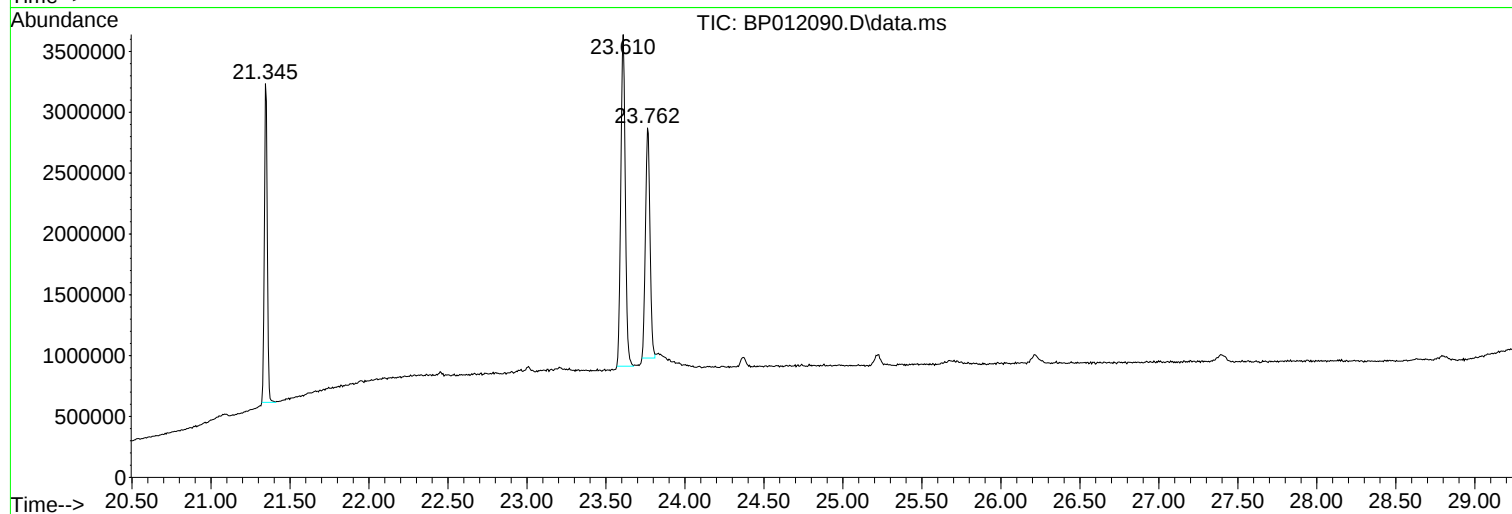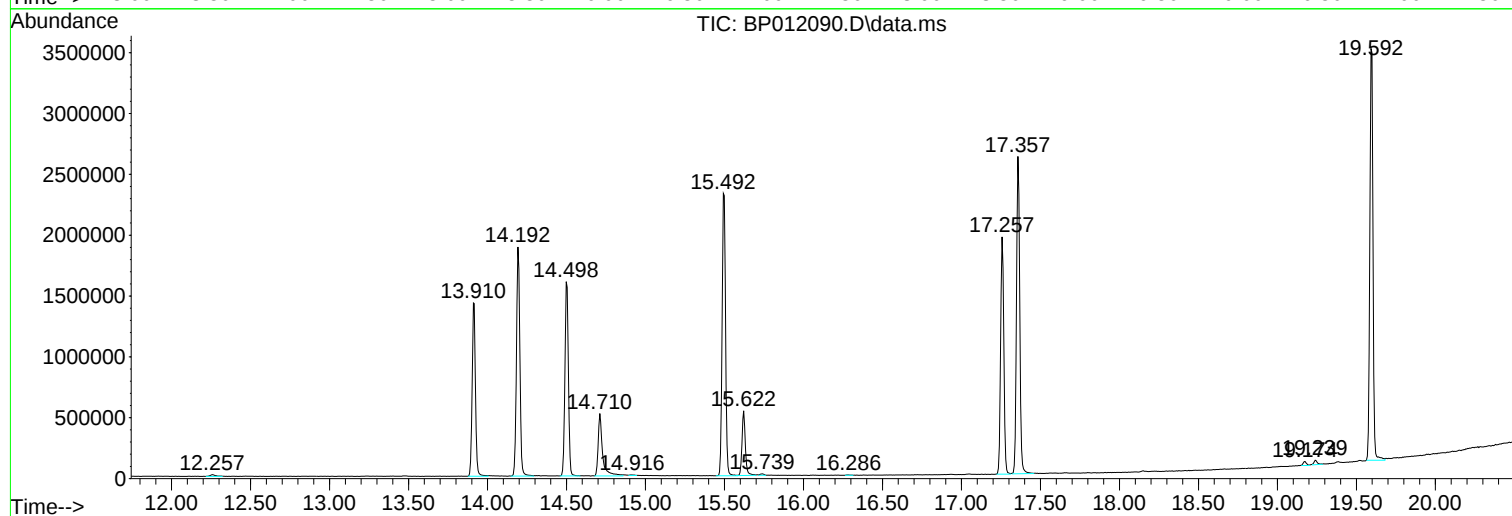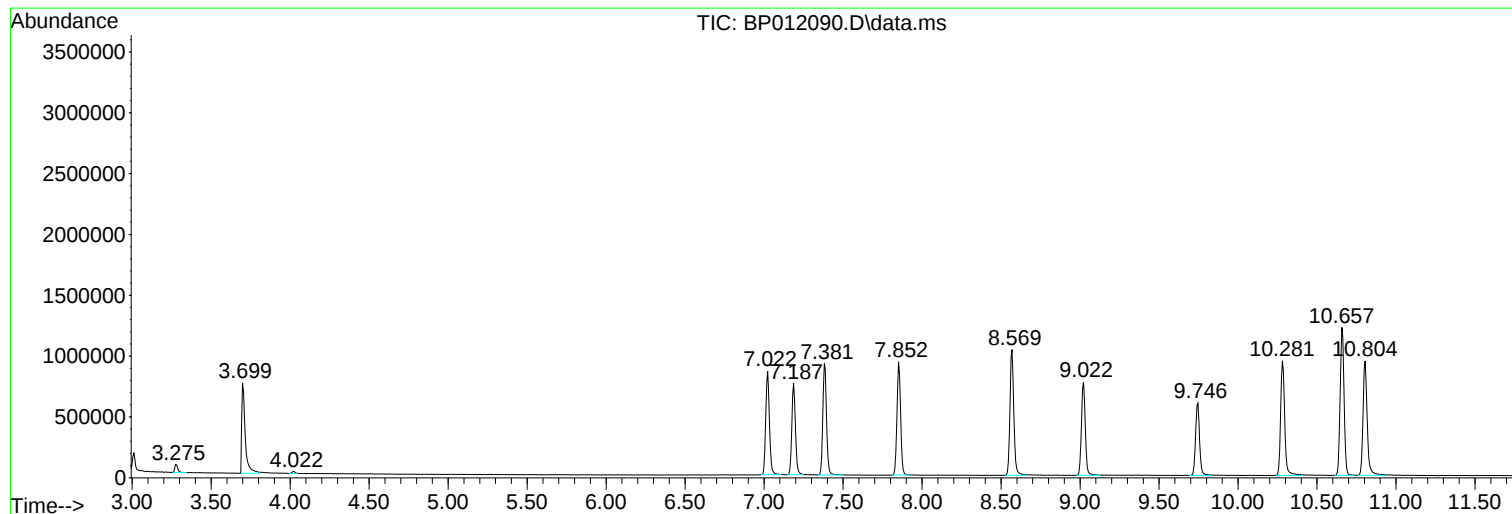

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012090.D
Acq On : 12 Oct 2022 20:57
Operator : CG/JU
Sample : PB148211BL
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK211

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012090.D
Acq On : 12 Oct 2022 20:57
Operator : CG/JU
Sample : PB148211BL
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK211

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc