

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012091.D
 Acq On : 12 Oct 2022 21:32
 Operator : CG/JU
 Sample : PB148213BL
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK213

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012091.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	46	49	56	rVB	72826	91651	1.44%	0.154%
2	3.699	119	121	140	rBV	843427	1265161	19.92%	2.123%
3	4.023	172	176	181	rVB	15148	22818	0.36%	0.038%
4	7.022	679	686	700	rBV	981308	1597599	25.16%	2.681%
5	7.187	707	714	727	rBV	843140	1360608	21.43%	2.283%
6	7.381	740	747	763	rBV	1022312	1707684	26.89%	2.866%
7	7.852	819	827	837	rBV	815557	1322151	20.82%	2.219%
8	8.569	940	949	962	rBV	1194495	2014199	31.72%	3.380%
9	9.022	1018	1026	1039	rBV	876634	1493728	23.52%	2.507%
10	9.740	1141	1148	1166	rBV	685541	1209532	19.05%	2.030%
11	10.281	1232	1240	1258	rBV	1105477	1975820	31.12%	3.316%
12	10.657	1297	1304	1319	rBV	1090703	1885835	29.70%	3.165%
13	10.805	1321	1329	1348	rBV	1107515	2048832	32.27%	3.438%
14	12.257	1570	1576	1588	rBV2	16451	42399	0.67%	0.071%
15	13.393	1761	1769	1776	rBV2	3496	9020	0.14%	0.015%
16	13.910	1850	1857	1870	rBV	1760972	2557979	40.28%	4.292%
17	14.193	1896	1905	1925	rBV	2266426	3480094	54.81%	5.840%
18	14.498	1950	1957	1971	rBV	1617987	2325017	36.62%	3.902%
19	14.710	1983	1993	2015	rBV	703401	1286314	20.26%	2.159%
20	15.498	2120	2127	2139	rBV	2931448	4322806	68.08%	7.254%
21	15.622	2141	2148	2161	rVV	708130	1023205	16.11%	1.717%
22	15.734	2164	2167	2173	rVB3	13711	22128	0.35%	0.037%
23	17.257	2420	2426	2436	rBV	1959847	2722363	42.87%	4.568%
24	17.357	2436	2443	2460	rVV2	3311132	4732529	74.53%	7.941%
25	18.145	2575	2577	2584	rBV8	7537	10952	0.17%	0.018%
26	19.169	2748	2751	2756	rVB	42143	52898	0.83%	0.089%
27	19.239	2760	2763	2769	rVB	39304	57579	0.91%	0.097%
28	19.592	2818	2823	2830	rBV	4264303	5789465	91.18%	9.715%
29	21.345	3116	3121	3130	rBV	2561366	3331958	52.47%	5.591%
30	23.610	3499	3506	3516	rVB2	3173858	6349783	100.00%	10.655%
31	23.763	3526	3532	3544	rVB2	1632029	3480344	54.81%	5.840%




Sum of corrected areas: 59592451

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012091.D
Acq On : 12 Oct 2022 21:32
Operator : CG/JU
Sample : PB148213BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK213

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

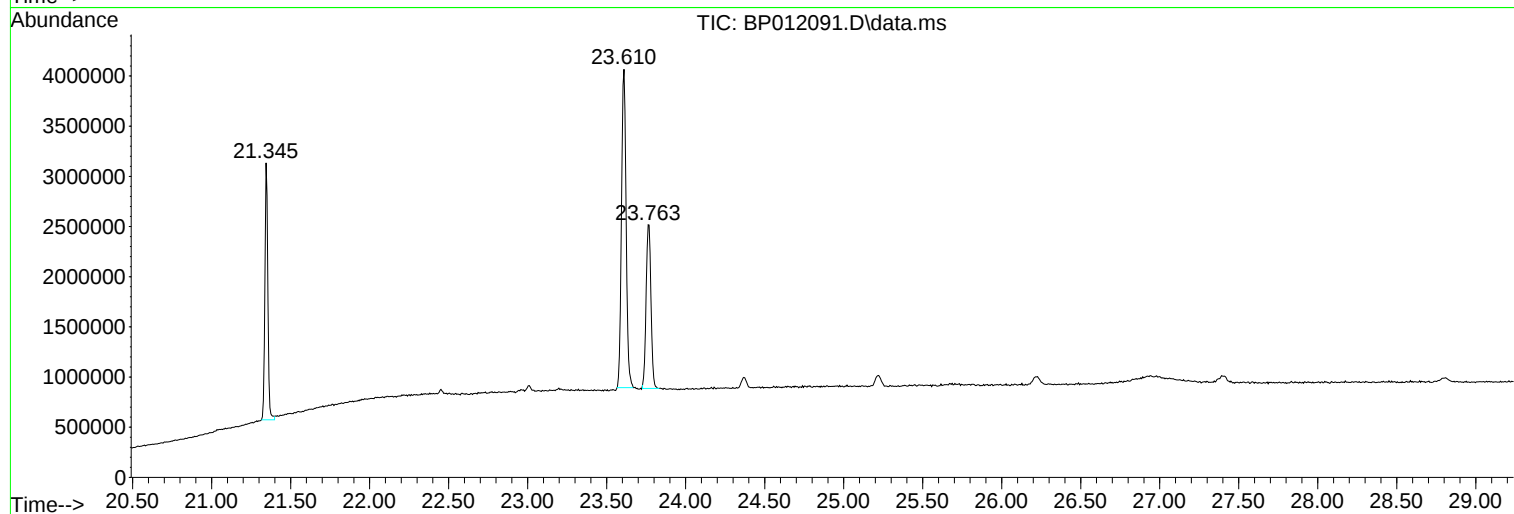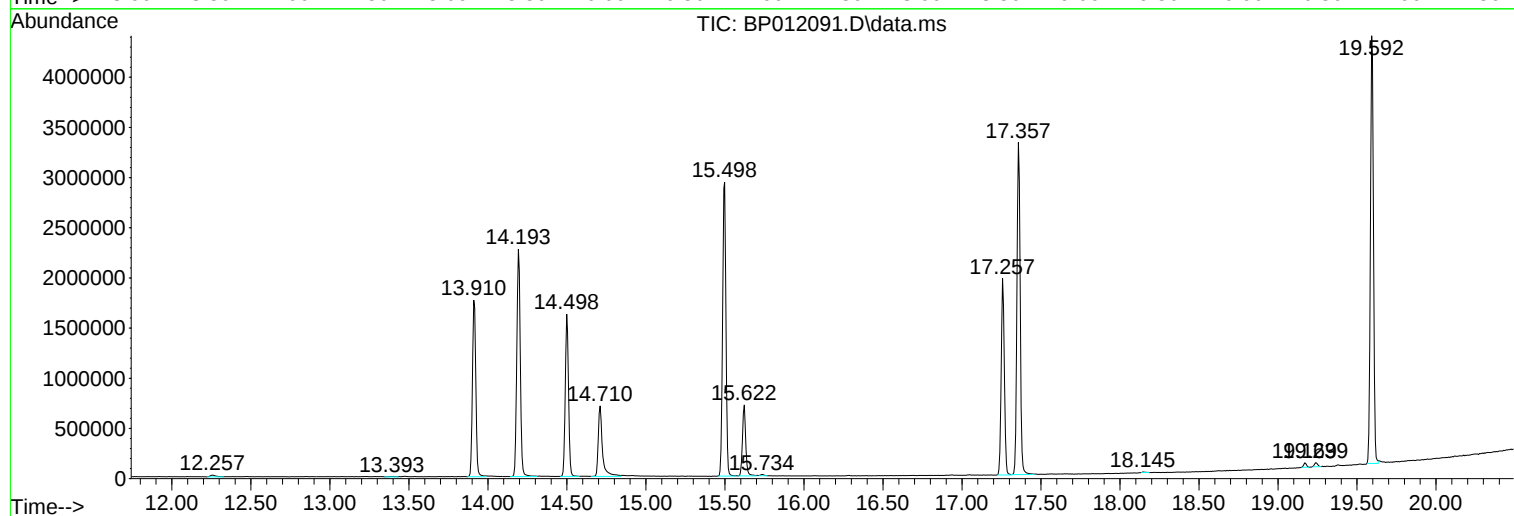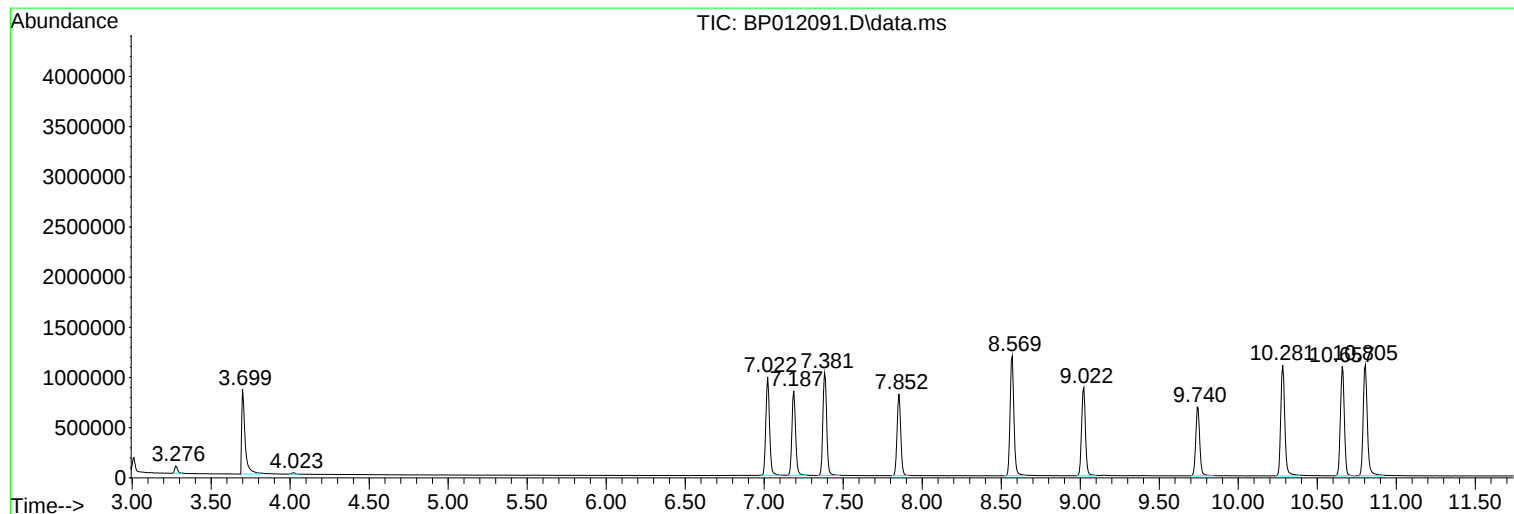

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012091.D
Acq On : 12 Oct 2022 21:32
Operator : CG/JU
Sample : PB148213BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK213

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012091.D
Acq On : 12 Oct 2022 21:32
Operator : CG/JU
Sample : PB148213BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK213

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc