

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012099.D
 Acq On : 13 Oct 2022 02:08
 Operator : CG/JU
 Sample : N5024-10
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012099.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	46	49	57	rVB	38049	49570	1.22%	0.119%
2	3.805	135	139	144	rVB	16663	21262	0.52%	0.051%
3	3.923	154	159	164	rVB2	43449	65786	1.62%	0.159%
4	4.017	171	175	182	rVB	32668	46795	1.15%	0.113%
5	4.399	238	240	244	rVB4	8254	10119	0.25%	0.024%
6	4.575	268	270	278	rVB9	4611	6934	0.17%	0.017%
7	4.946	326	333	342	rVB2	21406	43136	1.06%	0.104%
8	5.475	418	423	430	rBV9	4400	10725	0.26%	0.026%
9	5.540	432	434	442	rVB7	4233	8751	0.22%	0.021%
10	5.852	483	487	493	rVB8	7576	13054	0.32%	0.031%
11	7.022	679	686	702	rVB	256430	454947	11.20%	1.097%
12	7.181	707	713	729	rVB	470629	787579	19.39%	1.898%
13	7.381	739	747	757	rBV	417996	676250	16.65%	1.630%
14	7.464	757	761	764	rVV2	11066	16037	0.39%	0.039%
15	7.669	790	796	801	rVB6	4552	7941	0.20%	0.019%
16	7.852	817	827	837	rBV	912031	1512397	37.23%	3.646%
17	8.569	942	949	960	rBV2	99009	189128	4.66%	0.456%
18	8.687	963	969	980	rVB	29107	57584	1.42%	0.139%
19	9.016	1019	1025	1032	rBV	497892	841573	20.71%	2.029%
20	9.069	1032	1034	1042	rVB3	17229	26526	0.65%	0.064%
21	9.422	1089	1094	1102	rVB5	13010	25983	0.64%	0.063%
22	9.740	1141	1148	1160	rBV	360457	629134	15.49%	1.517%
23	10.281	1232	1240	1256	rBV	381097	718747	17.69%	1.733%
24	10.658	1294	1304	1310	rBV	1269079	2158243	53.12%	5.202%
25	10.705	1310	1312	1322	rVB	63480	98008	2.41%	0.236%
26	10.810	1322	1330	1346	rBV	88237	194264	4.78%	0.468%
27	12.075	1536	1545	1549	rBV8	8014	14070	0.35%	0.034%
28	12.252	1567	1575	1581	rBV2	10930	21170	0.52%	0.051%
29	12.322	1581	1587	1593	rVV	17950	31825	0.78%	0.077%
30	12.540	1620	1624	1631	rVB	17599	28911	0.71%	0.070%
31	12.857	1672	1678	1680	rBV7	3821	6711	0.17%	0.016%
32	13.316	1749	1756	1765	rBV2	16592	42921	1.06%	0.103%
33	13.393	1765	1769	1775	rVB6	6055	10367	0.26%	0.025%
34	13.663	1811	1815	1816	rBV4	4871	6215	0.15%	0.015%
35	13.681	1816	1818	1822	rVB5	5089	6348	0.16%	0.015%
36	13.822	1836	1842	1847	rBV5	16949	30564	0.75%	0.074%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012099.D
 Acq On : 13 Oct 2022 02:08
 Operator : CG/JU
 Sample : N5024-10
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

37	13.910	1851	1857	1873	rVB	1082355	1444847	35.56%	3.483%
38	14.057	1878	1882	1885	rVV3	8646	15110	0.37%	0.036%
39	14.087	1885	1887	1892	rVB5	4647	6027	0.15%	0.015%
40	14.193	1898	1905	1919	rBV	1211485	1963458	48.33%	4.733%
41	14.393	1934	1939	1943	rVB	12881	17170	0.42%	0.041%
42	14.498	1948	1957	1964	rBV	1705097	2504564	61.65%	6.037%
43	14.563	1964	1968	1975	rVB	23749	40819	1.00%	0.098%
44	14.640	1975	1981	1984	rBV6	5677	11287	0.28%	0.027%
45	14.740	1991	1998	2006	rBV10	11506	34095	0.84%	0.082%
46	14.898	2020	2025	2029	rBV	49999	72529	1.79%	0.175%
47	15.010	2042	2044	2051	rVB8	4539	6590	0.16%	0.016%
48	15.116	2058	2062	2069	rVB9	6670	11084	0.27%	0.027%
49	15.293	2087	2092	2095	rBV2	12028	18479	0.45%	0.045%
50	15.346	2097	2101	2106	rVB	16115	23255	0.57%	0.056%
51	15.493	2120	2126	2133	rBV	1617449	2346407	57.75%	5.656%
52	15.551	2133	2136	2143	rVB	21094	31931	0.79%	0.077%
53	15.622	2143	2148	2155	rBV	74984	115498	2.84%	0.278%
54	15.751	2163	2170	2174	rVB8	9017	20364	0.50%	0.049%
55	15.845	2181	2186	2192	rBV	19586	32433	0.80%	0.078%
56	15.993	2207	2211	2218	rVB	16451	30857	0.76%	0.074%
57	16.081	2222	2226	2233	rVB6	7055	11943	0.29%	0.029%
58	16.157	2233	2239	2244	rBV3	20931	36436	0.90%	0.088%
59	16.210	2244	2248	2250	rBV3	23785	34716	0.85%	0.084%
60	16.792	2343	2347	2350	rBV5	16244	25157	0.62%	0.061%
61	16.910	2362	2367	2375	rBV	76136	118873	2.93%	0.287%
62	16.987	2377	2380	2381	rVV3	9130	11093	0.27%	0.027%
63	17.004	2381	2383	2387	rVV	19110	23643	0.58%	0.057%
64	17.075	2389	2395	2403	rVB2	34781	68160	1.68%	0.164%
65	17.257	2419	2426	2430	rBV	1880484	2685687	66.11%	6.474%
66	17.298	2430	2433	2438	rVV	841524	1141090	28.09%	2.751%
67	17.357	2438	2443	2454	rVV	1406327	2197197	54.08%	5.296%
68	17.457	2457	2460	2469	rVB8	25639	44222	1.09%	0.107%
69	17.669	2492	2496	2506	rVB	45600	71684	1.76%	0.173%
70	17.751	2507	2510	2512	rVV3	13032	15467	0.38%	0.037%
71	17.781	2512	2515	2522	rVB4	13476	19808	0.49%	0.048%
72	17.928	2536	2540	2544	rBV6	16699	27582	0.68%	0.066%
73	18.128	2569	2574	2578	rBV	73064	137540	3.39%	0.332%
74	18.169	2578	2581	2586	rVB	83005	124355	3.06%	0.300%
75	18.310	2600	2605	2609	rBV2	59657	108414	2.67%	0.261%
76	18.351	2609	2612	2618	rVB	44735	60751	1.50%	0.146%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012099.D
 Acq On : 13 Oct 2022 02:08
 Operator : CG/JU
 Sample : N5024-10
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BP9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

77	18.422	2621	2624	2628	rBV4	17996	25827	0.64%	0.062%
78	18.610	2652	2656	2659	rBV	57340	79568	1.96%	0.192%
79	18.651	2659	2663	2669	rVB	88846	122040	3.00%	0.294%
80	19.016	2722	2725	2730	rBV3	36400	59442	1.46%	0.143%
81	19.151	2744	2748	2757	rBV2	80633	167263	4.12%	0.403%
82	19.269	2763	2768	2774	rVB	1363545	1741166	42.86%	4.197%
83	19.592	2818	2823	2826	rBV	2115973	3089246	76.04%	7.447%
84	19.622	2826	2828	2836	rVB	1153071	1275437	31.39%	3.074%
85	21.045	3066	3070	3073	rBV2	317078	419724	10.33%	1.012%
86	21.345	3115	3121	3125	rBV	2828259	4062759	100.00%	9.793%
87	21.380	3125	3127	3135	rVB	496857	613982	15.11%	1.480%
88	23.604	3500	3505	3510	rBV2	1006214	1882306	46.33%	4.537%
89	23.763	3526	3532	3539	rBV2	1711725	3366803	82.87%	8.116%



Sum of corrected areas: 41485760

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012099.D
Acq On : 13 Oct 2022 02:08
Operator : CG/JU
Sample : N5024-10
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BP9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

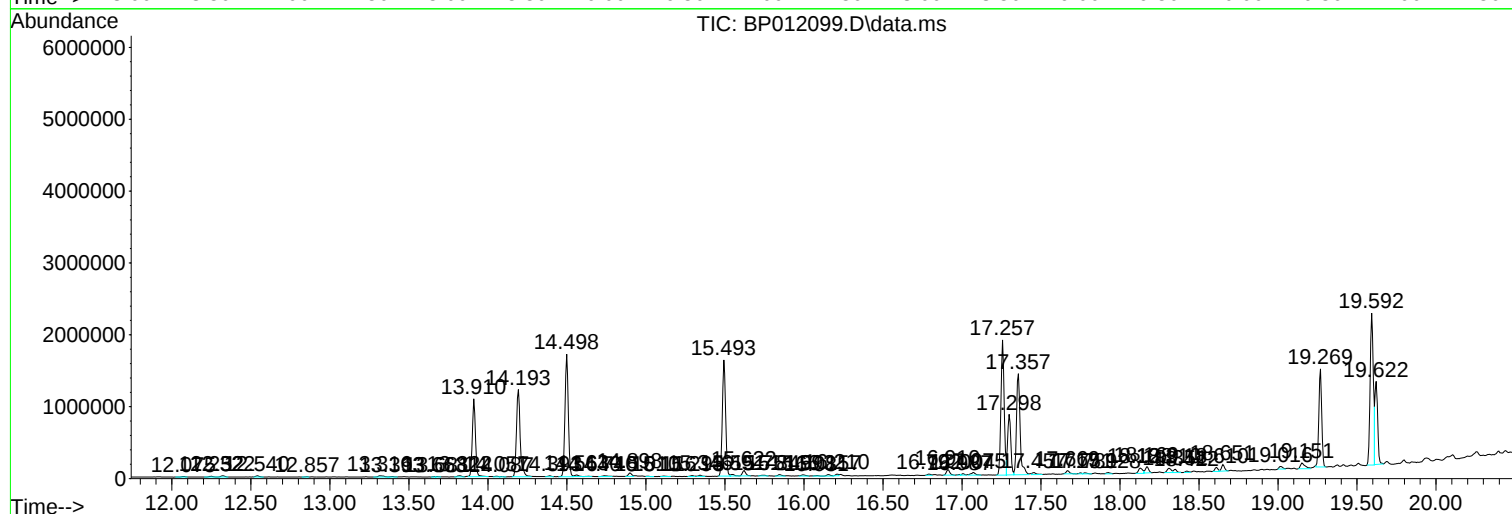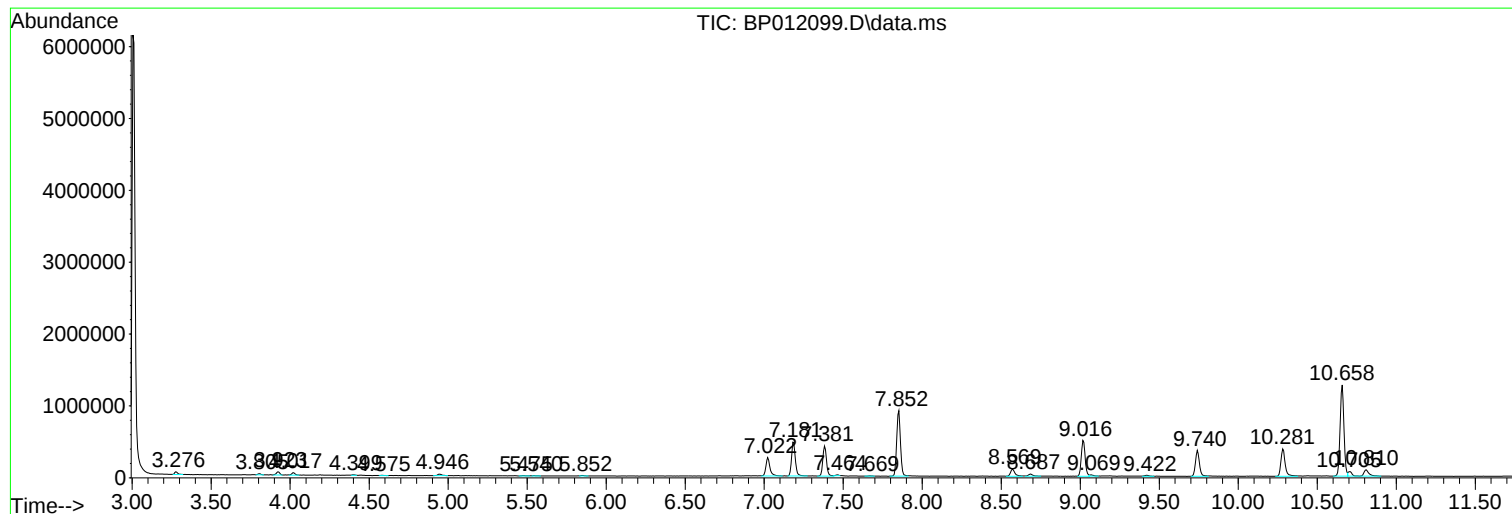

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012099.D
Acq On : 13 Oct 2022 02:08
Operator : CG/JU
Sample : N5024-10
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BP9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Pentadecafluorooctanoic aci... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.045	2.07 ng/ul	419724	Chrysene-d12	21.345

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	86
2			Ethanol, 2-(tetradecyloxy)-	258	C16H34O2	002136-70-1	70
3			1-Hexadecanesulfonyl chloride	324	C16H33ClO2S	038775-38-1	70
4			Octadecyl trifluoroacetate	366	C20H37F3O2	079392-43-1	64
5			Heptafluorobutyric acid, n-octad...	466	C22H37F7O2	000400-57-7	64

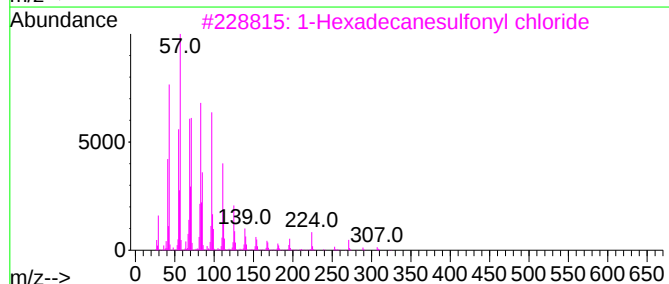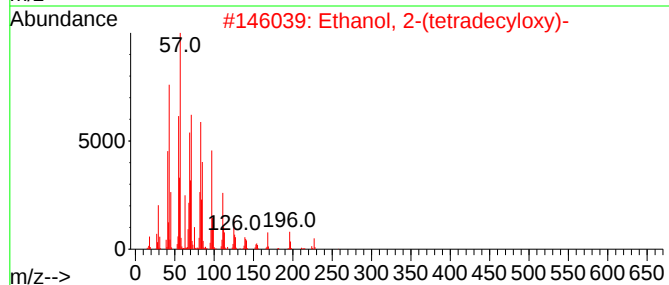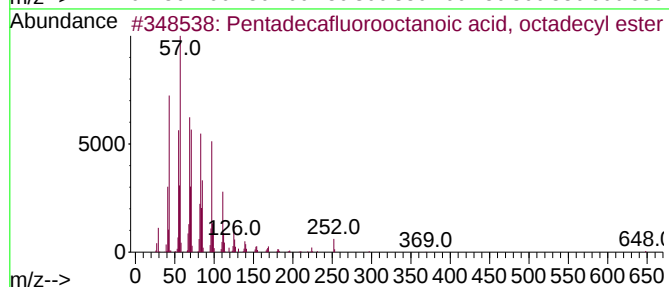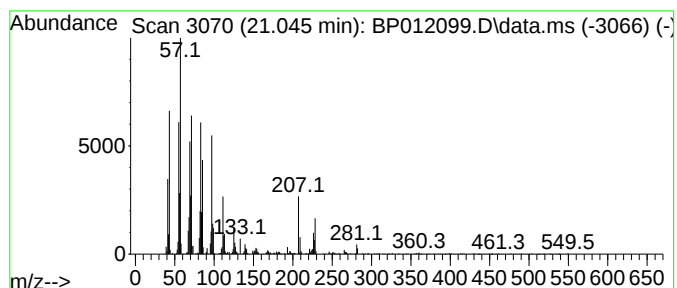

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012099.D
Acq On : 13 Oct 2022 02:08
Operator : CG/JU
Sample : N5024-10
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BP9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Pentadecafluoro...	21.045	2.1	ng/u1	419724	5	21.345	4062760	20.0