

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012103.D
 Acq On : 13 Oct 2022 04:25
 Operator : CG/JU
 Sample : N5026-02
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COBX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012103.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	45	49	58	rVB	48802	64599	0.91%	0.107%
2	3.705	120	122	136	rBV	210671	334176	4.70%	0.556%
3	3.922	154	159	164	rVB	25966	39708	0.56%	0.066%
4	4.017	171	175	181	rVB	21777	29697	0.42%	0.049%
5	4.393	237	239	246	rVB7	6504	10878	0.15%	0.018%
6	7.022	679	686	701	rVB	210440	392020	5.51%	0.652%
7	7.181	706	713	730	rBV	839005	1383271	19.44%	2.300%
8	7.381	739	747	758	rBV	816653	1319031	18.54%	2.193%
9	7.852	819	827	835	rBV	1018382	1665448	23.41%	2.769%
10	7.916	836	838	845	rVB4	8527	12391	0.17%	0.021%
11	8.563	938	948	965	rBV	589115	1019039	14.32%	1.694%
12	9.016	1018	1025	1038	rBV	902424	1552981	21.82%	2.582%
13	9.187	1051	1054	1061	rVB8	4905	9619	0.14%	0.016%
14	9.416	1086	1093	1097	rBV	18744	30290	0.43%	0.050%
15	9.740	1137	1148	1163	rBV	694786	1194404	16.79%	1.986%
16	10.281	1231	1240	1256	rBV	1037182	1834635	25.78%	3.050%
17	10.457	1263	1270	1276	rBV5	13496	32834	0.46%	0.055%
18	10.657	1295	1304	1319	rBV	1364761	2370965	33.32%	3.942%
19	10.799	1321	1328	1347	rBV	713694	1324644	18.62%	2.202%
20	12.075	1539	1545	1550	rBV6	6294	10735	0.15%	0.018%
21	12.246	1570	1574	1581	rBV2	17186	31310	0.44%	0.052%
22	13.316	1751	1756	1760	rBV	18135	23470	0.33%	0.039%
23	13.457	1777	1780	1789	rVB9	4256	9177	0.13%	0.015%
24	13.910	1850	1857	1871	rBV	1913541	2636560	37.05%	4.384%
25	14.192	1893	1905	1923	rBV	2263805	3485599	48.98%	5.795%
26	14.392	1935	1939	1945	rVB5	7232	11563	0.16%	0.019%
27	14.498	1949	1957	1972	rVV	1943450	2819412	39.62%	4.688%
28	14.716	1989	1994	2009	rBV	77015	203191	2.86%	0.338%
29	14.916	2024	2028	2035	rVB7	9333	21121	0.30%	0.035%
30	15.492	2119	2126	2141	rBV	3069433	4365770	61.35%	7.258%
31	15.616	2141	2147	2159	rBV	703209	1017858	14.30%	1.692%
32	15.734	2164	2167	2176	rVB2	15852	27792	0.39%	0.046%
33	16.281	2256	2260	2265	rVB7	6485	9248	0.13%	0.015%
34	17.257	2419	2426	2436	rBV	2264353	3186972	44.79%	5.299%
35	17.357	2436	2443	2458	rVV	3375481	4839379	68.01%	8.046%
36	17.922	2537	2539	2544	rVB6	9784	11491	0.16%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012103.D
 Acq On : 13 Oct 2022 04:25
 Operator : CG/JU
 Sample : N5026-02
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BX8

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

37	18.139	2571	2576	2585	rBV	172210	275574	3.87%	0.458%
38	19.169	2748	2751	2756	rVB	46927	54046	0.76%	0.090%
39	19.239	2759	2763	2775	rBV	60272	124700	1.75%	0.207%
40	19.375	2782	2786	2795	rBV	153455	245076	3.44%	0.407%
41	19.592	2817	2823	2835	rBV	4741586	6187279	86.95%	10.287%
42	21.045	3067	3070	3075	rBV2	143951	193391	2.72%	0.322%
43	21.345	3116	3121	3130	rBV	3253025	4100432	57.63%	6.817%
44	23.604	3499	3505	3518	rVB2	3471642	7115648	100.00%	11.830%
45	23.763	3526	3532	3546	rVB2	2217428	4519701	63.52%	7.514%




Sum of corrected areas: 60147125

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012103.D
Acq On : 13 Oct 2022 04:25
Operator : CG/JU
Sample : N5026-02
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

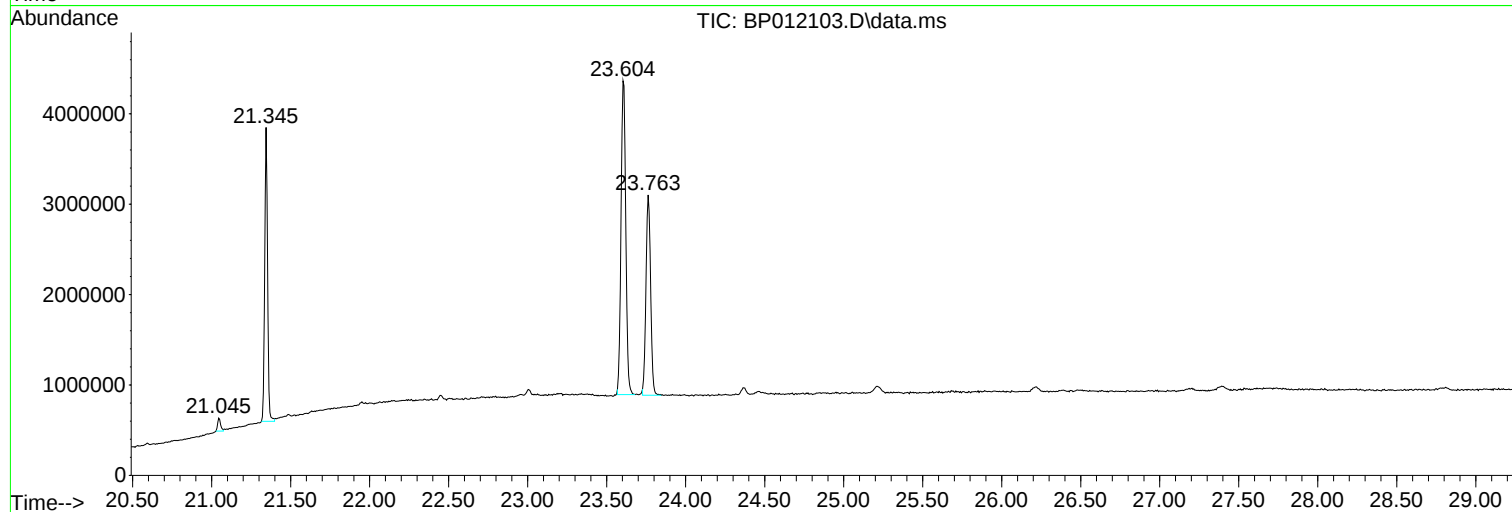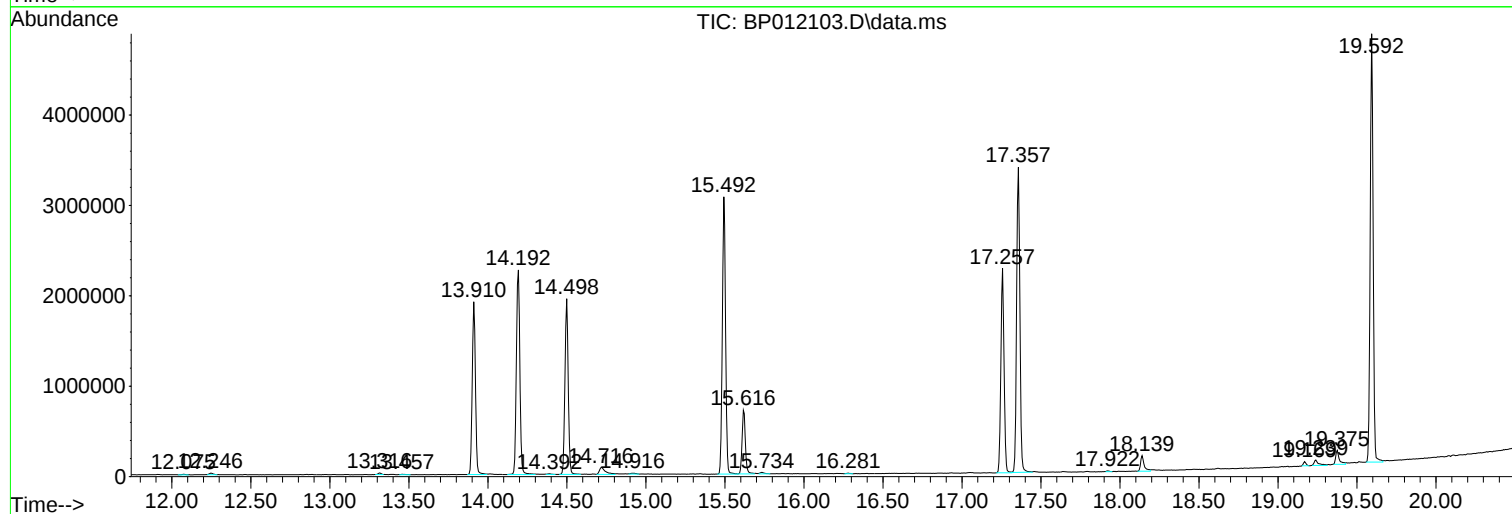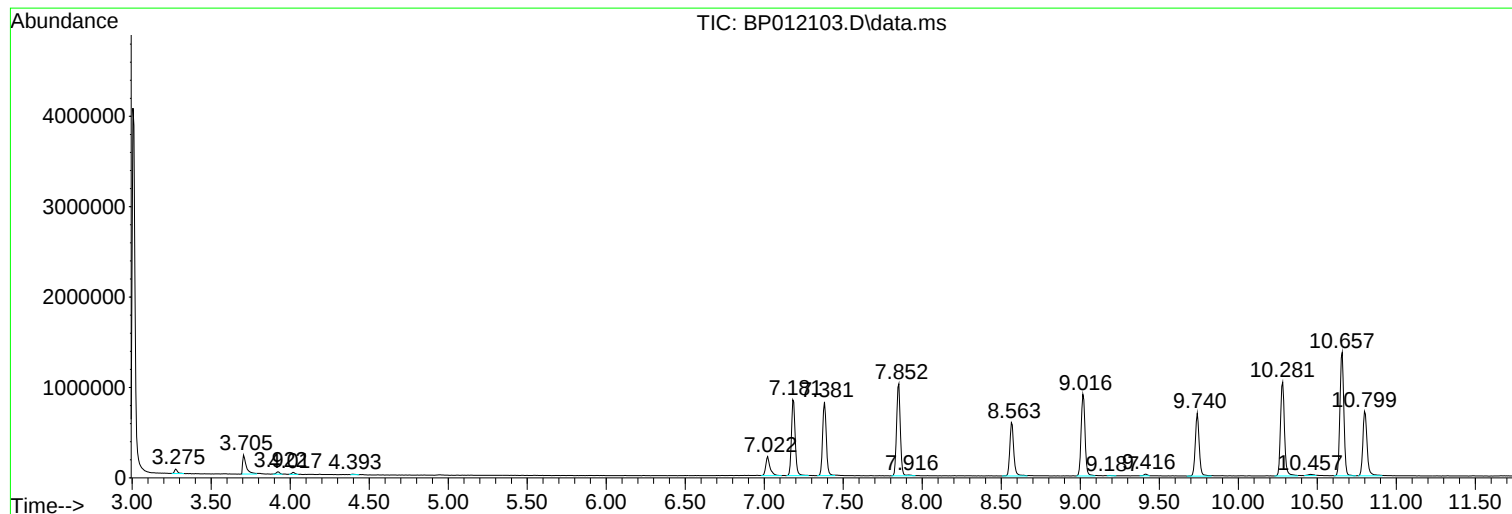

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012103.D
Acq On : 13 Oct 2022 04:25
Operator : CG/JU
Sample : N5026-02
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012103.D
Acq On : 13 Oct 2022 04:25
Operator : CG/JU
Sample : N5026-02
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc