

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012104.D
 Acq On : 13 Oct 2022 04:59
 Operator : CG/JU
 Sample : N5026-08
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COBX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012104.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	45	49	57	rVB	43202	56676	0.80%	0.100%
2	3.705	120	122	134	rBV	196393	306422	4.33%	0.543%
3	3.922	154	159	165	rVB	25870	37814	0.53%	0.067%
4	4.017	171	175	185	rVB	71850	103020	1.46%	0.183%
5	4.393	236	239	245	rVB8	5662	10264	0.15%	0.018%
6	4.958	329	335	342	rBV2	35732	61620	0.87%	0.109%
7	7.022	680	686	701	rVB	188844	363426	5.14%	0.644%
8	7.181	706	713	728	rBV	753598	1228331	17.36%	2.176%
9	7.381	740	747	758	rBV	735590	1188057	16.79%	2.105%
10	7.846	820	826	835	rBV	786981	1309992	18.51%	2.321%
11	7.911	835	837	846	rVB4	7610	15686	0.22%	0.028%
12	8.563	941	948	966	rBV	554771	957372	13.53%	1.696%
13	9.016	1018	1025	1044	rBV	821832	1395894	19.73%	2.473%
14	9.416	1088	1093	1098	rVB	14706	21540	0.30%	0.038%
15	9.740	1139	1148	1164	rBV	614264	1060750	14.99%	1.879%
16	10.275	1232	1239	1258	rBV	929948	1702596	24.06%	3.017%
17	10.457	1264	1270	1284	rVB7	7940	24459	0.35%	0.043%
18	10.657	1296	1304	1318	rBV	1097238	1880761	26.58%	3.332%
19	10.799	1321	1328	1345	rBV	580779	1101244	15.56%	1.951%
20	11.916	1514	1518	1523	rVB8	4701	7506	0.11%	0.013%
21	12.081	1538	1546	1551	rBV8	3836	8361	0.12%	0.015%
22	12.169	1554	1561	1566	rBV6	4268	8089	0.11%	0.014%
23	12.246	1568	1574	1582	rBV	16322	30287	0.43%	0.054%
24	13.316	1748	1756	1764	rBV2	14366	26920	0.38%	0.048%
25	13.393	1764	1769	1772	rVV6	4170	7784	0.11%	0.014%
26	13.469	1775	1782	1790	rVB6	5104	12472	0.18%	0.022%
27	13.910	1850	1857	1871	rBV	1779283	2584925	36.53%	4.580%
28	14.193	1898	1905	1922	rVB	2246017	3325688	47.00%	5.892%
29	14.387	1936	1938	1944	rVB2	7341	8922	0.13%	0.016%
30	14.498	1950	1957	1967	rBV	1586399	2358512	33.33%	4.179%
31	14.716	1988	1994	2011	rBV	93828	233251	3.30%	0.413%
32	14.916	2024	2028	2037	rVB6	12424	22132	0.31%	0.039%
33	15.340	2097	2100	2105	rVB7	7142	9276	0.13%	0.016%
34	15.492	2119	2126	2141	rBV	3022572	4387415	62.00%	7.773%
35	15.616	2141	2147	2162	rVV	785007	1092445	15.44%	1.936%
36	15.734	2162	2167	2171	rVB3	13702	22713	0.32%	0.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012104.D
 Acq On : 13 Oct 2022 04:59
 Operator : CG/JU
 Sample : N5026-08
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

37	16.281	2258	2260	2265	rVB6	8083	8571	0.12%	0.015%
38	16.657	2320	2324	2332	rBV9	4257	8076	0.11%	0.014%
39	17.257	2419	2426	2435	rBV	2012670	2841645	40.16%	5.035%
40	17.357	2436	2443	2456	rVV	3327277	4958872	70.07%	8.786%
41	18.139	2572	2576	2586	rBV	187474	282138	3.99%	0.500%
42	19.169	2748	2751	2756	rVB3	43195	54222	0.77%	0.096%
43	19.239	2759	2763	2769	rBV	63687	106895	1.51%	0.189%
44	19.375	2782	2786	2794	rBV	157055	244477	3.45%	0.433%
45	19.592	2817	2823	2836	rBV	4730282	6372138	90.05%	11.290%
46	21.045	3067	3070	3075	rBV	252191	302685	4.28%	0.536%
47	21.345	3116	3121	3127	rBV	2739173	3495522	49.40%	6.193%
48	23.604	3498	3505	3518	rBV2	3512369	7076551	100.00%	12.538%
49	23.763	3526	3532	3541	rVB2	1811524	3717429	52.53%	6.586%




Sum of corrected areas: 56441843

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012104.D
Acq On : 13 Oct 2022 04:59
Operator : CG/JU
Sample : N5026-08
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BX6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

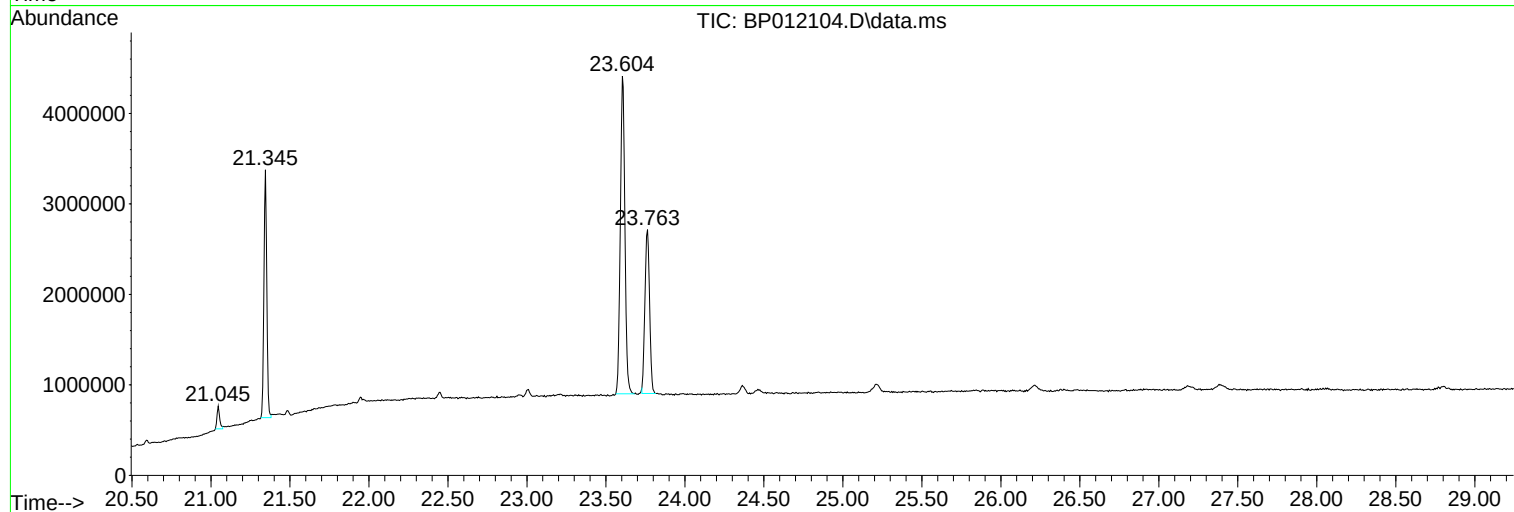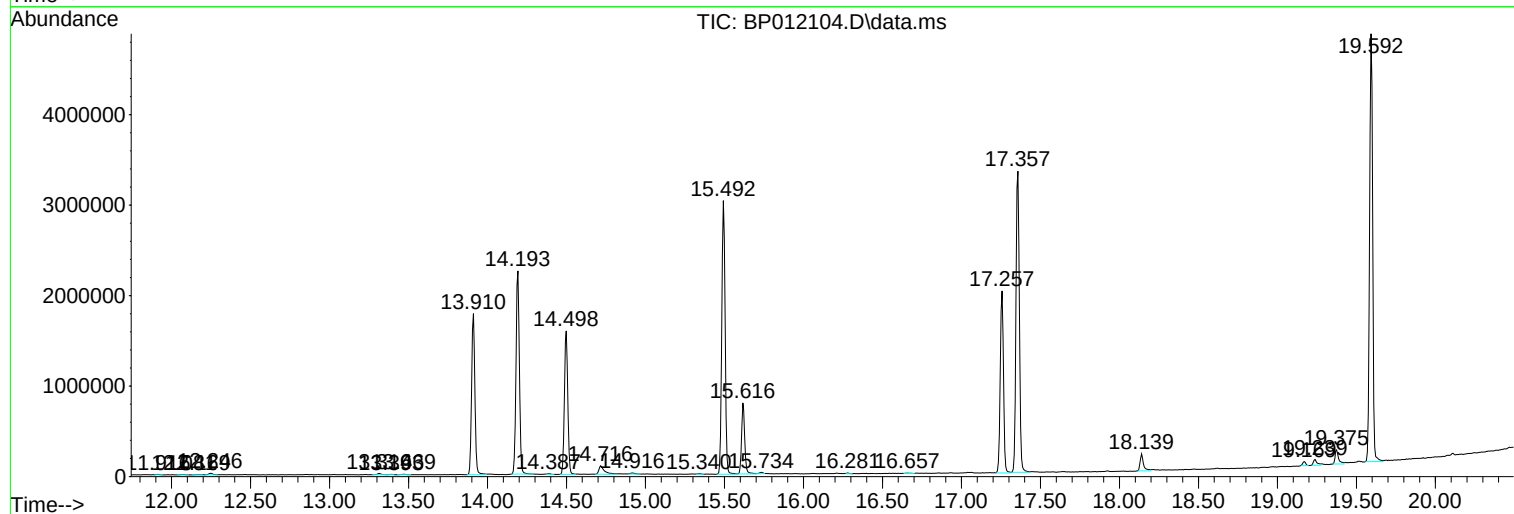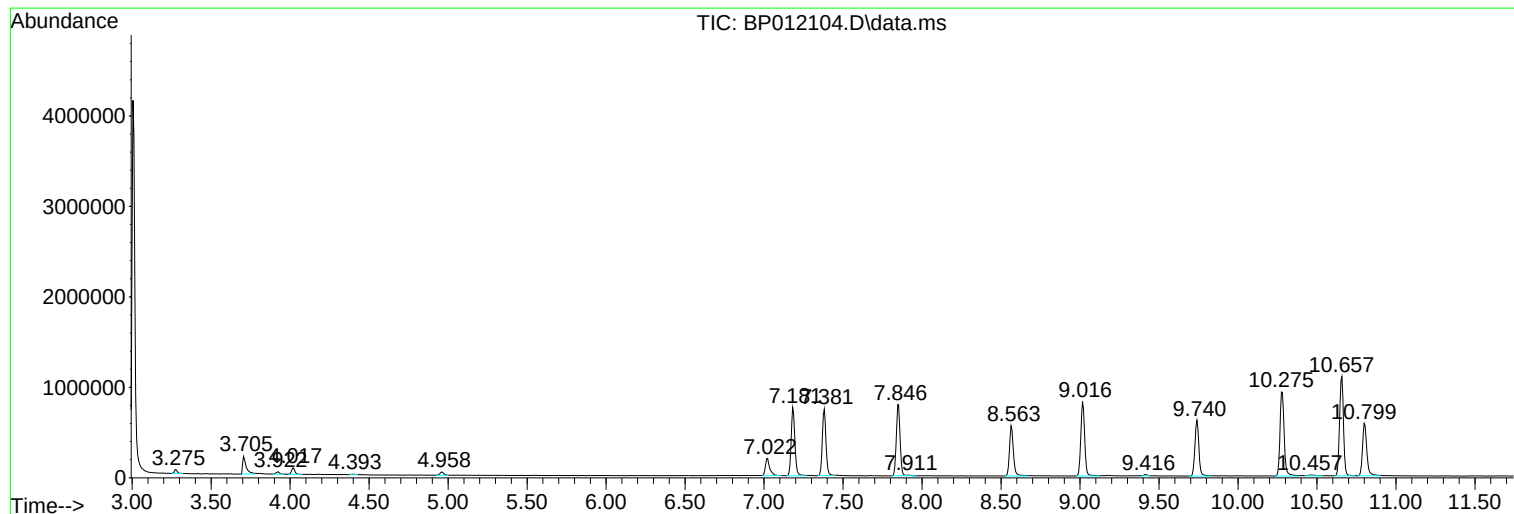

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012104.D
Acq On : 13 Oct 2022 04:59
Operator : CG/JU
Sample : N5026-08
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BX6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012104.D
Acq On : 13 Oct 2022 04:59
Operator : CG/JU
Sample : N5026-08
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BX6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc