

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012105.D
 Acq On : 13 Oct 2022 05:33
 Operator : CG/JU
 Sample : N5026-06
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COBX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012105.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	45	49	54	rBV	46050	54091	0.71%	0.090%
2	3.705	120	122	138	rBV	188012	298490	3.90%	0.498%
3	3.923	155	159	164	rVB	24270	36093	0.47%	0.060%
4	4.017	172	175	182	rVB	15913	21482	0.28%	0.036%
5	4.958	330	335	343	rVB2	31452	53496	0.70%	0.089%
6	7.022	679	686	698	rBV	206653	371817	4.86%	0.620%
7	7.181	706	713	725	rBV	751679	1226410	16.03%	2.047%
8	7.381	740	747	758	rBV	736330	1215953	15.89%	2.029%
9	7.846	820	826	835	rBV	764033	1261487	16.48%	2.105%
10	8.563	941	948	963	rBV	579372	1003958	13.12%	1.675%
11	9.016	1016	1025	1043	rBV	831350	1412638	18.46%	2.357%
12	9.416	1083	1093	1098	rBV3	14967	27382	0.36%	0.046%
13	9.740	1139	1148	1163	rBV	626987	1074316	14.04%	1.793%
14	10.275	1232	1239	1257	rBV	965636	1737921	22.71%	2.900%
15	10.657	1292	1304	1320	rBV	1074159	1849537	24.17%	3.086%
16	10.799	1320	1328	1348	rBV	689292	1274638	16.66%	2.127%
17	12.075	1540	1545	1551	rBV8	4414	8197	0.11%	0.014%
18	12.246	1568	1574	1581	rBV2	15156	28246	0.37%	0.047%
19	13.316	1751	1756	1763	rVB	14767	23691	0.31%	0.040%
20	13.910	1850	1857	1869	rBV	2056778	2776580	36.28%	4.633%
21	14.193	1898	1905	1917	rBV	2349041	3538210	46.24%	5.904%
22	14.387	1932	1938	1942	rVB8	6280	10427	0.14%	0.017%
23	14.498	1950	1957	1974	rBV	1686722	2427106	31.72%	4.050%
24	14.716	1988	1994	2010	rBV	119565	277575	3.63%	0.463%
25	14.922	2023	2029	2037	rVB	10072	24742	0.32%	0.041%
26	15.493	2117	2126	2138	rBV	3345955	4787405	62.56%	7.989%
27	15.616	2141	2147	2163	rVV	879714	1246226	16.29%	2.080%
28	15.734	2163	2167	2175	rVB	17330	26676	0.35%	0.045%
29	16.204	2245	2247	2255	rVB9	4612	8064	0.11%	0.013%
30	17.257	2419	2426	2436	rBV	2134198	3032066	39.62%	5.060%
31	17.357	2436	2443	2457	rBV	3929120	5643586	73.75%	9.418%
32	18.139	2572	2576	2585	rBV	162120	242082	3.16%	0.404%
33	19.169	2747	2751	2756	rBV2	52029	74558	0.97%	0.124%
34	19.233	2759	2762	2768	rBV	62346	94562	1.24%	0.158%
35	19.375	2782	2786	2794	rBV2	135969	207863	2.72%	0.347%
36	19.592	2817	2823	2836	rBV	5344409	7088479	92.63%	11.829%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012105.D
Acq On : 13 Oct 2022 05:33
Operator : CG/JU
Sample : N5026-06
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BX4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Title : SVOA CALIBRATION

37	21.045	3067	3070	3075	rBV	185441	237126	3.10%	0.396%
38	21.345	3116	3121	3127	rBV	2887115	3630291	47.44%	6.058%
39	23.610	3499	3506	3516	rVB	3821021	7652504	100.00%	12.770%
40	23.763	3526	3532	3543	rVB2	1930918	3918480	51.21%	6.539%




Sum of corrected areas: 59924451

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012105.D
Acq On : 13 Oct 2022 05:33
Operator : CG/JU
Sample : N5026-06
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BX4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

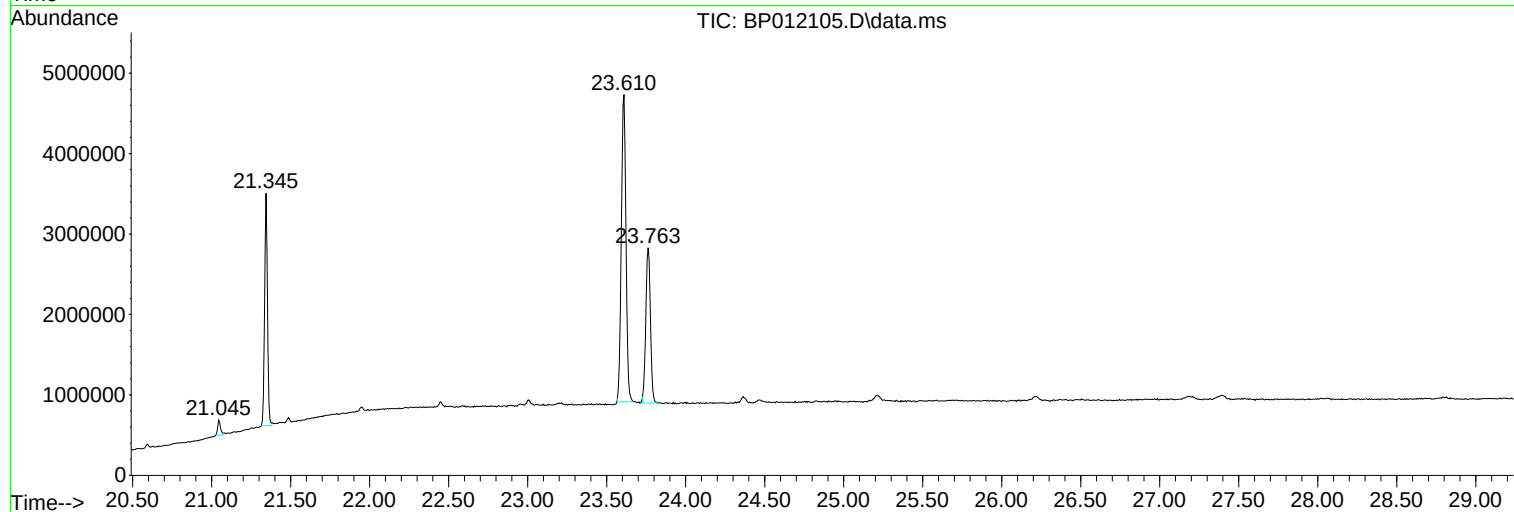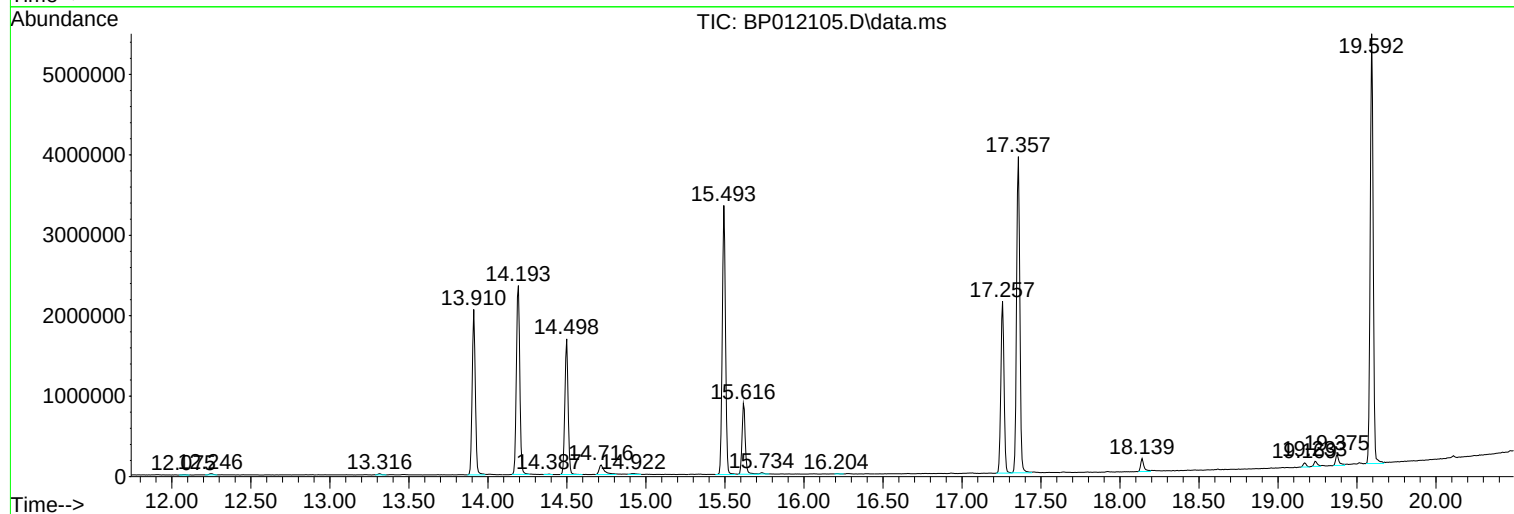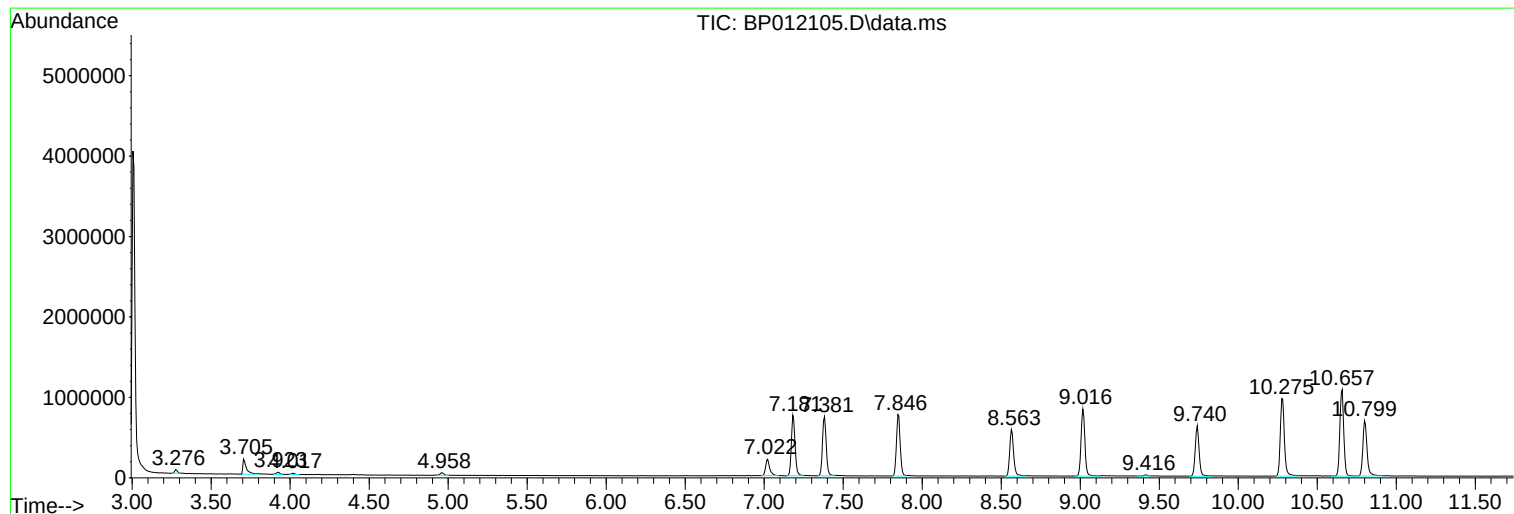

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012105.D
Acq On : 13 Oct 2022 05:33
Operator : CG/JU
Sample : N5026-06
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BX4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012105.D
Acq On : 13 Oct 2022 05:33
Operator : CG/JU
Sample : N5026-06
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BX4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc