

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012110.D
 Acq On : 13 Oct 2022 08:59
 Operator : CG/JU
 Sample : N5026-09
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COBX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012110.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	46	49	59	rVB	48859	69937	0.94%	0.114%
2	3.717	122	124	133	rBV	53474	78175	1.05%	0.128%
3	3.922	155	159	164	rVB	26459	34271	0.46%	0.056%
4	4.017	172	175	180	rVB	15186	19845	0.27%	0.032%
5	4.964	330	336	341	rVB2	20055	32518	0.44%	0.053%
6	7.016	679	685	698	rVB	186162	329343	4.41%	0.537%
7	7.181	707	713	733	rVB	692574	1137000	15.21%	1.855%
8	7.381	738	747	757	rBV	681676	1129548	15.11%	1.843%
9	7.846	819	826	837	rBV	823251	1369950	18.33%	2.235%
10	8.563	941	948	960	rBV	531698	905898	12.12%	1.478%
11	9.016	1018	1025	1040	rBV	781435	1322926	17.70%	2.158%
12	9.416	1088	1093	1098	rVB4	6808	12701	0.17%	0.021%
13	9.740	1138	1148	1164	rBV	584683	1014645	13.57%	1.655%
14	10.275	1232	1239	1260	rBV	902816	1635237	21.88%	2.668%
15	10.652	1296	1303	1318	rVB	1206986	2079599	27.82%	3.392%
16	10.799	1321	1328	1348	rBV	576422	1107346	14.81%	1.806%
17	12.246	1569	1574	1580	rBV3	15087	27557	0.37%	0.045%
18	13.316	1751	1756	1764	rVB9	5952	11490	0.15%	0.019%
19	13.910	1850	1857	1872	rBV	1957453	2717519	36.36%	4.433%
20	14.193	1898	1905	1922	rVV	2217854	3368070	45.06%	5.494%
21	14.498	1949	1957	1974	rBV	1930358	2924566	39.13%	4.771%
22	14.716	1988	1994	2008	rBV	115202	273578	3.66%	0.446%
23	14.922	2024	2029	2035	rVB10	9204	21505	0.29%	0.035%
24	15.492	2115	2126	2140	rBV	3289855	4673473	62.52%	7.624%
25	15.616	2141	2147	2162	rVV	948099	1298558	17.37%	2.118%
26	15.728	2162	2166	2172	rVB2	12786	24537	0.33%	0.040%
27	16.928	2367	2370	2374	rBV5	5311	7985	0.11%	0.013%
28	17.257	2419	2426	2436	rBV	2647751	3763278	50.35%	6.139%
29	17.357	2436	2443	2458	rVV	3931899	5747774	76.90%	9.376%
30	18.139	2571	2576	2584	rBV	154020	239263	3.20%	0.390%
31	19.169	2748	2751	2755	rVB	51305	59374	0.79%	0.097%
32	19.239	2759	2763	2769	rBV2	55190	88641	1.19%	0.145%
33	19.375	2782	2786	2791	rBV2	135166	192666	2.58%	0.314%
34	19.592	2817	2823	2834	rBV	5327789	7137342	95.49%	11.643%
35	21.345	3116	3121	3128	rBV	3602350	4403422	58.91%	7.183%
36	23.604	3499	3505	3519	rVB2	3665319	7474707	100.00%	12.194%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012110.D
Acq On : 13 Oct 2022 08:59
Operator : CG/JU
Sample : N5026-09
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BX7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Title : SVOA CALIBRATION

37	23.763	3526	3532	3543	rVB2	2289566	4566205	61.09%	7.449%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 61300449

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012110.D
Acq On : 13 Oct 2022 08:59
Operator : CG/JU
Sample : N5026-09
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BX7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

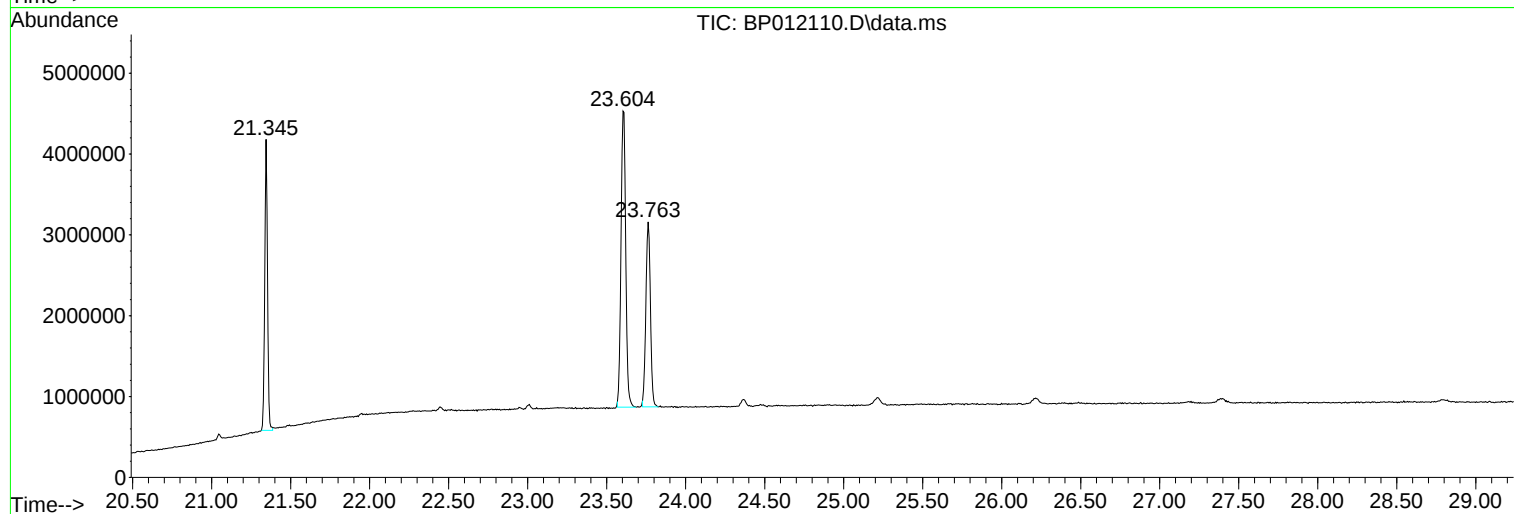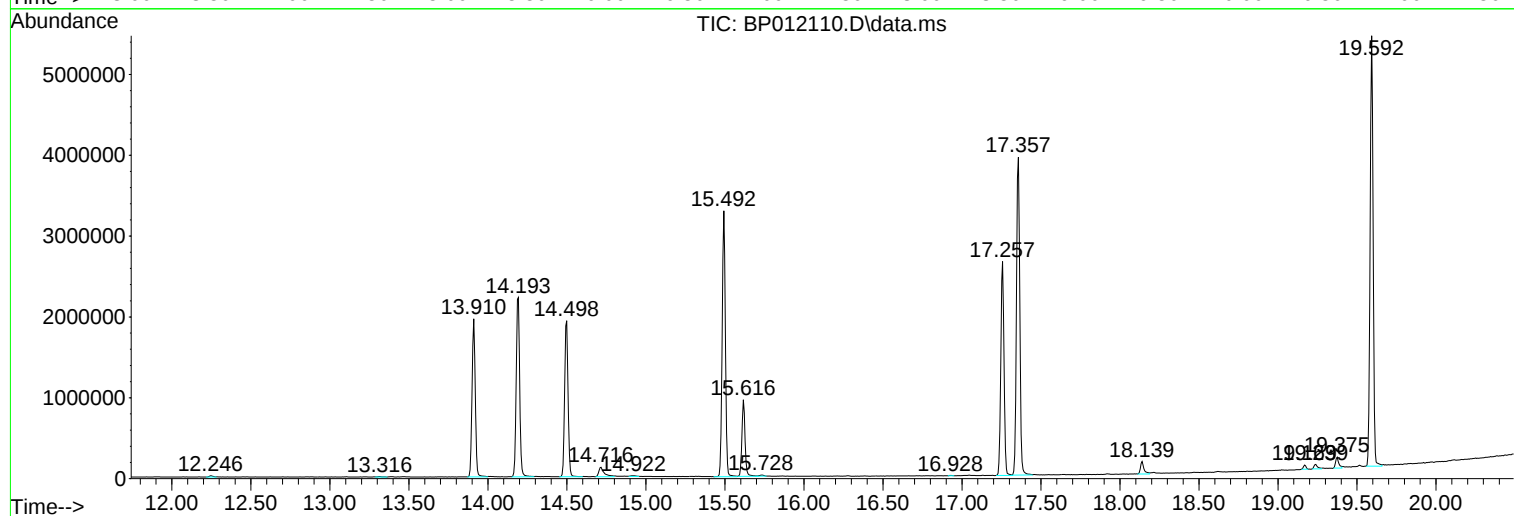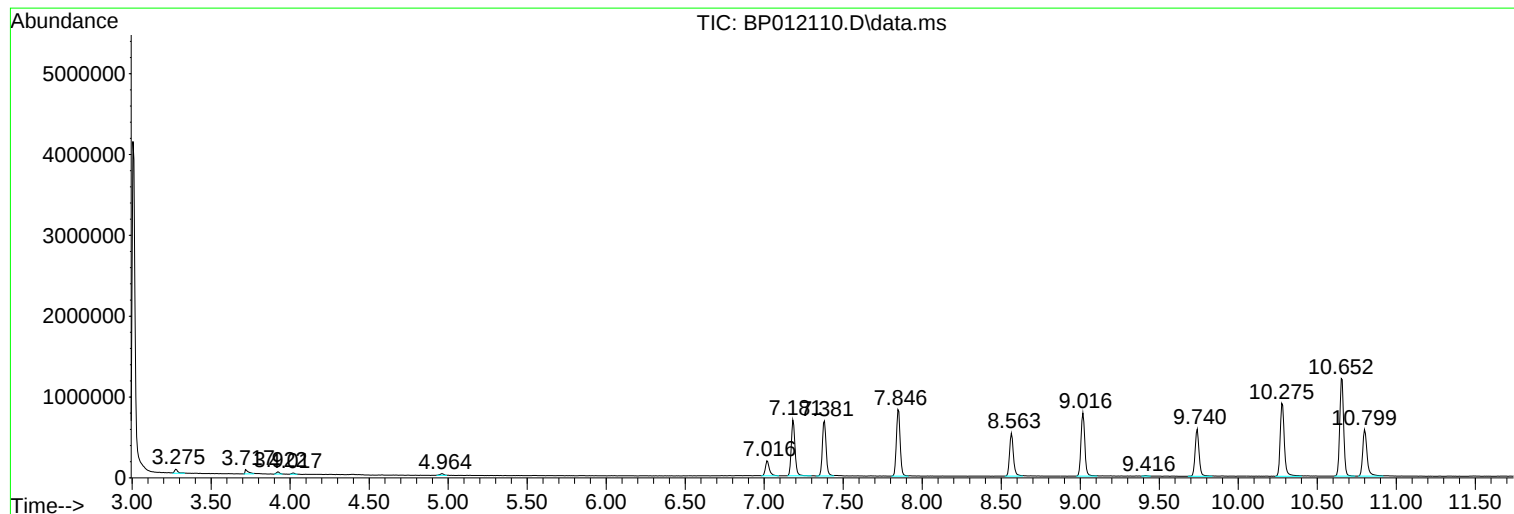

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012110.D
Acq On : 13 Oct 2022 08:59
Operator : CG/JU
Sample : N5026-09
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BX7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012110.D
Acq On : 13 Oct 2022 08:59
Operator : CG/JU
Sample : N5026-09
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BX7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc