

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012112.D
 Acq On : 13 Oct 2022 10:07
 Operator : CG/JU
 Sample : N5026-10
 Misc :
 ALS Vial : 83 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012112.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	46	49	55	rBB	48354	57476	0.80%	0.101%
2	3.705	119	122	136	rBV	179644	290115	4.06%	0.509%
3	3.922	154	159	164	rVB	31599	45322	0.63%	0.080%
4	4.016	172	175	181	rVB	13810	19133	0.27%	0.034%
5	4.957	329	335	343	rVB2	68277	107733	1.51%	0.189%
6	7.016	679	685	696	rBV	233909	416350	5.83%	0.731%
7	7.181	706	713	727	rBV	880308	1433587	20.07%	2.516%
8	7.381	739	747	758	rBV	860779	1415433	19.82%	2.484%
9	7.457	758	760	765	rVB5	5214	7490	0.10%	0.013%
10	7.846	819	826	836	rBV	759111	1234338	17.28%	2.166%
11	8.563	940	948	964	rBV	668215	1148238	16.08%	2.015%
12	9.016	1015	1025	1040	rBV	967851	1616104	22.63%	2.836%
13	9.410	1087	1092	1099	rVB2	20984	35357	0.50%	0.062%
14	9.740	1140	1148	1161	rBV	721745	1234692	17.29%	2.167%
15	10.275	1230	1239	1261	rBV	1102293	1964363	27.50%	3.447%
16	10.651	1294	1303	1319	rBV	1025679	1770336	24.79%	3.106%
17	10.798	1319	1328	1347	rBV	743785	1368288	19.16%	2.401%
18	11.910	1513	1517	1523	rVB8	4760	7821	0.11%	0.014%
19	12.075	1541	1545	1550	rVB6	6403	9425	0.13%	0.017%
20	12.245	1567	1574	1581	rBV	17961	32459	0.45%	0.057%
21	13.316	1751	1756	1760	rBV	20649	31079	0.44%	0.055%
22	13.392	1764	1769	1774	rVB8	6501	12794	0.18%	0.022%
23	13.469	1778	1782	1787	rVB5	4764	8438	0.12%	0.015%
24	13.910	1850	1857	1871	rBV	1978565	2760820	38.66%	4.844%
25	14.186	1895	1904	1921	rBV	2387183	3649803	51.10%	6.404%
26	14.386	1935	1938	1943	rVB4	8567	11719	0.16%	0.021%
27	14.498	1950	1957	1968	rBV	1464630	2150450	30.11%	3.773%
28	14.716	1988	1994	2015	rBV	98294	253166	3.54%	0.444%
29	14.916	2025	2028	2038	rVB	8491	18095	0.25%	0.032%
30	15.298	2088	2093	2095	rBV2	5718	8932	0.13%	0.016%
31	15.492	2119	2126	2139	rBV	3181245	4614380	64.61%	8.097%
32	15.616	2141	2147	2159	rVV	810889	1129646	15.82%	1.982%
33	15.733	2163	2167	2172	rVB2	14154	21806	0.31%	0.038%
34	16.280	2256	2260	2265	rVB8	6553	9065	0.13%	0.016%
35	17.257	2419	2426	2436	rBV	1743207	2502360	35.04%	4.391%
36	17.357	2436	2443	2457	rVV	3448491	5063658	70.90%	8.885%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012112.D
 Acq On : 13 Oct 2022 10:07
 Operator : CG/JU
 Sample : N5026-10
 Misc :
 ALS Vial : 83 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BY0

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

37	18.139	2572	2576	2585	rBV	100048	149692	2.10%	0.263%
38	19.168	2748	2751	2755	rVB3	42859	55312	0.77%	0.097%
39	19.239	2759	2763	2769	rBV	53526	89591	1.25%	0.157%
40	19.374	2782	2786	2792	rBV	93539	135899	1.90%	0.238%
41	19.592	2817	2823	2836	rBV	4893610	6401495	89.63%	11.233%
42	21.045	3067	3070	3077	rBV3	148245	222332	3.11%	0.390%
43	21.345	3116	3121	3128	rBV	2373227	3066898	42.94%	5.382%
44	23.609	3499	3506	3518	rVB2	3522494	7141985	100.00%	12.532%
45	23.762	3526	3532	3544	rVB2	1666513	3265523	45.72%	5.730%




Sum of corrected areas: 56988998

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012112\
Data File : BP012112.D
Acq On : 13 Oct 2022 10:07
Operator : CG/JU
Sample : N5026-10
Misc :
ALS Vial : 83 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BY0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012112.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

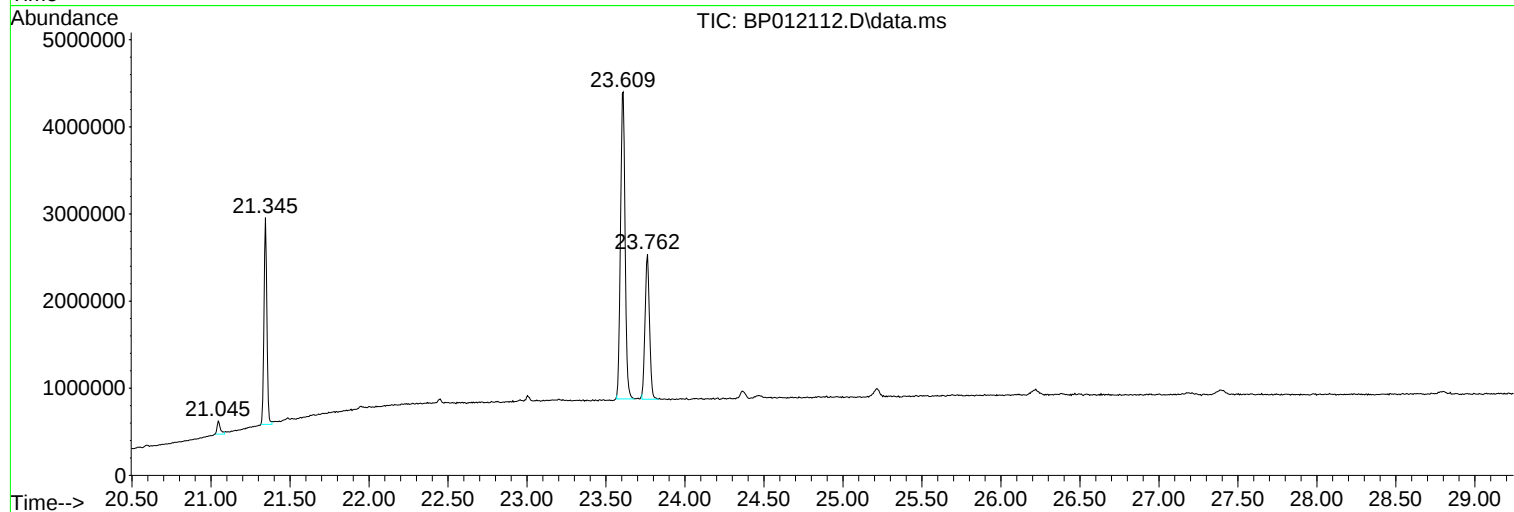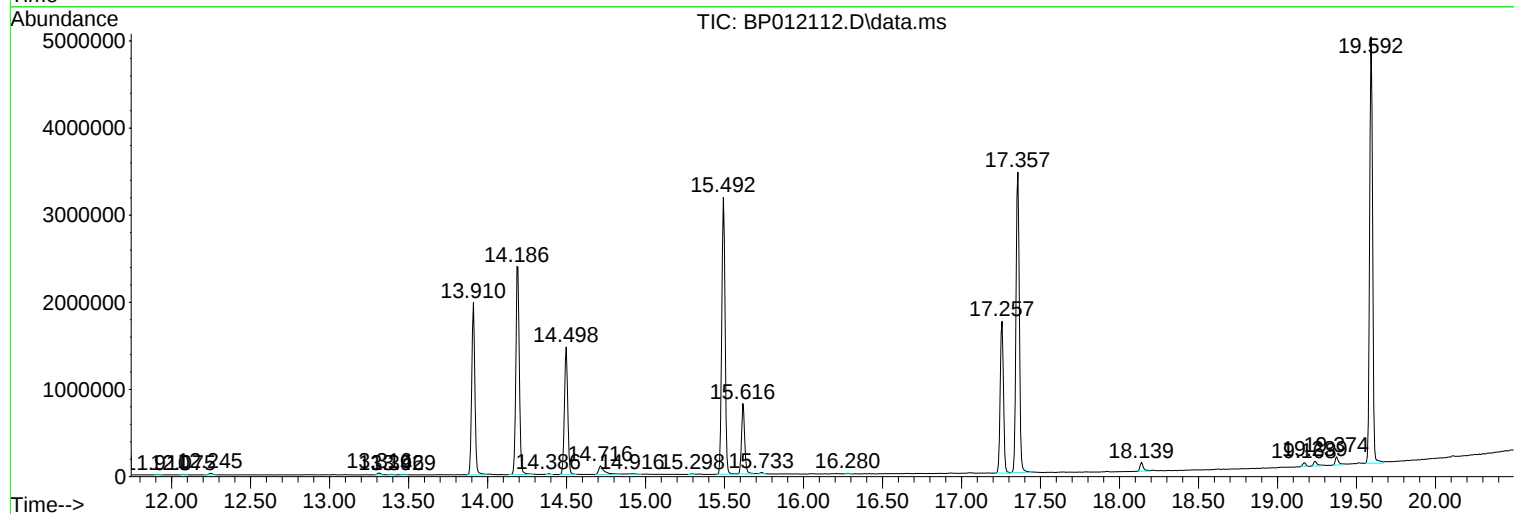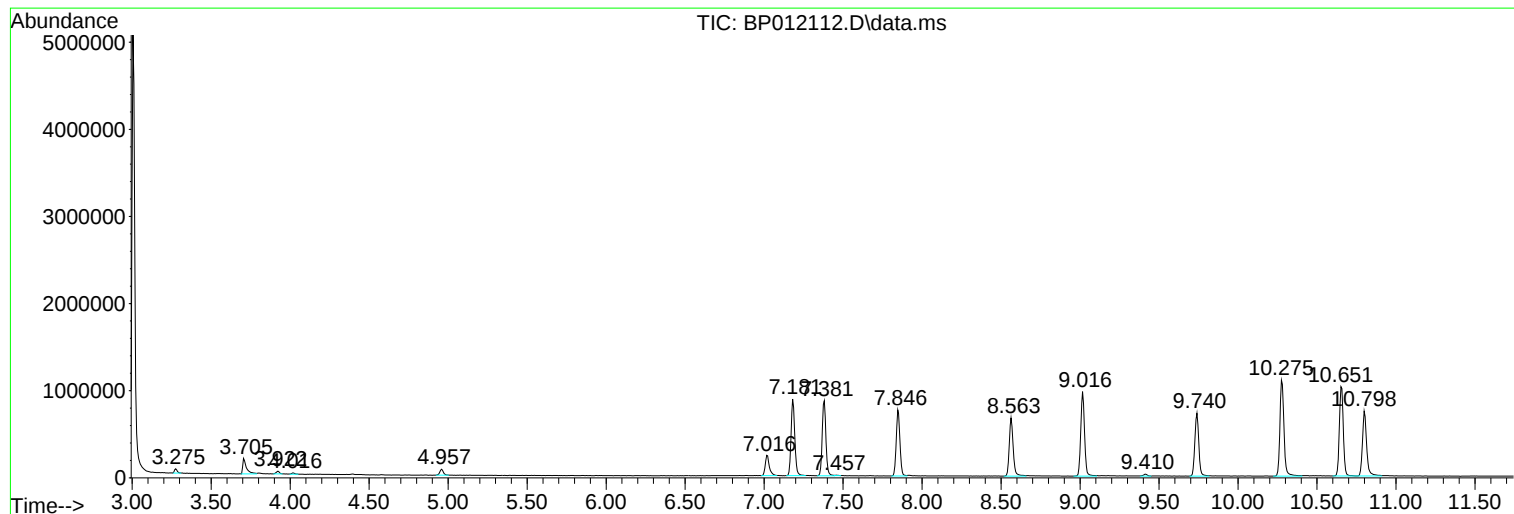

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012112.D
Acq On : 13 Oct 2022 10:07
Operator : CG/JU
Sample : N5026-10
Misc :
ALS Vial : 83 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BY0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012112.D
Acq On : 13 Oct 2022 10:07
Operator : CG/JU
Sample : N5026-10
Misc :
ALS Vial : 83 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BY0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc