

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012113.D
 Acq On : 13 Oct 2022 10:42
 Operator : CG/JU
 Sample : N5049-21
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012113.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	45	49	54	rBV	50476	63096	0.98%	0.116%
2	3.705	120	122	145	rBV	200928	333365	5.18%	0.611%
3	3.922	154	159	164	rVB	34990	52169	0.81%	0.096%
4	4.017	171	175	181	rVB	27318	35773	0.56%	0.066%
5	4.946	329	333	341	rVB	9477	18027	0.28%	0.033%
6	7.022	680	686	698	rBV2	248369	452193	7.02%	0.829%
7	7.181	706	713	729	rBV	931836	1522250	23.64%	2.790%
8	7.381	739	747	757	rBV	899711	1462563	22.71%	2.681%
9	7.646	786	792	795	rBV4	8437	13815	0.21%	0.025%
10	7.846	819	826	839	rBV	923224	1505497	23.38%	2.759%
11	8.563	941	948	968	rBV	692149	1166414	18.11%	2.138%
12	9.016	1017	1025	1042	rBV	1020819	1695420	26.33%	3.108%
13	9.416	1088	1093	1102	rVB5	6323	13174	0.20%	0.024%
14	9.740	1138	1148	1162	rBV	501056	869038	13.50%	1.593%
15	10.275	1232	1239	1254	rBV	1050378	1881898	29.22%	3.449%
16	10.651	1295	1303	1319	rVB	1278693	2183048	33.90%	4.001%
17	10.799	1321	1328	1350	rBV	799591	1506460	23.39%	2.761%
18	11.910	1508	1517	1526	rBV	39491	63886	0.99%	0.117%
19	12.251	1570	1575	1584	rBV3	16095	36545	0.57%	0.067%
20	13.469	1777	1782	1788	rVB8	5327	9156	0.14%	0.017%
21	13.822	1837	1842	1847	rBV9	4357	6519	0.10%	0.012%
22	13.910	1850	1857	1872	rBV	1931535	2710429	42.09%	4.968%
23	14.192	1897	1905	1920	rBV	2424474	3569992	55.44%	6.543%
24	14.498	1950	1957	1967	rBV	1742090	2552364	39.64%	4.678%
25	14.734	1990	1997	2006	rBV3	20305	63825	0.99%	0.117%
26	14.934	2023	2031	2037	rVB3	8572	17831	0.28%	0.033%
27	15.492	2119	2126	2142	rBV	3125479	4407717	68.45%	8.079%
28	15.616	2142	2147	2159	rVV	188178	299621	4.65%	0.549%
29	15.734	2164	2167	2174	rVB2	13030	22176	0.34%	0.041%
30	17.257	2419	2426	2436	rBV	1969273	2689803	41.77%	4.930%
31	17.357	2437	2443	2456	rVV	3251630	4609838	71.59%	8.449%
32	18.145	2574	2577	2581	rBV5	18398	25053	0.39%	0.046%
33	19.175	2748	2752	2758	rBV3	38453	56438	0.88%	0.103%
34	19.239	2760	2763	2768	rVV2	38664	49477	0.77%	0.091%
35	19.592	2818	2823	2830	rBV	4141126	5505055	85.49%	10.090%
36	21.345	3117	3121	3129	rBV	2523070	3201222	49.71%	5.868%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012113.D
Acq On : 13 Oct 2022 10:42
Operator : CG/JU
Sample : N5049-21
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BE1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Title : SVOA CALIBRATION

37	23.610	3499	3506	3522	rVB2	3147960	6439470	100.00%	11.803%
38	23.768	3527	3533	3541	rVB2	1718507	3447365	53.53%	6.319%




Sum of corrected areas: 54557982

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012113.D
Acq On : 13 Oct 2022 10:42
Operator : CG/JU
Sample : N5049-21
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

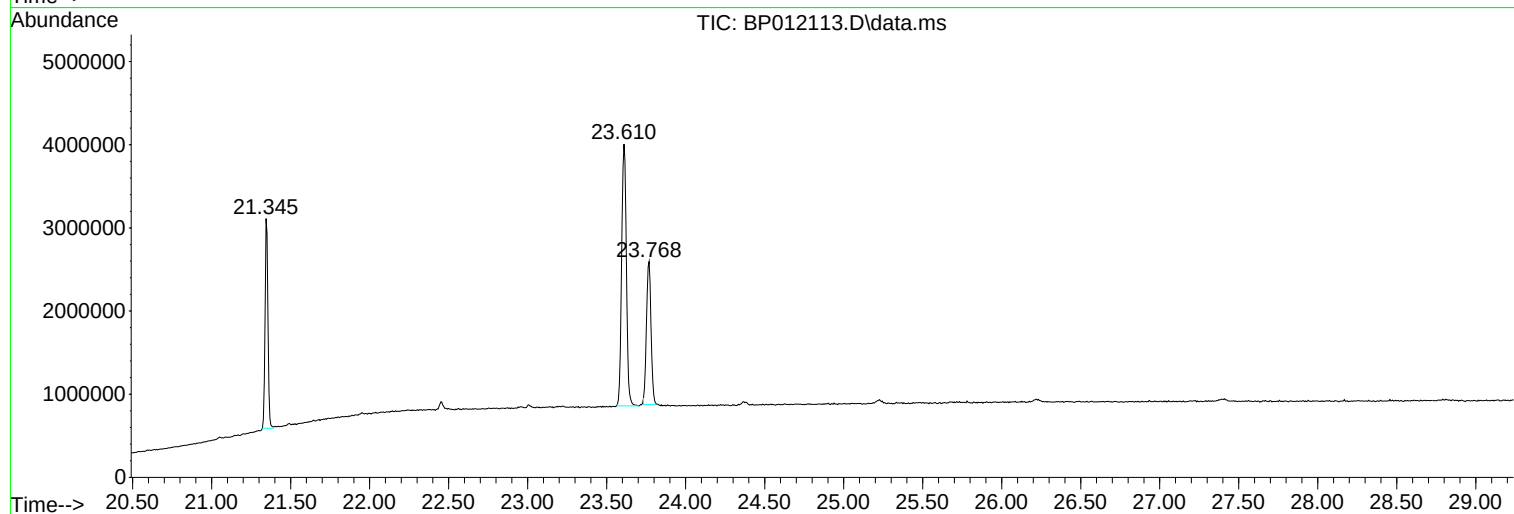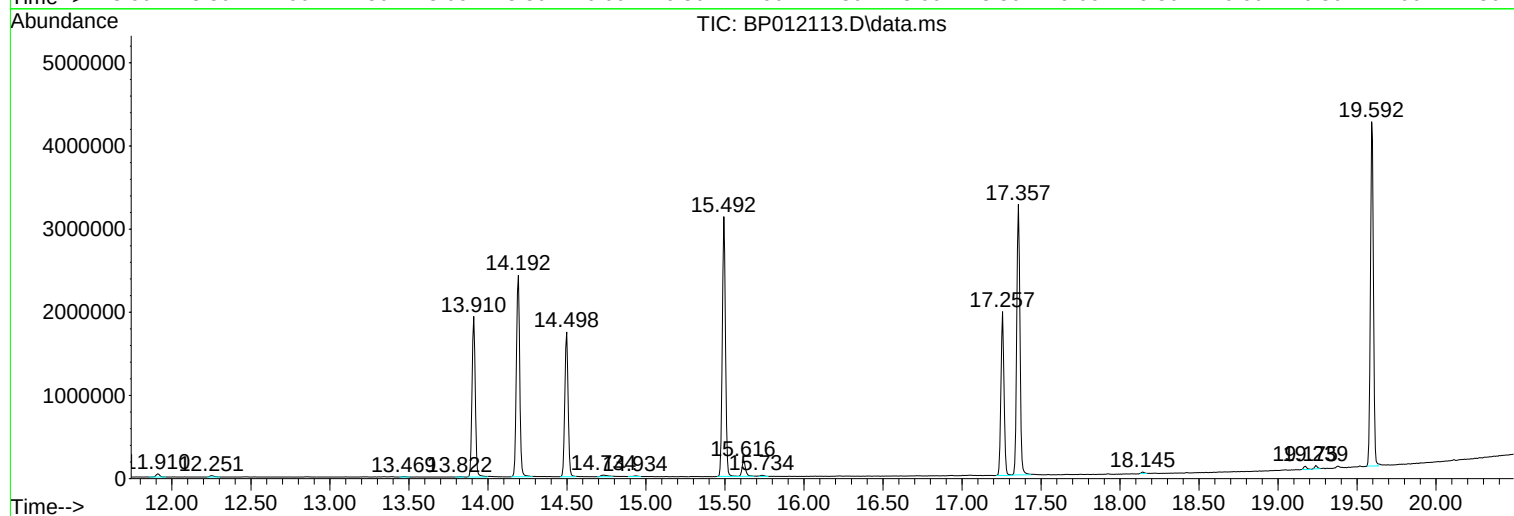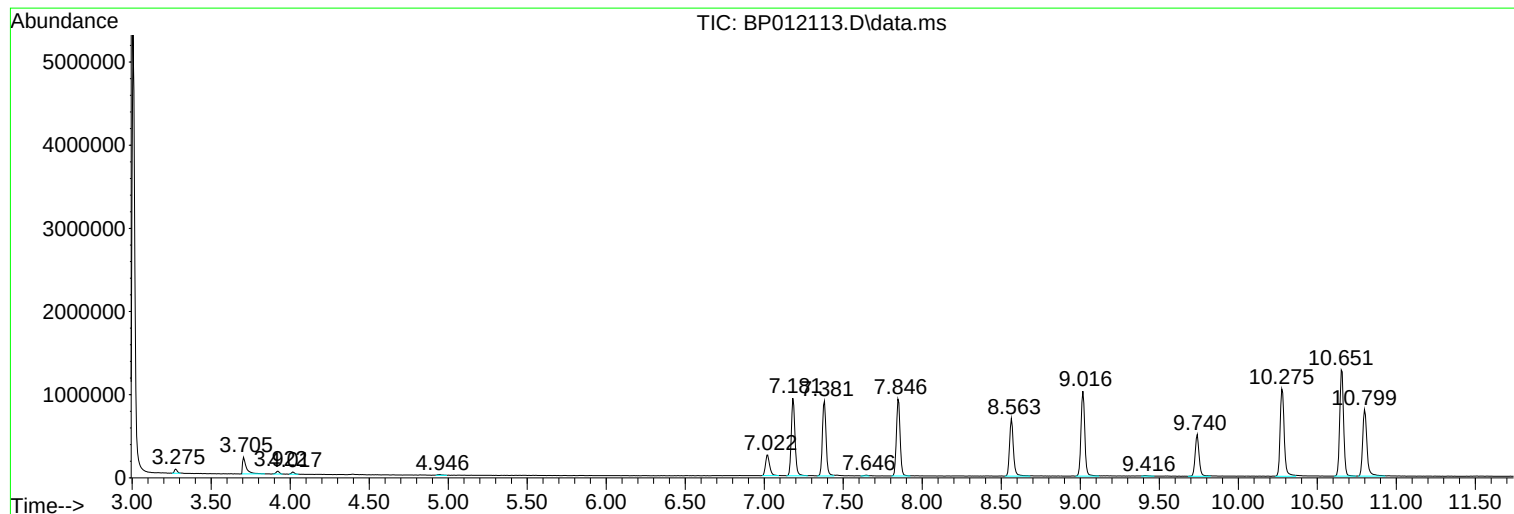

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012113.D
Acq On : 13 Oct 2022 10:42
Operator : CG/JU
Sample : N5049-21
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012113.D
Acq On : 13 Oct 2022 10:42
Operator : CG/JU
Sample : N5049-21
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
