

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012117.D
 Acq On : 13 Oct 2022 13:00
 Operator : CG/JU
 Sample : PB148253BL
 Misc :
 ALS Vial : 88 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK253

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012117.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	45	49	56	rVB	66730	83813	1.52%	0.151%
2	3.699	117	121	135	rBV	728260	1108079	20.08%	2.002%
3	4.017	172	175	181	rVB	18190	25528	0.46%	0.046%
4	7.016	678	685	700	rBV	881915	1439243	26.08%	2.600%
5	7.181	706	713	730	rVB	769171	1239788	22.47%	2.240%
6	7.381	738	747	759	rBV	912887	1531110	27.75%	2.766%
7	7.846	819	826	843	rBV	895010	1460928	26.48%	2.639%
8	8.563	941	948	966	rBV	1070577	1813214	32.86%	3.276%
9	9.016	1018	1025	1038	rBV	807134	1382930	25.06%	2.498%
10	9.740	1139	1148	1161	rBV	630854	1080117	19.57%	1.951%
11	10.275	1232	1239	1256	rBV	971241	1743646	31.60%	3.150%
12	10.657	1295	1304	1320	rBV	1191780	2094060	37.95%	3.783%
13	10.799	1320	1328	1348	rBV	996510	1817538	32.94%	3.283%
14	12.257	1570	1576	1585	rBV2	13846	32674	0.59%	0.059%
15	13.234	1736	1742	1747	rBV9	2993	5844	0.11%	0.011%
16	13.910	1851	1857	1871	rBV	1584931	2235179	40.51%	4.038%
17	14.193	1897	1905	1921	rBV	1970674	3036177	55.02%	5.485%
18	14.498	1950	1957	1966	rBV	1723950	2506480	45.42%	4.528%
19	14.710	1987	1993	2015	rBV	554861	1060614	19.22%	1.916%
20	14.910	2024	2027	2036	rVB10	5041	11056	0.20%	0.020%
21	15.492	2119	2126	2141	rBV	2632568	3765928	68.25%	6.803%
22	15.616	2141	2147	2159	rVV	584166	835356	15.14%	1.509%
23	15.734	2163	2167	2174	rVB4	13335	24194	0.44%	0.044%
24	17.039	2385	2389	2392	rBV3	4957	7685	0.14%	0.014%
25	17.257	2419	2426	2436	rBV	2057076	2902608	52.60%	5.244%
26	17.357	2436	2443	2458	rVV	2798415	4083228	74.00%	7.377%
27	19.169	2748	2751	2758	rBV2	35748	48784	0.88%	0.088%
28	19.239	2760	2763	2769	rVV2	34136	51153	0.93%	0.092%
29	19.592	2818	2823	2837	rBV	3910346	5033061	91.21%	9.092%
30	21.345	3116	3121	3129	rBV	2761267	3625274	65.70%	6.549%
31	23.610	3499	3506	3519	rVB2	2741064	5517972	100.00%	9.968%
32	23.769	3526	3533	3542	rVB2	1911262	3750964	67.98%	6.776%




Sum of corrected areas: 55354225

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012117.D
Acq On : 13 Oct 2022 13:00
Operator : CG/JU
Sample : PB148253BL
Misc :
ALS Vial : 88 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK253

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

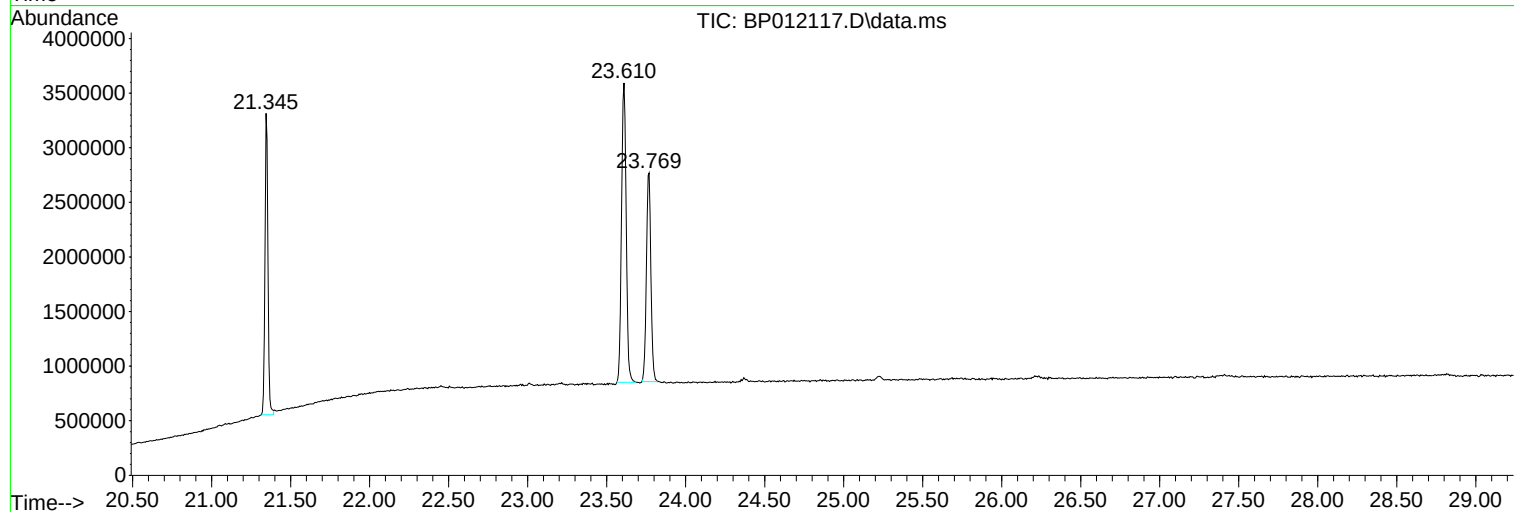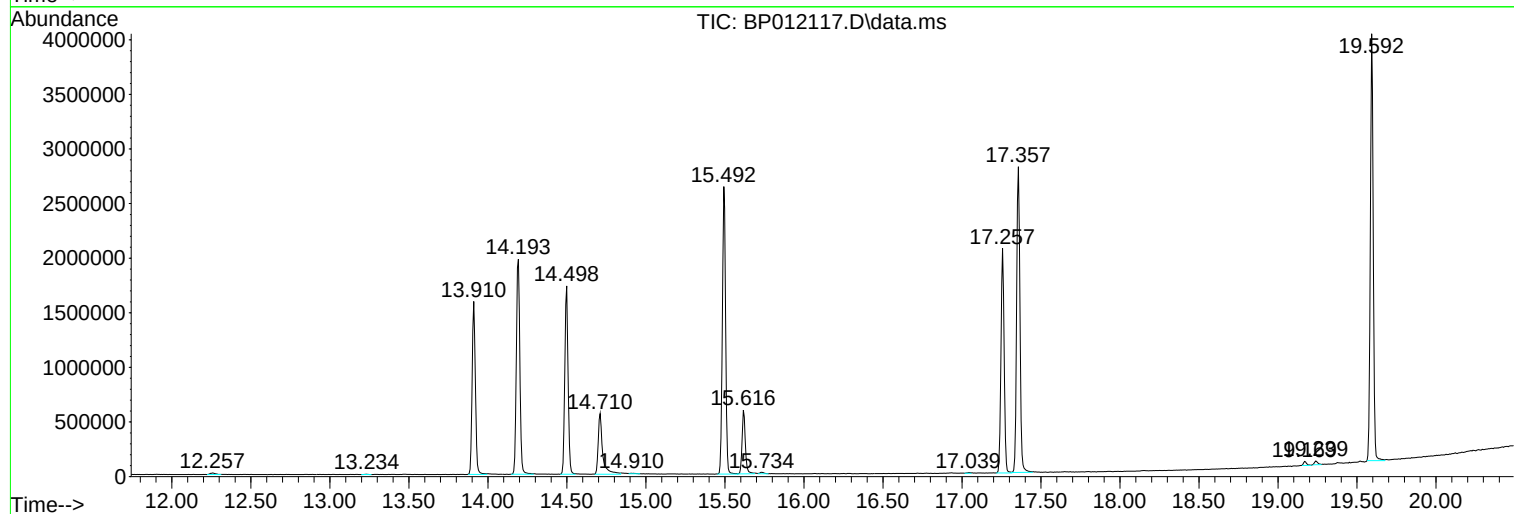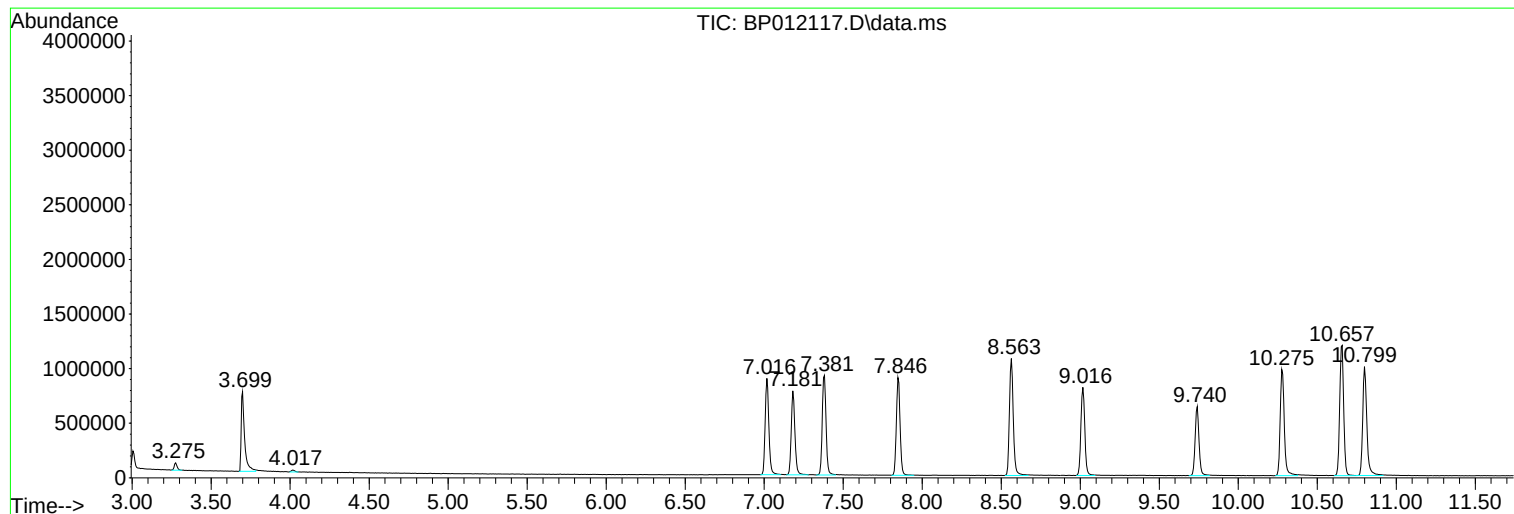

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012117.D
Acq On : 13 Oct 2022 13:00
Operator : CG/JU
Sample : PB148253BL
Misc :
ALS Vial : 88 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK253

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012117.D
Acq On : 13 Oct 2022 13:00
Operator : CG/JU
Sample : PB148253BL
Misc :
ALS Vial : 88 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK253

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc