

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012118.D
 Acq On : 13 Oct 2022 13:35
 Operator : CG/JU
 Sample : N5013-07
 Misc :
 ALS Vial : 89 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012118.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	45	49	53	rBV	53677	66990	0.96%	0.114%
2	3.705	119	122	140	rBV	281926	465703	6.68%	0.796%
3	3.923	155	159	165	rVB	32640	50754	0.73%	0.087%
4	4.017	172	175	182	rVB2	15849	24439	0.35%	0.042%
5	4.393	237	239	246	rVB7	7864	10863	0.16%	0.019%
6	4.940	329	332	343	rVB4	8230	20234	0.29%	0.035%
7	7.017	679	685	701	rBV	246832	435548	6.25%	0.744%
8	7.181	706	713	726	rBV	891379	1445104	20.73%	2.470%
9	7.381	739	747	758	rBV	885188	1425384	20.45%	2.436%
10	7.846	818	826	835	rBV	860105	1400550	20.09%	2.393%
11	8.564	941	948	964	rBV	706303	1166688	16.74%	1.994%
12	9.016	1017	1025	1036	rBV	977058	1639229	23.52%	2.801%
13	9.375	1081	1086	1088	rBV4	6056	9593	0.14%	0.016%
14	9.411	1088	1092	1098	rVB2	17560	30113	0.43%	0.051%
15	9.740	1139	1148	1165	rBV	734470	1240925	17.80%	2.121%
16	10.275	1232	1239	1254	rBV	1115830	1935509	27.77%	3.308%
17	10.475	1269	1273	1281	rVB10	5073	11031	0.16%	0.019%
18	10.652	1295	1303	1316	rBV	1151444	1989311	28.54%	3.400%
19	10.799	1321	1328	1342	rBV	970303	1753846	25.16%	2.997%
20	11.675	1470	1477	1481	rBV10	3918	7388	0.11%	0.013%
21	11.910	1512	1517	1521	rVB8	4215	7375	0.11%	0.013%
22	12.246	1565	1574	1583	rVB	20896	45281	0.65%	0.077%
23	12.469	1602	1612	1616	rBV	7067	19490	0.28%	0.033%
24	12.610	1630	1636	1640	rBV4	8933	16175	0.23%	0.028%
25	12.757	1655	1661	1666	rBV7	8692	16929	0.24%	0.029%
26	12.852	1670	1677	1680	rVV8	5595	11353	0.16%	0.019%
27	12.881	1680	1682	1687	rVB6	5540	7801	0.11%	0.013%
28	13.040	1702	1709	1712	rBV3	10745	19131	0.27%	0.033%
29	13.093	1712	1718	1724	rVV4	20865	34338	0.49%	0.059%
30	13.222	1735	1740	1746	rBV9	4277	7593	0.11%	0.013%
31	13.310	1751	1755	1761	rVV	16610	25778	0.37%	0.044%
32	13.393	1764	1769	1776	rVV2	28227	48463	0.70%	0.083%
33	13.463	1777	1781	1785	rVB6	4681	8008	0.11%	0.014%
34	13.781	1829	1835	1840	rBV6	8887	14017	0.20%	0.024%
35	13.910	1850	1857	1871	rBV	1890924	2644452	37.94%	4.519%
36	14.022	1872	1876	1884	rVB6	26083	42819	0.61%	0.073%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012118.D
 Acq On : 13 Oct 2022 13:35
 Operator : CG/JU
 Sample : N5013-07
 Misc :
 ALS Vial : 89 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

37	14.193	1898	1905	1913	rVV	2362220	3520923	50.52%	6.017%
38	14.387	1935	1938	1942	rBV4	5297	7309	0.10%	0.012%
39	14.499	1949	1957	1967	rBV	1632388	2392197	34.32%	4.088%
40	14.716	1988	1994	2005	rBV	104330	238885	3.43%	0.408%
41	14.922	2024	2029	2036	rVB10	11176	24550	0.35%	0.042%
42	15.398	2104	2110	2113	rBV8	6829	13552	0.19%	0.023%
43	15.493	2119	2126	2139	rBV	3104277	4383484	62.89%	7.491%
44	15.616	2141	2147	2162	rVV	772896	1075961	15.44%	1.839%
45	15.734	2162	2167	2173	rVV5	16847	37044	0.53%	0.063%
46	15.787	2173	2176	2186	rVB5	9534	23744	0.34%	0.041%
47	16.004	2208	2213	2219	rBV3	37031	62119	0.89%	0.106%
48	16.057	2219	2222	2229	rVB2	10245	17120	0.25%	0.029%
49	16.175	2238	2242	2245	rBV3	8211	13629	0.20%	0.023%
50	16.651	2319	2323	2325	rBV5	7947	12922	0.19%	0.022%
51	17.004	2381	2383	2387	rBV4	7991	9001	0.13%	0.015%
52	17.257	2419	2426	2436	rBV	1892263	2746078	39.40%	4.693%
53	17.357	2436	2443	2459	rBV	3236994	4831337	69.32%	8.256%
54	17.616	2483	2487	2491	rBV5	12602	21224	0.30%	0.036%
55	17.881	2528	2532	2536	rBV	37890	55684	0.80%	0.095%
56	17.922	2536	2539	2543	rVB6	13976	19589	0.28%	0.033%
57	18.022	2553	2556	2560	rVB6	15754	23062	0.33%	0.039%
58	18.140	2572	2576	2585	rBV	116679	175049	2.51%	0.299%
59	18.287	2597	2601	2606	rBV	42343	59426	0.85%	0.102%
60	18.387	2615	2618	2620	rBV	24869	27856	0.40%	0.048%
61	18.434	2623	2626	2630	rVB	67611	85020	1.22%	0.145%
62	19.169	2748	2751	2755	rVB2	50610	60943	0.87%	0.104%
63	19.234	2759	2762	2769	rVV	52120	77139	1.11%	0.132%
64	19.375	2782	2786	2794	rBV2	97185	128329	1.84%	0.219%
65	19.592	2817	2823	2835	rBV	4806784	6141613	88.11%	10.495%
66	21.345	3116	3121	3128	rBV	2815070	3463082	49.69%	5.918%
67	23.604	3499	3505	3518	rVB2	3539348	6970008	100.00%	11.911%
68	23.763	3526	3532	3542	rVB2	1839887	3701255	53.10%	6.325%




Sum of corrected areas: 58517339

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012118.D
Acq On : 13 Oct 2022 13:35
Operator : CG/JU
Sample : N5013-07
Misc :
ALS Vial : 89 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA44

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

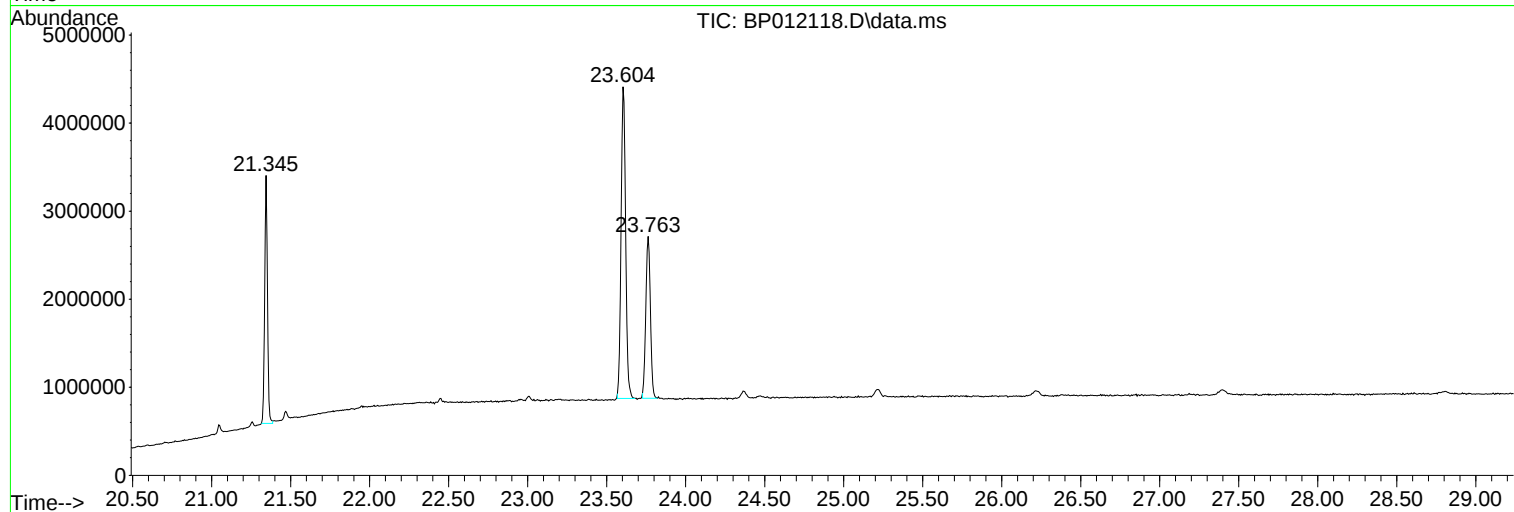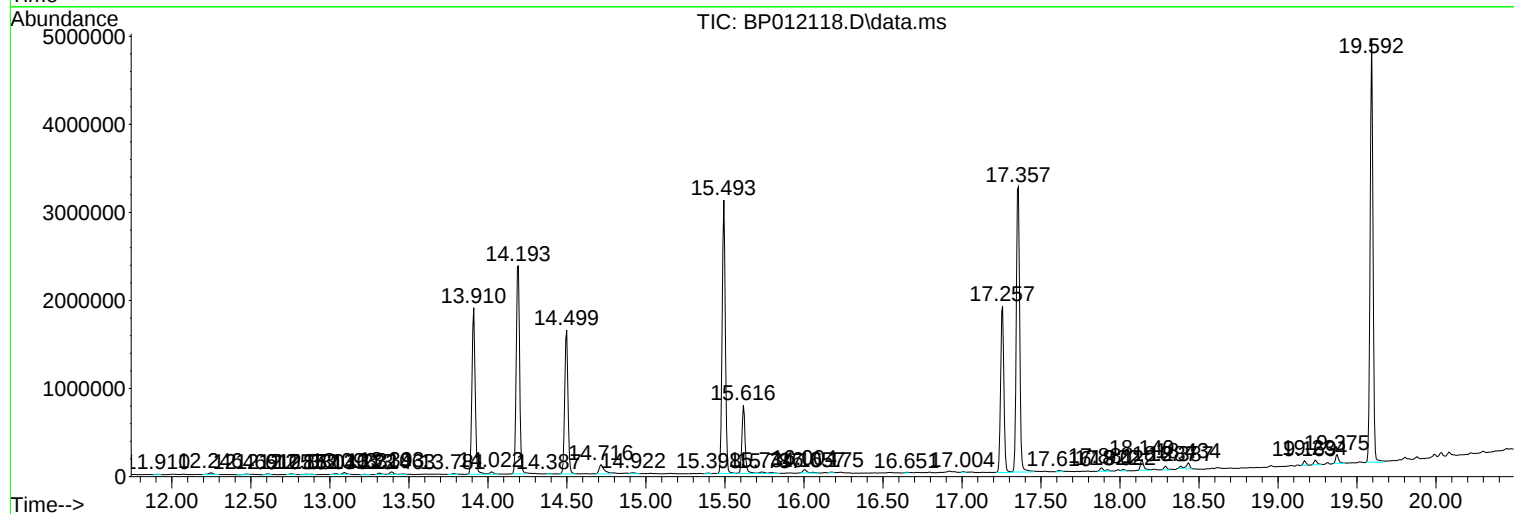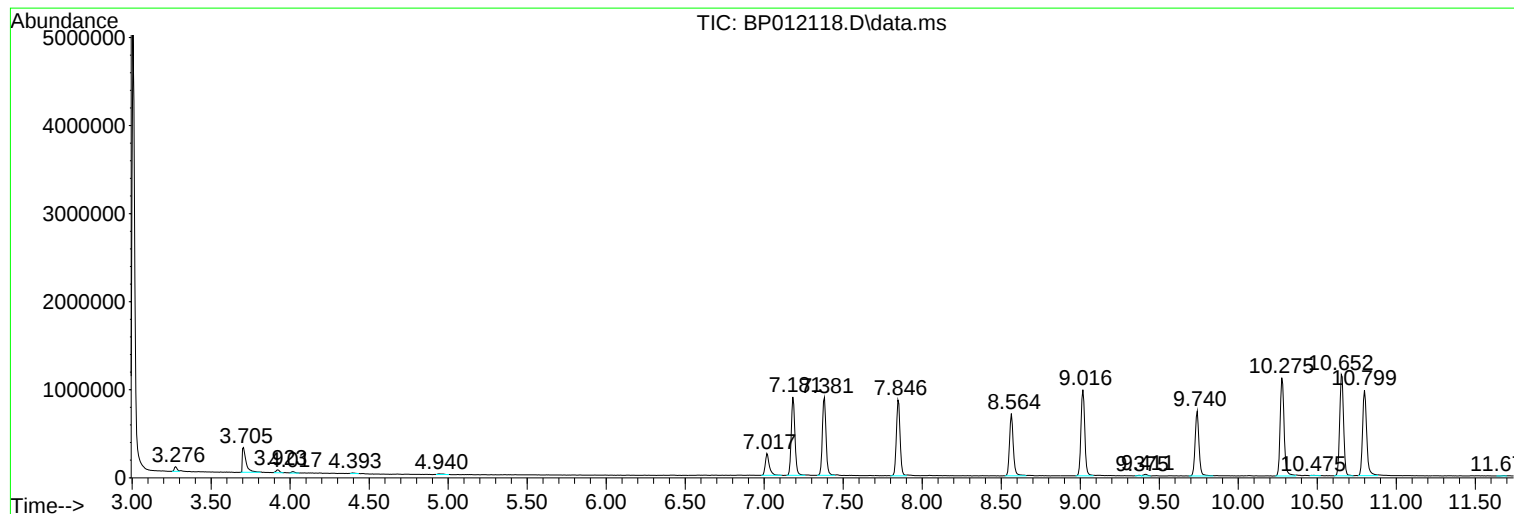

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012118.D
Acq On : 13 Oct 2022 13:35
Operator : CG/JU
Sample : N5013-07
Misc :
ALS Vial : 89 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA44

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012118.D
Acq On : 13 Oct 2022 13:35
Operator : CG/JU
Sample : N5013-07
Misc :
ALS Vial : 89 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA44

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc