

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
 Data File : BP012120.D
 Acq On : 13 Oct 2022 14:44
 Operator : CG/JU
 Sample : N5041-02
 Misc :
 ALS Vial : 91 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGS19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	45	49	53	rBV	52345	63708	0.91%	0.112%
2	3.711	121	123	139	rVB	83315	123032	1.75%	0.215%
3	3.922	154	159	164	rVB	33318	47441	0.68%	0.083%
4	4.016	172	175	181	rVB	25299	33597	0.48%	0.059%
5	4.940	329	332	342	rVB4	8036	18265	0.26%	0.032%
6	7.016	679	685	696	rBV	231498	399367	5.69%	0.699%
7	7.181	707	713	728	rBV	862696	1387819	19.78%	2.430%
8	7.381	740	747	758	rBV	851624	1389065	19.80%	2.432%
9	7.846	819	826	837	rBV	866041	1465669	20.89%	2.566%
10	8.099	862	869	877	rBV4	19614	34859	0.50%	0.061%
11	8.563	941	948	971	rBV	663957	1123132	16.01%	1.966%
12	9.016	1018	1025	1043	rBV	934472	1578692	22.50%	2.764%
13	9.416	1087	1093	1097	rVB4	7224	12192	0.17%	0.021%
14	9.740	1140	1148	1162	rBV	710174	1195938	17.04%	2.094%
15	10.275	1232	1239	1262	rBV	1033511	1850702	26.37%	3.240%
16	10.463	1264	1271	1287	rVB3	14836	51906	0.74%	0.091%
17	10.657	1296	1304	1318	rVB	1204750	2099413	29.92%	3.676%
18	10.798	1322	1328	1345	rBV	512270	972513	13.86%	1.703%
19	12.245	1568	1574	1583	rBV	17806	32796	0.47%	0.057%
20	13.316	1752	1756	1760	rVB6	5844	8705	0.12%	0.015%
21	13.469	1775	1782	1787	rVB6	5755	10356	0.15%	0.018%
22	13.910	1850	1857	1872	rBV	1862750	2620344	37.34%	4.588%
23	14.010	1872	1874	1885	rVB8	5444	13710	0.20%	0.024%
24	14.192	1892	1905	1922	rBV	2288746	3463283	49.36%	6.064%
25	14.498	1948	1957	1971	rBV	1715980	2549989	36.34%	4.465%
26	14.716	1988	1994	2009	rBV	94643	239703	3.42%	0.420%
27	15.322	2094	2097	2105	rVB	12683	20215	0.29%	0.035%
28	15.492	2119	2126	2141	rBV	3096347	4380782	62.43%	7.670%
29	15.622	2141	2148	2163	rVV	765867	1106751	15.77%	1.938%
30	15.733	2163	2167	2173	rVB2	14486	24893	0.35%	0.044%
31	16.280	2256	2260	2265	rBV8	4423	7924	0.11%	0.014%
32	17.257	2419	2426	2436	rBV	2079660	2901745	41.35%	5.080%
33	17.357	2436	2443	2455	rBV	3522853	4989116	71.10%	8.735%
34	17.922	2537	2539	2544	rVB3	10859	11906	0.17%	0.021%
35	18.139	2572	2576	2585	rBV	60475	96031	1.37%	0.168%
36	19.169	2748	2751	2757	rBV2	43658	55679	0.79%	0.097%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012120.D
Acq On : 13 Oct 2022 14:44
Operator : CG/JU
Sample : N5041-02
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGS19

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Title : SVOA CALIBRATION

37	19.239	2760	2763	2768	rVV	39747	50947	0.73%	0.089%
38	19.374	2783	2786	2792	rBV3	63757	89631	1.28%	0.157%
39	19.592	2818	2823	2837	rBV	4682595	6192676	88.25%	10.842%
40	21.345	3117	3121	3130	rBV	2750355	3546430	50.54%	6.209%
41	23.610	3499	3506	3519	rVB2	3499539	7016966	100.00%	12.285%
42	23.768	3526	3533	3543	rVB	1944358	3837980	54.70%	6.720%




Sum of corrected areas: 57115868

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012120.D
Acq On : 13 Oct 2022 14:44
Operator : CG/JU
Sample : N5041-02
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGS19

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

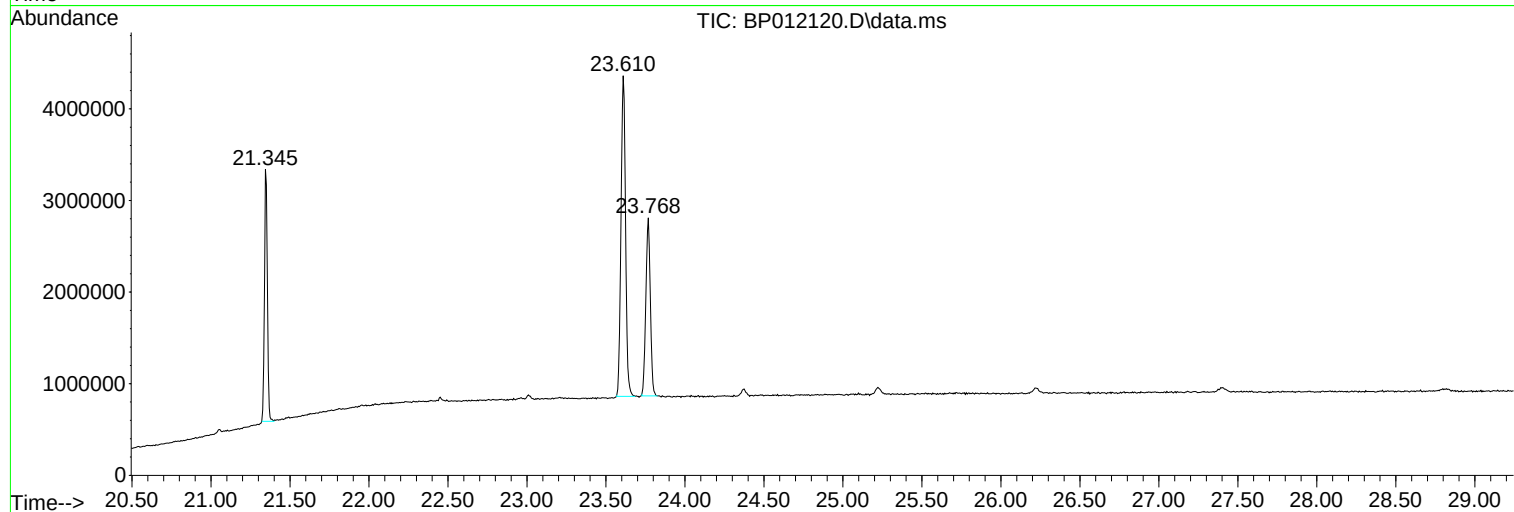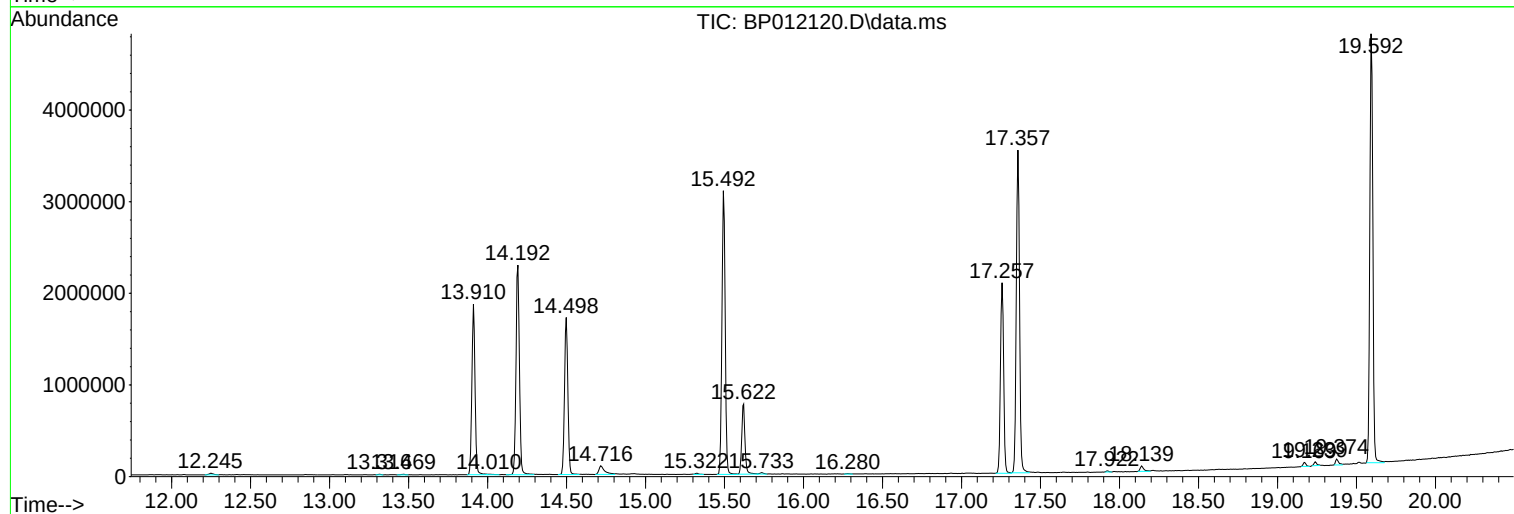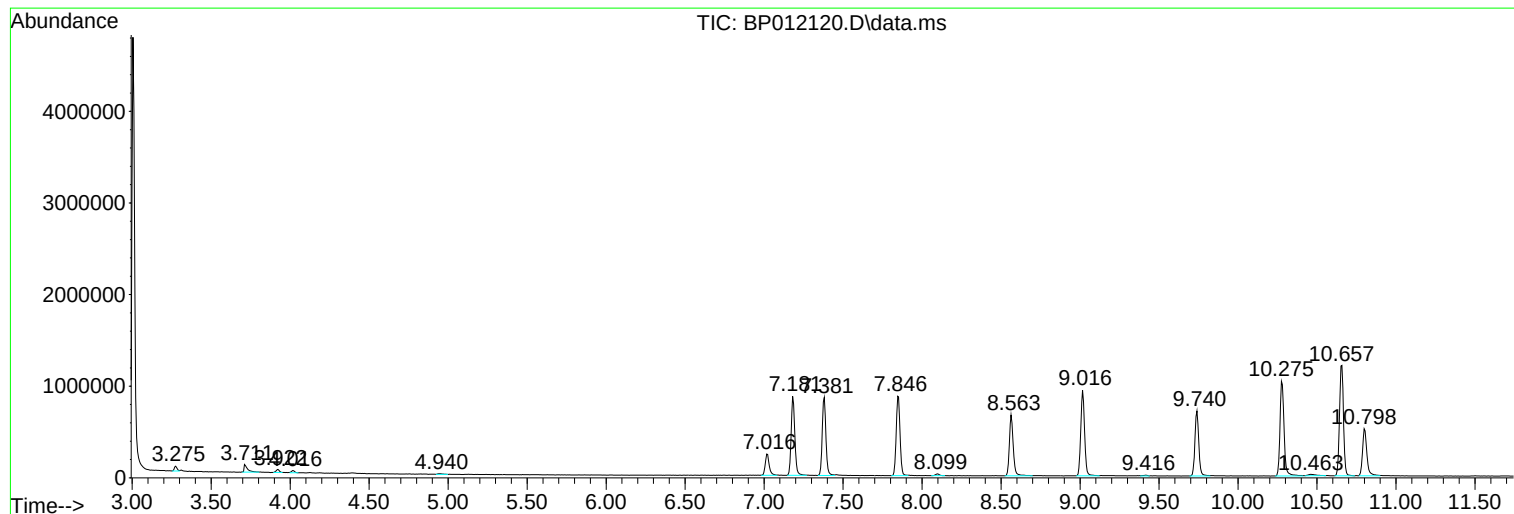

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012120.D
Acq On : 13 Oct 2022 14:44
Operator : CG/JU
Sample : N5041-02
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGS19

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101122\
Data File : BP012120.D
Acq On : 13 Oct 2022 14:44
Operator : CG/JU
Sample : N5041-02
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGS19

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
