




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101124\
 Data File : BP022339.D
 Acq On : 11 Oct 2024 18:11
 Operator : RC/JU
 Sample : P4237-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4F26

Manual Integrations APPROVED

Quant Time: Oct 11 18:44:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 08 02:14:47 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/14/2024
 Supervised By :mohammad ahmed 10/15/2024

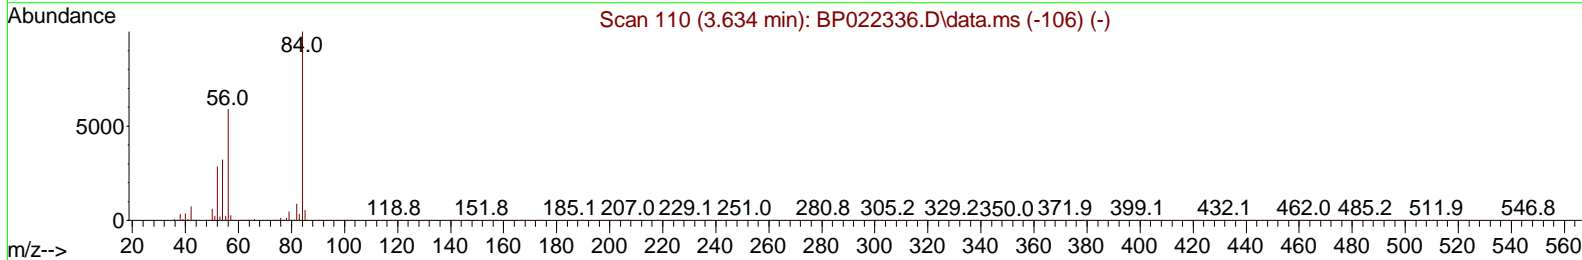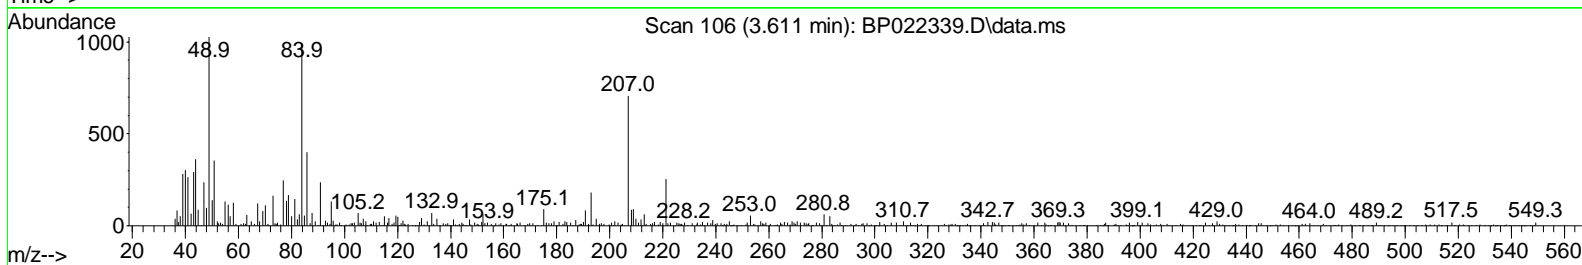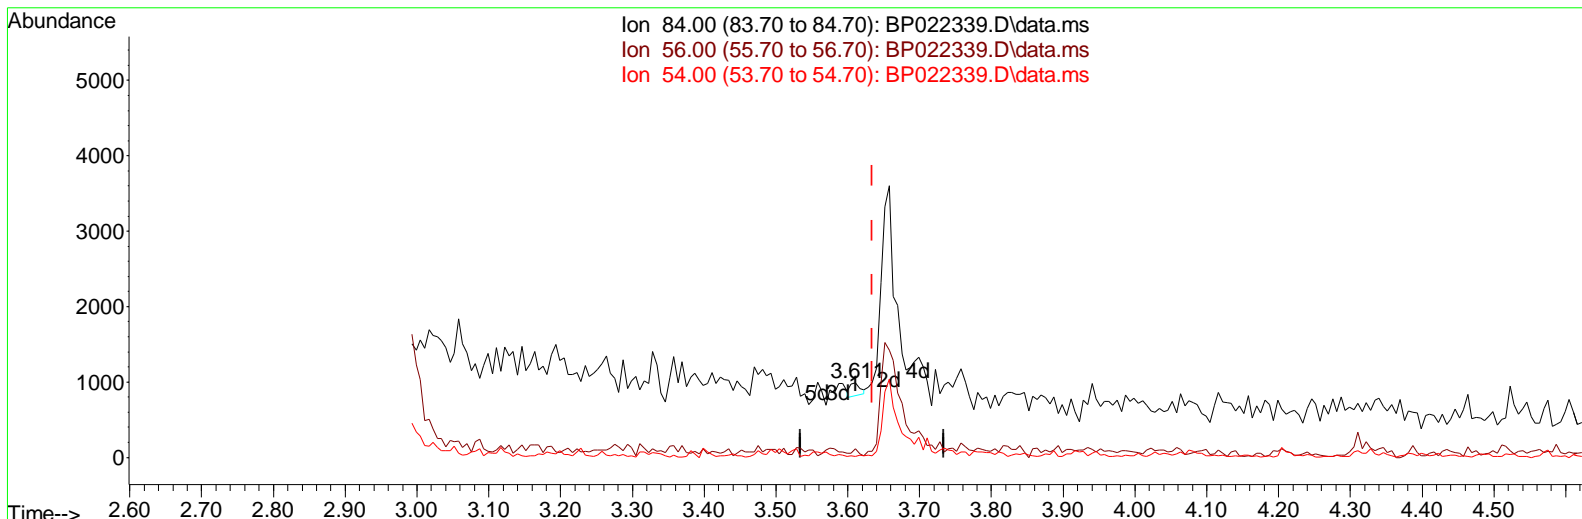

TIC: BP022339.D\data.ms

(4) Pyridine-d5 (s)

3.611min (-0.024) 0.02 ng/ul

response	171	
Ion	Exp%	Act%
84.00	100.00	100.00
56.00	61.10	11.72#
54.00	30.90	1.01#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101124\
 Data File : BP022339.D
 Acq On : 11 Oct 2024 18:11
 Operator : RC/JU
 Sample : P4237-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4F26

Manual Integrations APPROVED

Quant Time: Oct 11 18:44:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 08 02:14:47 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/14/2024
 Supervised By :mohammad ahmed 10/15/2024

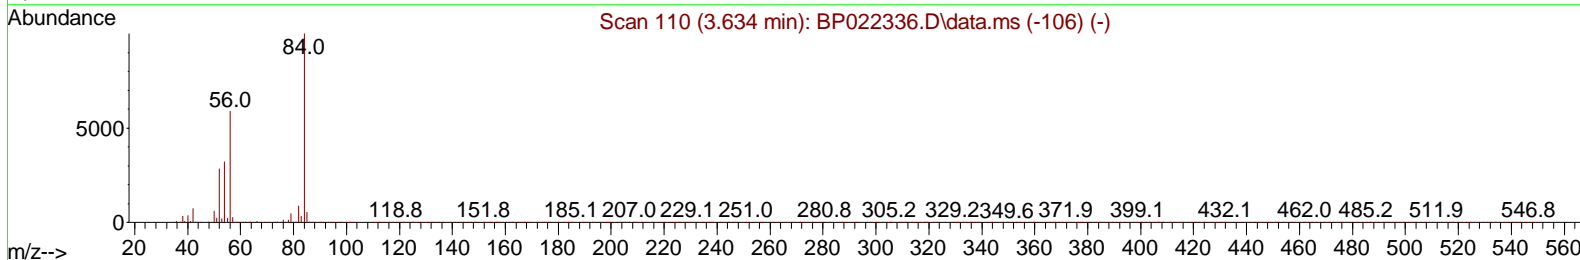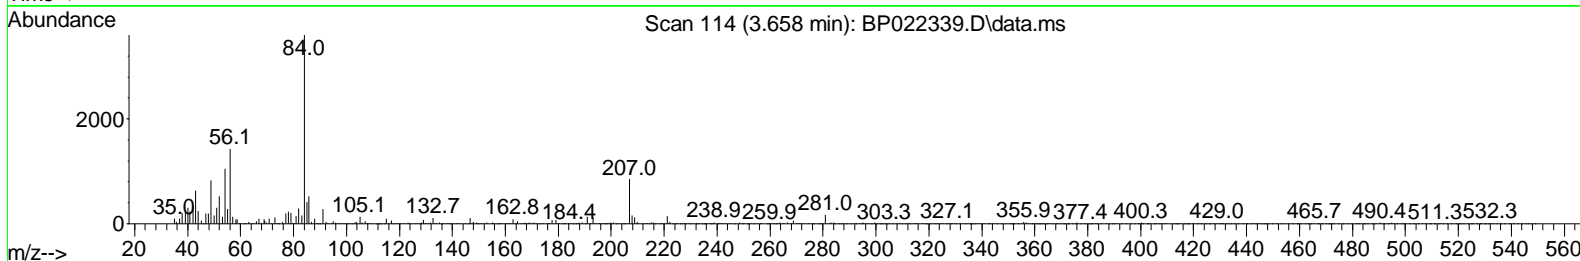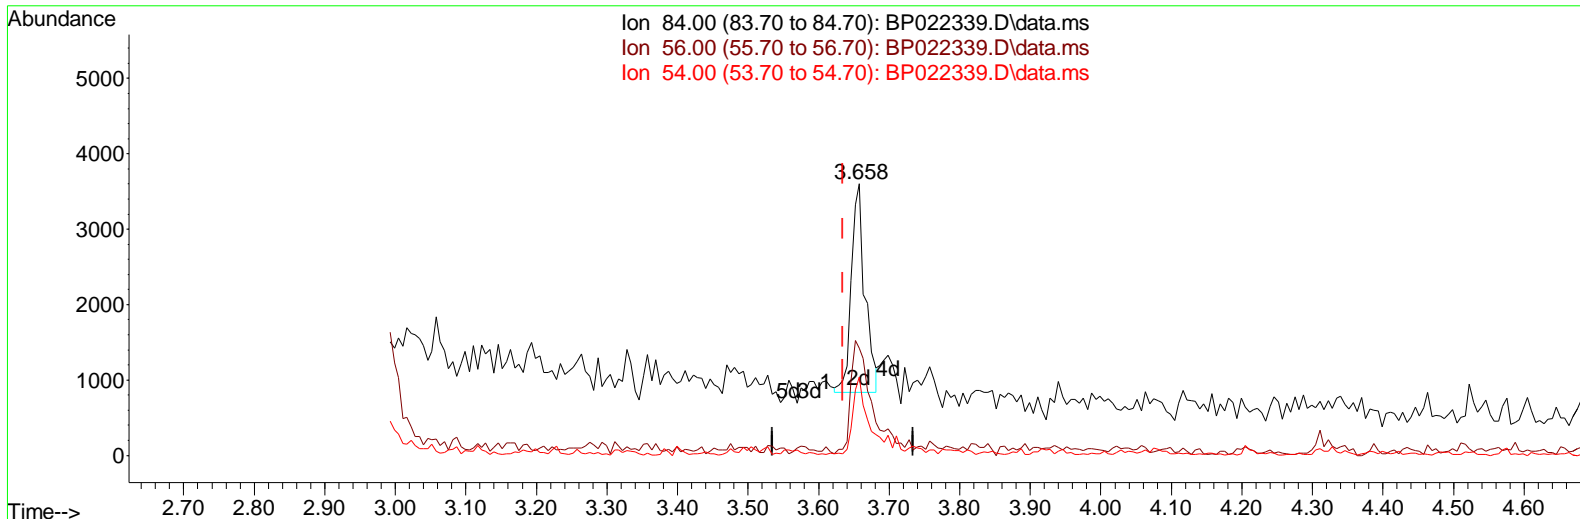

TIC: BP022339.D\data.ms

(4) Pyridine-d5 (s)

3.658min (+ 0.023) 0.52 ng/ul m

response	3757	
Ion	Exp%	Act%
84.00	100.00	100.00
56.00	61.10	39.56#
54.00	30.90	29.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101124\
 Data File : BP022339.D
 Acq On : 11 Oct 2024 18:11
 Operator : RC/JU
 Sample : P4237-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
ClientSampleId :
 A4F26

Manual Integrations APPROVED

Reviewed By : Jagrut Upadhyay 10/14/2024
 Supervised By : mohammad ahmed 10/15/2024

Quant Time: Oct 11 18:45:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 08 02:14:47 2024
 Response via : Initial Calibration

Compound	R.T.	QI on	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.704	152	101807	20.000	ng/ul	0.00
20) Naphthalene-d8	10.463	136	390090	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.322	164	309461	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.104	188	752253	20.000	ng/ul	0.00
79) Chrysene-d12	21.545	240	807116	20.000	ng/ul	0.00
88) Perylene-d12	24.839	264	948546	20.000	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.222	96	4521	1.726	ng/uL	0.00
4) Pyridine-d5	3.658	84	3757m	0.522	ng/ul	0.02
7) Phenol-d5	6.887	99	78927	9.210	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.040	67	45230	8.980	ng/ul	0.00
11) 2-Chlorophenol-d4	7.246	132	59792	9.833	ng/ul	0.00
15) 4-Methylphenol-d8	8.404	113	55900	8.174	ng/ul	0.00
21) Nitrobenzene-d5	8.846	128	28148	9.385	ng/ul	0.00
24) 2-Nitrophenol-d4	9.551	143	33257	9.577	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.098	165	71722	9.718	ng/ul	0.00
31) 4-Chloroaniline-d4	10.598	131	59303	6.800	ng/ul	0.00
46) Dimethylphthalate-d6	13.710	166	240347	9.775	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	264679	10.135	ng/ul	0.00
54) 4-Nitrophenol-d4	14.551	143	26947	6.533	ng/ul	0.02
60) Fluorene-d10	15.322	176	226240	10.608	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.439	200	28005	5.660	ng/ul	-0.01
73) Anthracene-d10	17.204	188	374051	10.570	ng/ul	-0.01
81) Pyrene-d10	19.592	212	438203	10.267	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.615	264	375120	7.405	ng/ul	0.02
Target Compounds						
16) Acetophenone	8.516	105	15652	1.386	ng/ul	99
80) Fluoranthene	19.245	202	78685	1.604	ng/ul	99
82) Pyrene	19.627	202	64332	1.223	ng/ul	98
90) Benzo(b)fluoranthene	23.792	252	62418	1.045	ng/ul #	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101124\
 Data File : BP022339.D
 Acq On : 11 Oct 2024 18:11
 Operator : RC/JU
 Sample : P4237-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4F26

Manual Integrations APPROVED

Reviewed By : Jagrut Upadhyay 10/14/2024
 Supervised By : mohammad ahmed 10/15/2024

Quant Time: Oct 11 18:45:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 08 02:14:47 2024
 Response via : Initial Calibration

