

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101124\
 Data File : BP022342.D
 Acq On : 11 Oct 2024 20:14
 Operator : RC/JU
 Sample : P4237-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4EP6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 10/14/2024
 Supervised By :mohammad ahmed 10/15/2024

Quant Time: Oct 12 01:13:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 08 02:14:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.699	152	100324	20.000	ng/u1	0.00
20) Naphthalene-d8	10.463	136	379895	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.304	164	309628	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.116	188	783563	20.000	ng/u1	0.00
79) Chrysene-d12	21.539	240	833698	20.000	ng/u1	0.00
88) Perylene-d12	24.833	264	1012644	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.222	96	2135	0.827	ng/uL	0.00
4) Pyridine-d5	3.658	84	5396m	0.761	ng/u1	0.02
7) Phenol-d5	6.893	99	27888	3.302	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.040	67	23046	4.643	ng/u1	0.00
11) 2-Chlorophenol-d4	7.246	132	27135	4.528	ng/u1	0.00
15) 4-Methylphenol-d8	8.405	113	22258	3.303	ng/u1	0.00
21) Nitrobenzene-d5	8.846	128	14761	5.053	ng/u1	0.00
24) 2-Nitrophenol-d4	9.557	143	16488	4.876	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.099	165	29017	4.037	ng/u1	0.00
31) 4-Chloroaniline-d4	10.604	131	16161	1.903	ng/u1	0.01
46) Dimethylphthalate-d6	13.710	166	122384	4.975	ng/u1	0.00
49) Acenaphthylene-d8	13.992	160	137964	5.280	ng/u1	0.00
54) 4-Nitrophenol-d4	14.557	143	5223m	1.266	ng/u1	0.03
60) Fluorene-d10	15.322	176	126030	5.906	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.445	200	12978	2.518	ng/u1	0.00
73) Anthracene-d10	17.198	188	211506	5.738	ng/u1	-0.02
81) Pyrene-d10	19.592	212	252464	5.726	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.610	264	219134	4.052	ng/u1	0.01
Target Compounds						
					Qvalue	
72) Phenanthrene	17.151	178	127647	3.045	ng/u1	99
80) Fluoranthene	19.245	202	423916	8.364	ng/u1	100
82) Pyrene	19.622	202	305832	5.630	ng/u1	99
85) Benzo(a)anthracene	21.522	228	173030	2.961	ng/u1	98
86) Bis(2-ethylhexyl)phtha...	21.457	149	39723	1.463	ng/u1	97
87) Chrysene	21.592	228	234731	4.331	ng/u1	98
90) Benzo(b)fluoranthene	23.792	252	334926	5.254	ng/u1	98
91) Benzo(k)fluoranthene	23.857	252	139085m	2.229	ng/u1	
93) Benzo(a)pyrene	24.686	252	126068	2.149	ng/u1	97
94) Indeno(1,2,3-cd)pyrene	28.556	276	127588	1.630	ng/u1	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101124\
 Data File : BP022342.D
 Acq On : 11 Oct 2024 20:14
 Operator : RC/JU
 Sample : P4237-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1


Instrument :
 BNA_P
 ClientSampleId :
 A4EP6

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 10/14/2024
 Supervised By :mohammad ahmed 10/15/2024

Quant Time: Oct 12 01:13:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 08 02:14:47 2024
 Response via : Initial Calibration

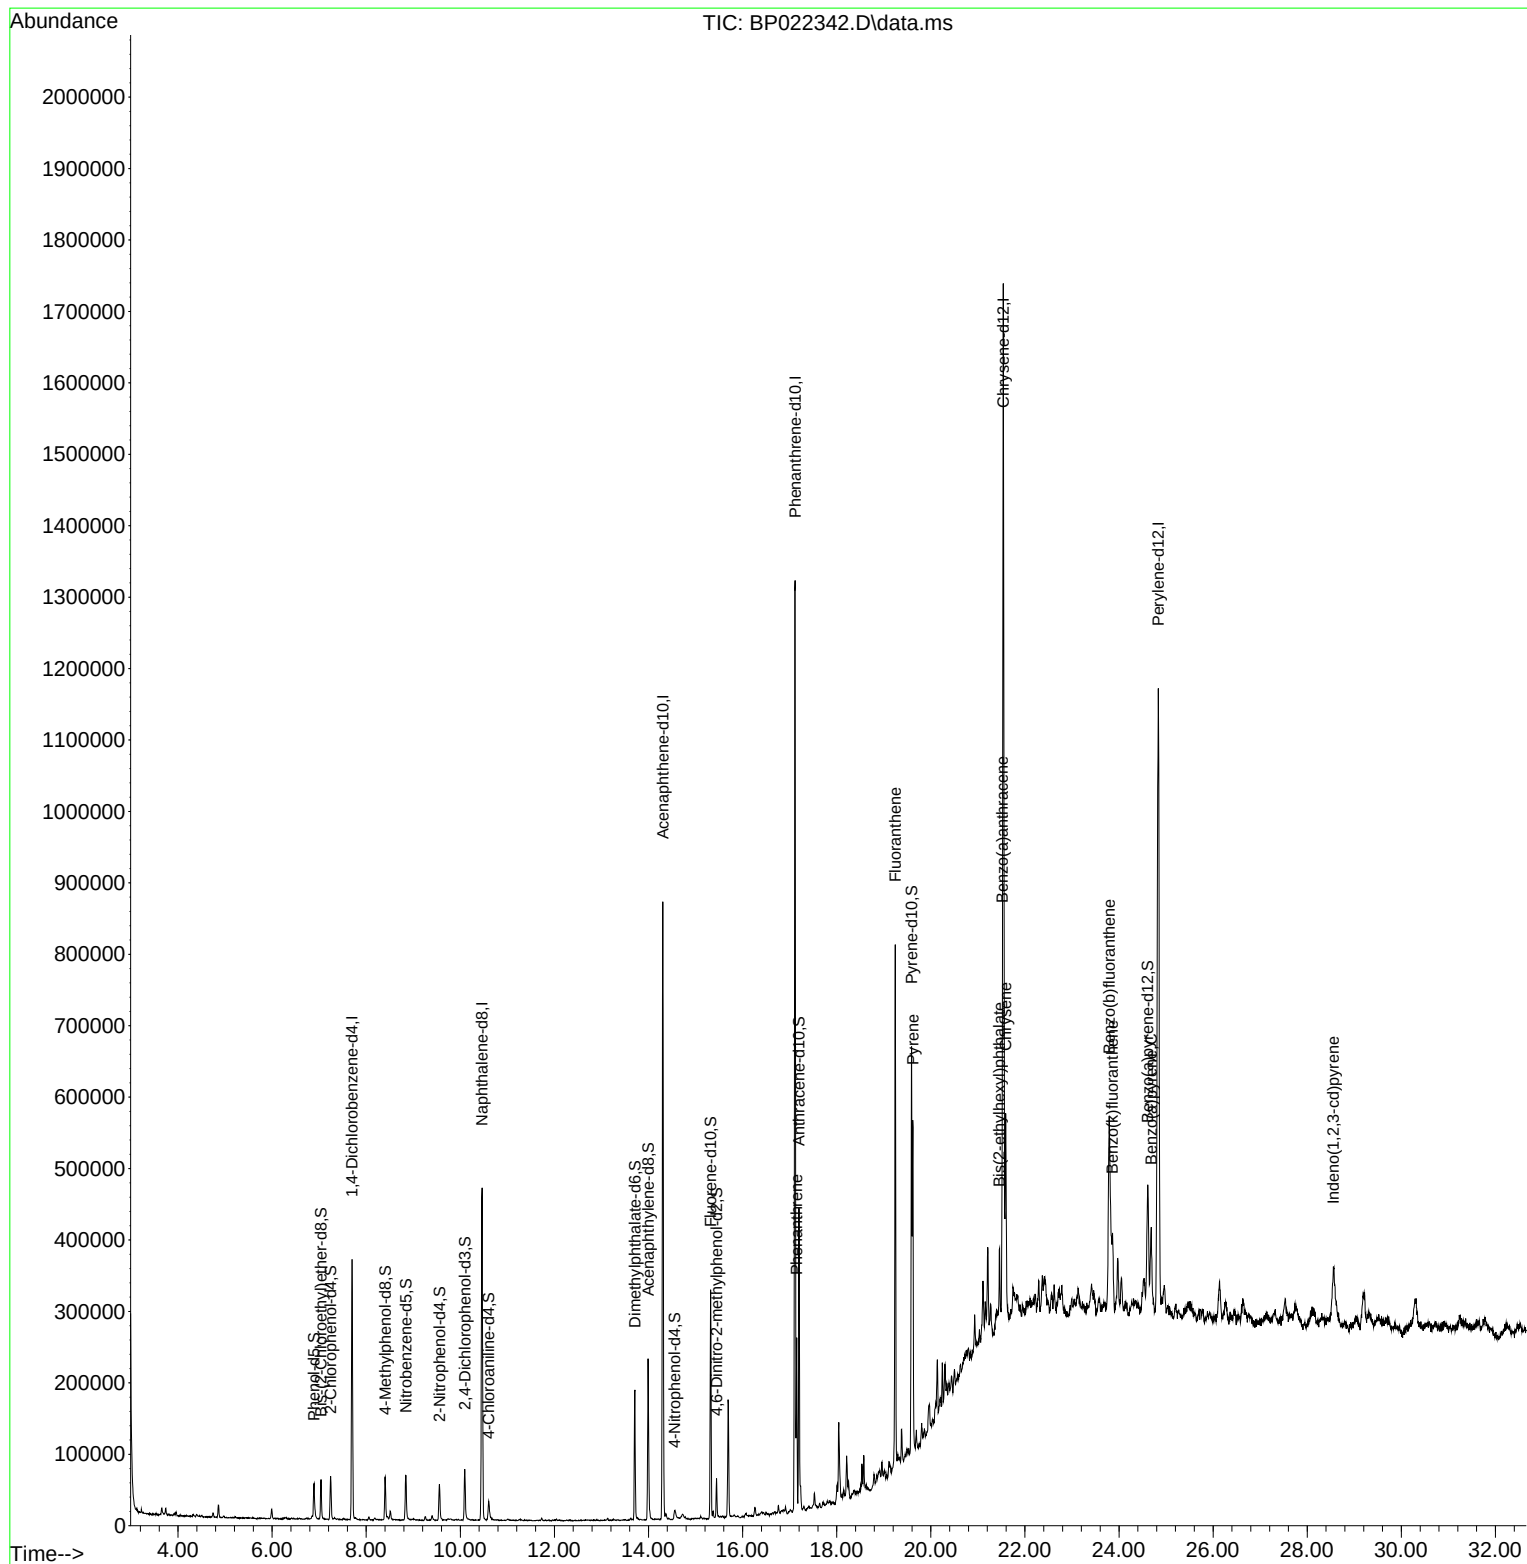

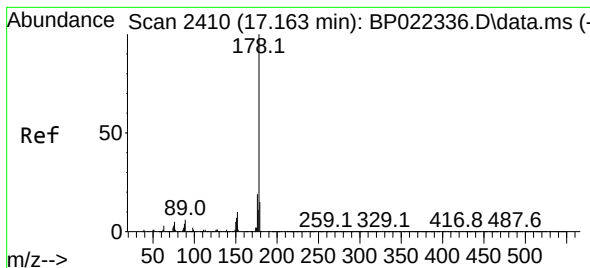

#72

Phenanthrene

Concen: 3.045 ng/ul

RT: 17.151 min Scan# 2410

Delta R.T. -0.006 min

Lab File: BP022342.D

Acq: 11 Oct 2024 20:14

Instrument :

BNA_P

ClientSampleId :





A4EP6

Tgt Ion:178	Resp: 12764
Ion Ratio	Lower Upper
178 100	
179 16.3	12.2 18.4
176 19.5	15.7 23.5

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 10/14/2024
Supervised By :mohammad ahmed 10/15/2024

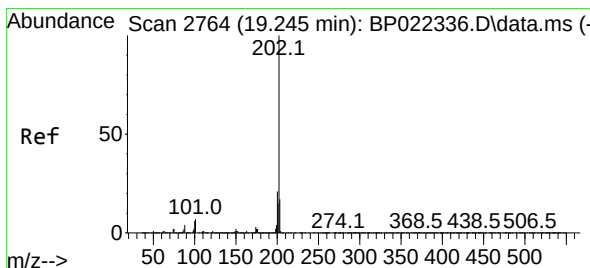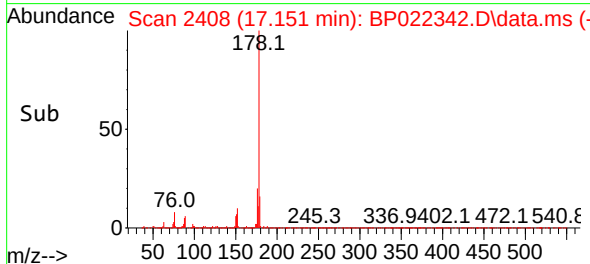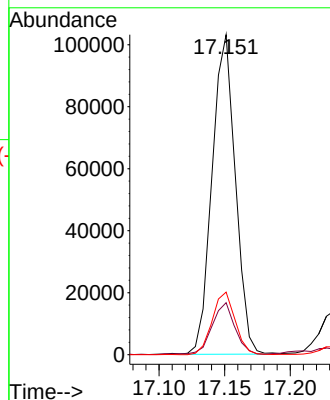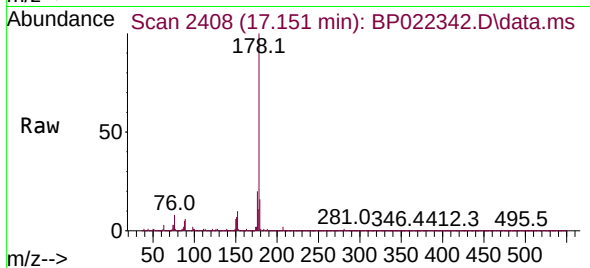

#80

Fluoranthene

Concen: 8.364 ng/ul




RT: 19.245 min Scan# 2764


Delta R.T. -0.000 min

Lab File: BP022342.D

Acq: 11 Oct 2024 20:14

Tgt Ion:202	Resp: 423916
Ion Ratio	Lower Upper
202 100	
101 7.1	5.8 8.8
100 5.5	4.5 6.7

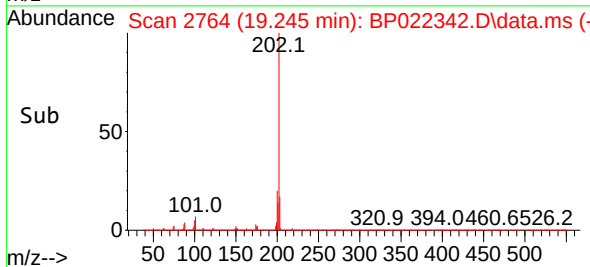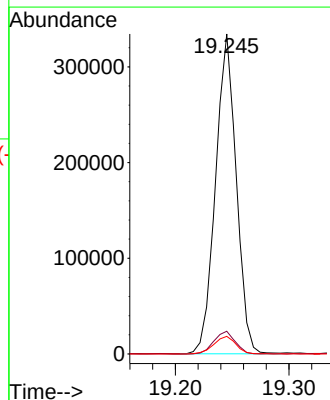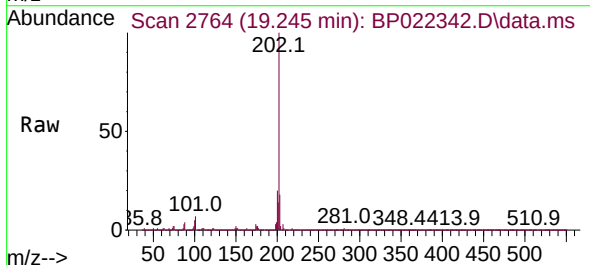



#82

Pyrene

Concen: 5.630 ng/ul

RT: 19.622 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP022342.D

Acq: 11 Oct 2024 20:14

Instrument :

BNA_P

ClientSampleId :





A4EP6

Tgt Ion:202	Resp: 30583
Ion Ratio	Lower Upper
202 100	
101 8.6	6.7 10.1
100 6.8	5.8 8.6

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 10/14/2024
Supervised By :mohammad ahmed 10/15/2024

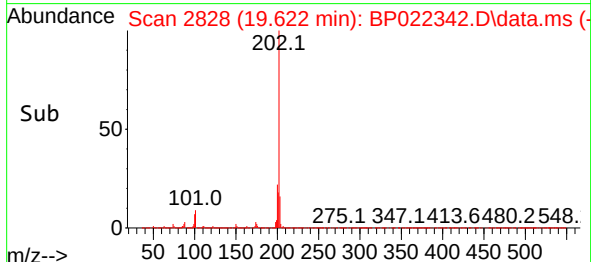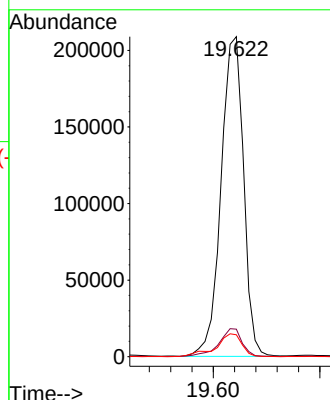

#85

Benzo(a)anthracene

Concen: 2.961 ng/ul




RT: 21.522 min Scan# 3151


Delta R.T. -0.000 min

Lab File: BP022342.D

Acq: 11 Oct 2024 20:14


Tgt Ion:228	Resp: 173030
Ion Ratio	Lower Upper
228 100	
229 20.0	15.4 23.0
226 28.2	21.5 32.3

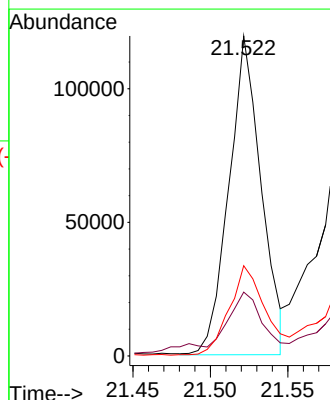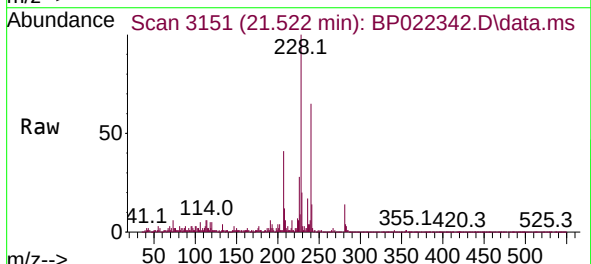

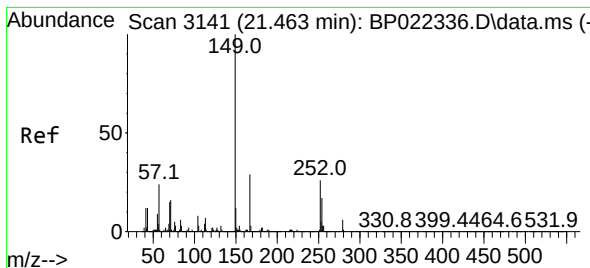

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.463 ng/ul
RT: 21.457 min Scan# 3141
Delta R.T. -0.006 min
Lab File: BP022342.D
Acq: 11 Oct 2024 20:14




Instrument :
BNA_P
ClientSampleId :
A4EP6

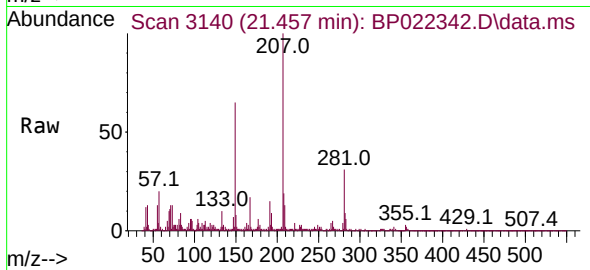

Tgt Ion:149 Resp: 3972
Ion Ratio Lower Upper
149 100
167 26.6 23.0 34.4
279 6.1 4.8 7.2




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 10/14/2024
Supervised By :mohammad ahmed 10/15/2024

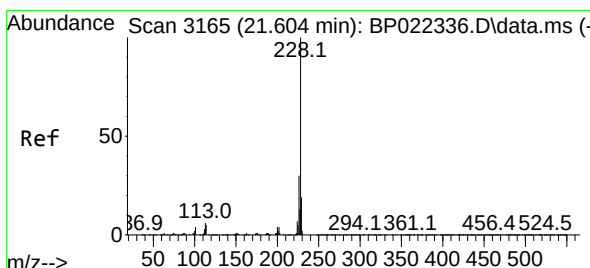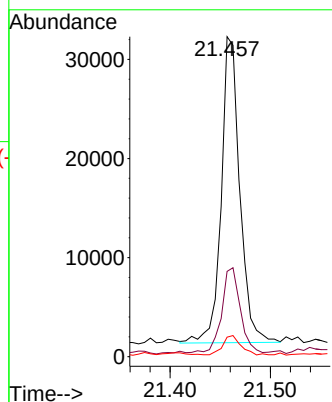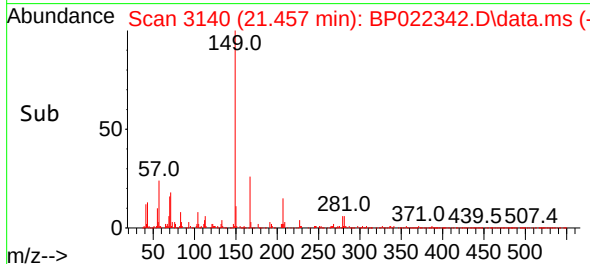

#87
Chrysene
Concen: 4.331 ng/ul
RT: 21.592 min Scan# 3163
Delta R.T. -0.000 min
Lab File: BP022342.D
Acq: 11 Oct 2024 20:14

Tgt Ion:228 Resp: 234731
Ion Ratio Lower Upper
228 100
226 30.5 23.8 35.8
229 21.1 15.5 23.3

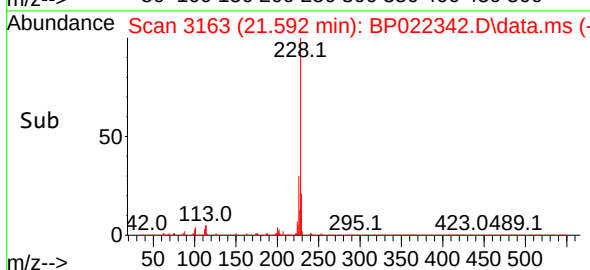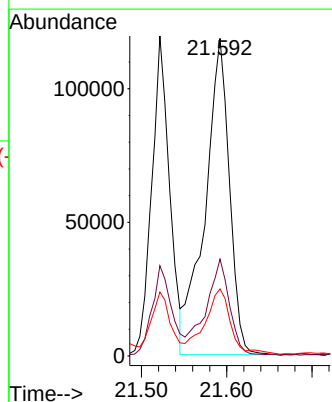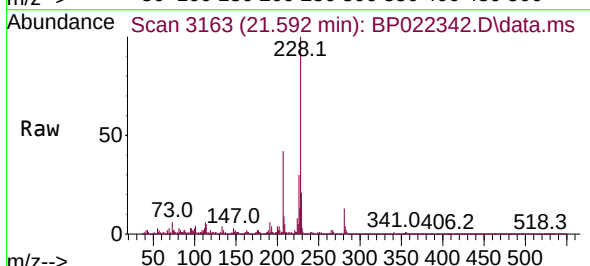



#90

Benzo(b)fluoranthene

Concen: 5.254 ng/ul

RT: 23.792 min Scan# 3537

Delta R.T. 0.006 min

Lab File: BP022342.D

Acq: 11 Oct 2024 20:14

Instrument :

BNA_P

ClientSampleId :

A4EP6





Tgt Ion:252 Resp: 334920

Ion	Ratio	Lower	Upper
252	100		
253	23.3	17.8	26.8
125	6.2	5.0	7.4

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 10/14/2024
Supervised By :mohammad ahmed 10/15/2024

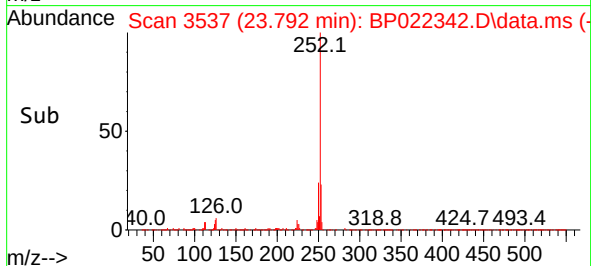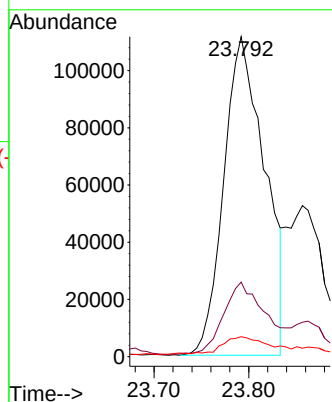

#91

Benzo(k)fluoranthene

Concen: 2.229 ng/ul m

RT: 23.857 min Scan# 3548




Delta R.T. -0.000 min


Lab File: BP022342.D

Acq: 11 Oct 2024 20:14

Tgt Ion:252 Resp: 139085

Ion	Ratio	Lower	Upper
252	100		
253	22.7	17.4	26.0
125	5.6	4.6	6.8

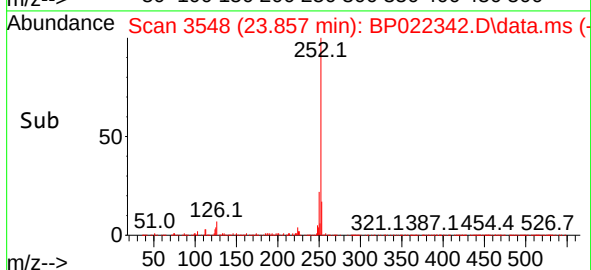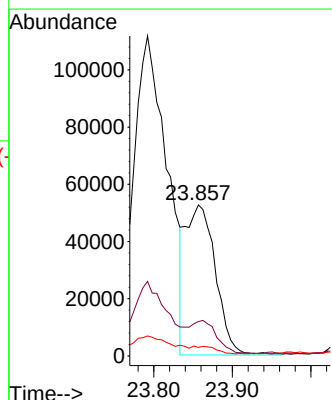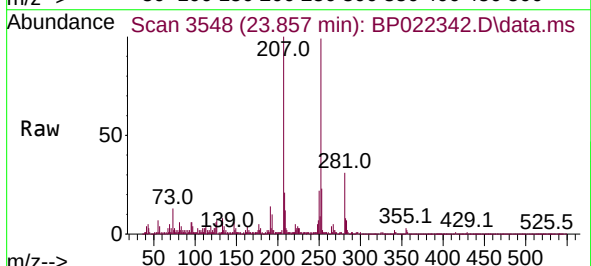



#93

Benzo(a)pyrene

Concen: 2.149 ng/ul

RT: 24.686 min Scan# 30

Delta R.T. 0.012 min

Lab File: BP022342.D

Acq: 11 Oct 2024 20:14

Instrument :

BNA_P

ClientSampleId :

A4EP6

Tgt Ion:252 Resp: 12606

Ion Ratio Lower Upper

252 100





253 23.6 17.7 26.5

125 6.9 4.9 7.3

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 10/14/2024
Supervised By :mohammad ahmed 10/15/2024

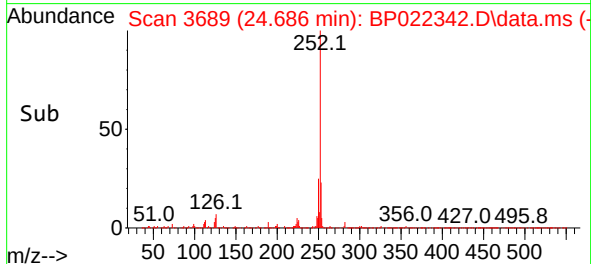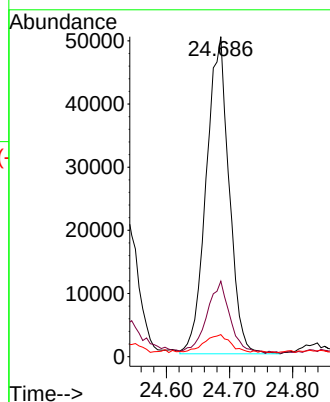

#94

Indeno(1,2,3-cd)pyrene

Concen: 1.630 ng/ul

RT: 28.556 min Scan# 4347

Delta R.T. -0.006 min

Lab File: BP022342.D

Acq: 11 Oct 2024 20:14

Tgt Ion:276 Resp: 127588

Ion Ratio Lower Upper

276 100

138 9.6 9.1 13.7

277 25.9 18.6 27.8

