

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101124\
 Data File : BP022330.D
 Acq On : 11 Oct 2024 11:42
 Operator : RC/JU
 Sample : PB163830BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK830

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022330.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	36	40	47	rBV	22685	30952	1.19%	0.118%
2	3.640	106	111	129	rBV	255697	418618	16.06%	1.592%
3	3.958	162	165	172	rVB	6366	9371	0.36%	0.036%
4	6.893	653	664	681	rBV	316753	550947	21.14%	2.095%
5	7.040	682	689	699	rVB	245584	396746	15.22%	1.509%
6	7.246	716	724	736	rBV	316524	549188	21.07%	2.088%
7	7.704	794	802	812	rBV	392320	649835	24.93%	2.471%
8	8.404	911	921	936	rBV	407973	678838	26.04%	2.581%
9	8.840	987	995	1008	rBV	306400	533406	20.46%	2.028%
10	9.251	1061	1065	1071	rVB7	2830	5136	0.20%	0.020%
11	9.557	1109	1117	1132	rBV	290449	471856	18.10%	1.794%
12	10.093	1200	1208	1220	rBV	404528	745497	28.60%	2.835%
13	10.463	1263	1271	1279	rBV	517132	856409	32.86%	3.256%
14	10.604	1287	1295	1309	rBV	400084	682507	26.18%	2.595%
15	11.734	1481	1487	1493	rVB8	2192	4550	0.17%	0.017%
16	12.051	1533	1541	1550	rVB3	5450	12133	0.47%	0.046%
17	13.710	1816	1823	1835	rBV	882394	1111216	42.63%	4.225%
18	13.992	1864	1871	1880	rBV	847586	1297170	49.77%	4.932%
19	14.310	1917	1925	1932	rBV	813356	1294407	49.66%	4.922%
20	14.522	1953	1961	1985	rBV	272041	545979	20.95%	2.076%
21	15.310	2086	2095	2104	rBV	1115915	1696853	65.10%	6.452%
22	15.439	2111	2117	2132	rBV	332060	485050	18.61%	1.844%
23	15.551	2132	2136	2145	rVB5	6664	12299	0.47%	0.047%
24	16.110	2229	2231	2238	rVB7	1658	2734	0.10%	0.010%
25	16.769	2341	2343	2349	rVB7	3056	4393	0.17%	0.017%
26	17.104	2393	2400	2409	rBV	1285417	1741048	66.80%	6.620%
27	17.204	2410	2417	2429	rVV	1296042	1990108	76.35%	7.567%
28	19.133	2741	2745	2751	rBV5	18643	25826	0.99%	0.098%
29	19.204	2753	2757	2762	rVV2	18159	26667	1.02%	0.101%
30	19.580	2816	2821	2831	rBV	1858327	2545235	97.65%	9.678%
31	21.545	3149	3155	3164	rBV2	1367495	2168929	83.21%	8.247%
32	24.604	3666	3675	3686	rVB	971491	2606503	100.00%	9.911%
33	24.827	3704	3713	3722	rVB	803407	2148431	82.43%	8.169%




Sum of corrected areas: 26298837

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101124\
Data File : BP022330.D
Acq On : 11 Oct 2024 11:42
Operator : RC/JU
Sample : PB163830BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK830

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

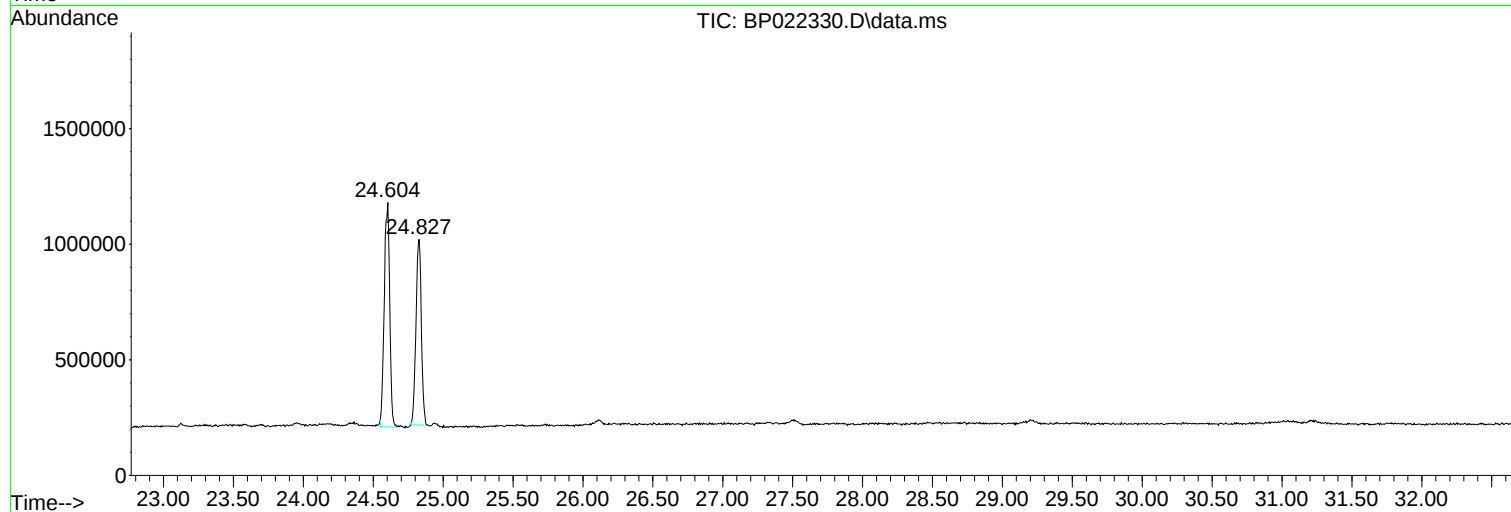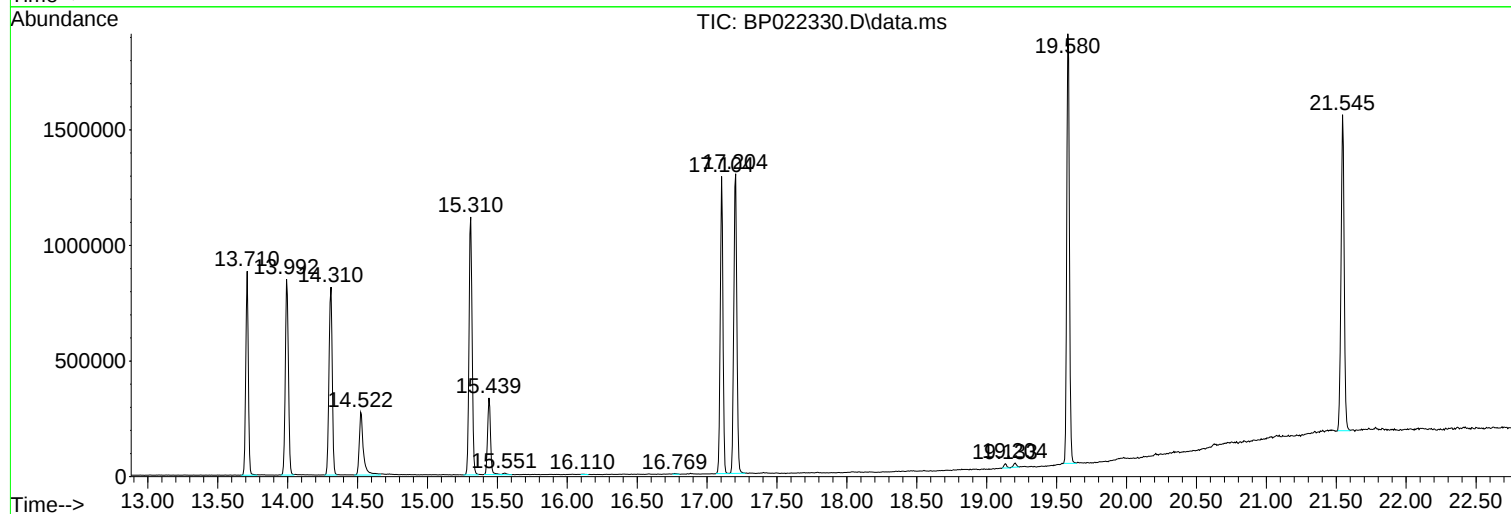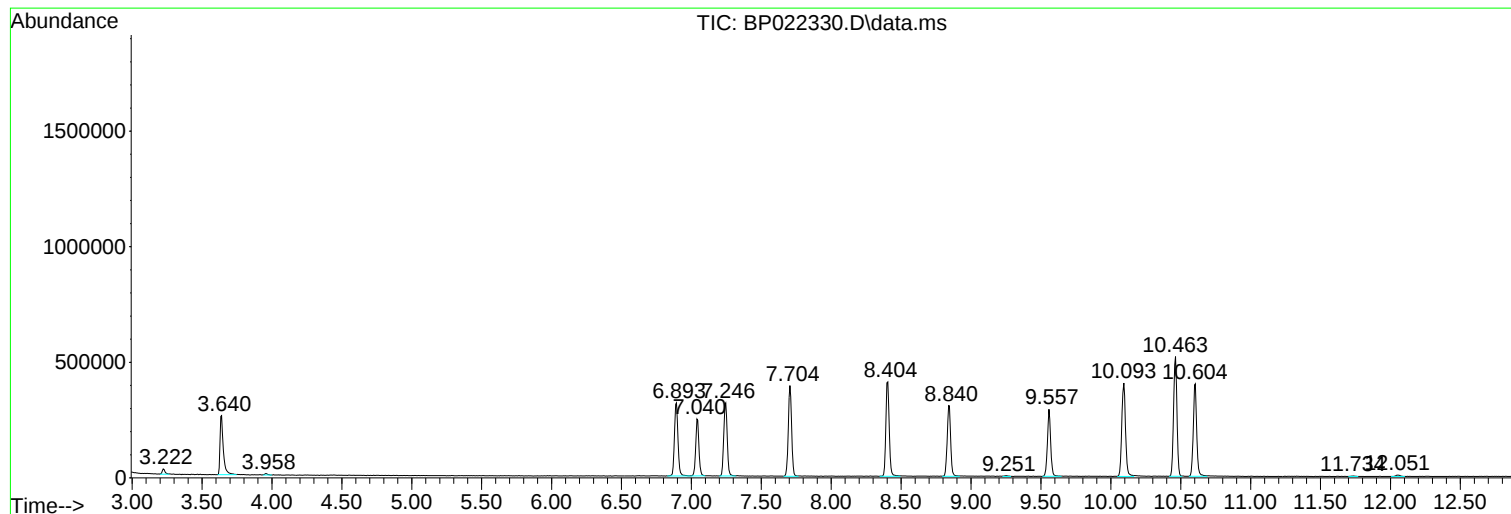

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101124\
Data File : BP022330.D
Acq On : 11 Oct 2024 11:42
Operator : RC/JU
Sample : PB163830BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK830

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101124\
Data File : BP022330.D
Acq On : 11 Oct 2024 11:42
Operator : RC/JU
Sample : PB163830BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK830

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc