

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101124\
 Data File : BP022337.D
 Acq On : 11 Oct 2024 16:49
 Operator : RC/JU
 Sample : PB163830BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK830

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022337.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	37	40	47	rVB	20857	29486	1.12%	0.118%
2	3.640	107	111	126	rVB	233741	351266	13.38%	1.410%
3	3.958	162	165	170	rVB3	4205	5926	0.23%	0.024%
4	6.893	654	664	672	rBV	276554	473493	18.04%	1.901%
5	7.040	683	689	703	rVB	204500	333622	12.71%	1.339%
6	7.246	717	724	733	rBV	290916	470097	17.91%	1.887%
7	7.699	794	801	811	rBV	342927	548387	20.89%	2.201%
8	8.399	912	920	932	rBV	361707	595835	22.70%	2.392%
9	8.599	947	954	955	rBV7	1716	2949	0.11%	0.012%
10	8.840	987	995	1006	rBV	273543	457257	17.42%	1.835%
11	9.252	1061	1065	1067	rBV5	1946	2785	0.11%	0.011%
12	9.558	1109	1117	1127	rBV	232286	406231	15.48%	1.631%
13	10.087	1199	1207	1229	rBV	371094	656581	25.01%	2.636%
14	10.457	1262	1270	1279	rVB	435093	759271	28.93%	3.048%
15	10.599	1286	1294	1314	rBV	314480	601357	22.91%	2.414%
16	11.728	1482	1486	1490	rVB7	2163	3466	0.13%	0.014%
17	12.052	1532	1541	1547	rBV3	5740	11621	0.44%	0.047%
18	13.716	1817	1824	1833	rBV	791456	1034221	39.40%	4.151%
19	13.998	1862	1872	1883	rBV	789434	1205743	45.94%	4.840%
20	14.304	1917	1924	1937	rBV	760086	1210305	46.11%	4.858%
21	14.528	1956	1962	1976	rBV	274353	524691	19.99%	2.106%
22	14.734	1995	1997	2002	rVB6	2396	3678	0.14%	0.015%
23	15.316	2088	2096	2108	rBV	1134780	1615851	61.56%	6.486%
24	15.451	2111	2119	2128	rBV	320876	472871	18.02%	1.898%
25	15.563	2133	2138	2143	rVB3	5490	10382	0.40%	0.042%
26	16.592	2307	2313	2316	rBV8	1983	3477	0.13%	0.014%
27	16.781	2340	2345	2352	rBV10	2899	5818	0.22%	0.023%
28	16.898	2362	2365	2368	rVB3	3294	4213	0.16%	0.017%
29	17.110	2394	2401	2411	rBV	1082730	1731762	65.98%	6.951%
30	17.216	2413	2419	2427	rBV	1387564	1949322	74.27%	7.825%
31	19.133	2741	2745	2752	rBV3	19419	30487	1.16%	0.122%
32	19.216	2755	2759	2764	rVV2	16664	25967	0.99%	0.104%
33	19.598	2817	2824	2834	rBV	1789617	2482496	94.58%	9.965%
34	21.551	3150	3156	3165	rBV	1419359	2116714	80.64%	8.497%
35	24.616	3668	3677	3690	rVB	936095	2624804	100.00%	10.536%
36	24.839	3707	3715	3727	rVB2	766855	2149922	81.91%	8.630%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101124\
Data File : BP022337.D
Acq On : 11 Oct 2024 16:49
Operator : RC/JU
Sample : PB163830BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK830

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 24912354

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101124\
Data File : BP022337.D
Acq On : 11 Oct 2024 16:49
Operator : RC/JU
Sample : PB163830BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK830

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

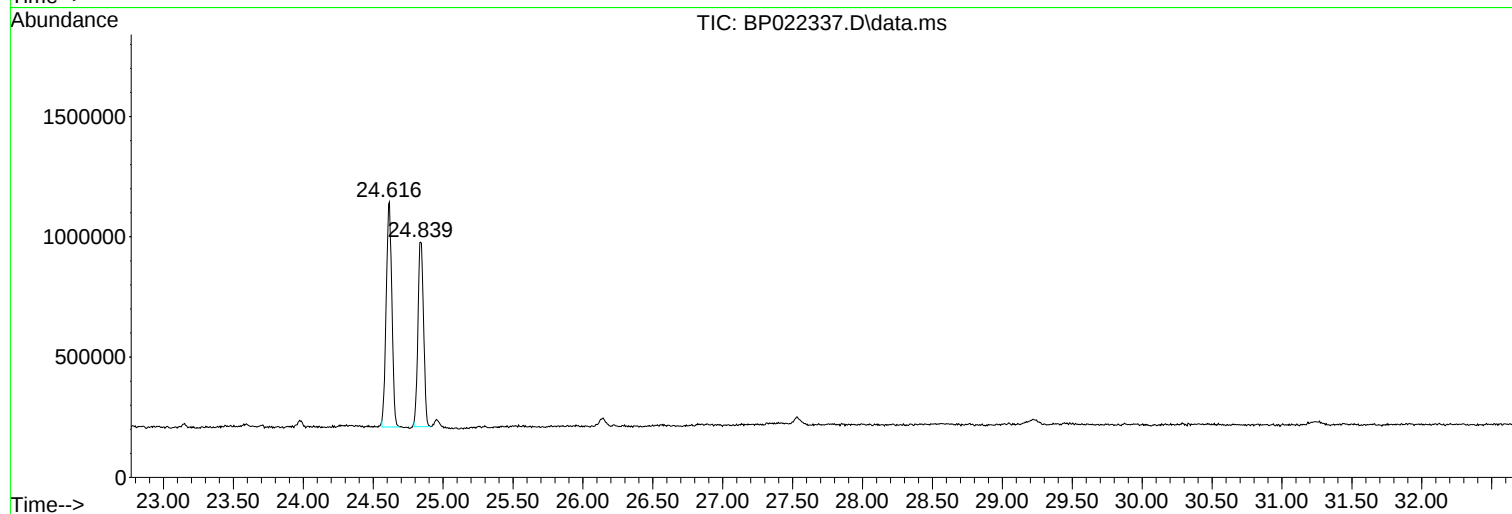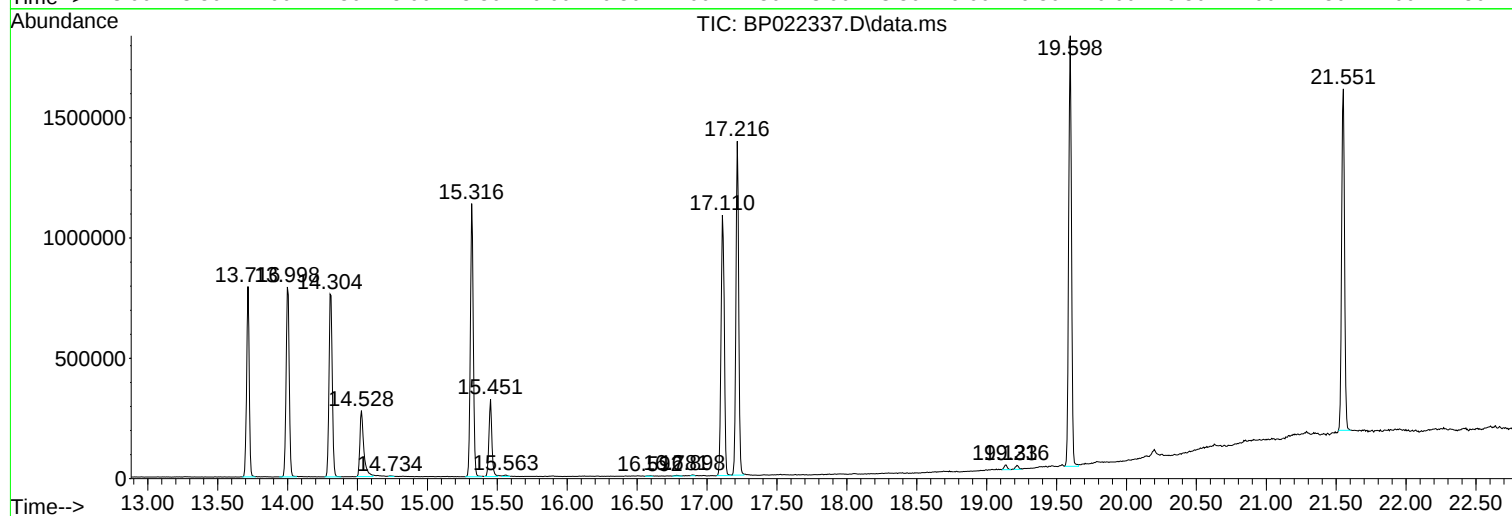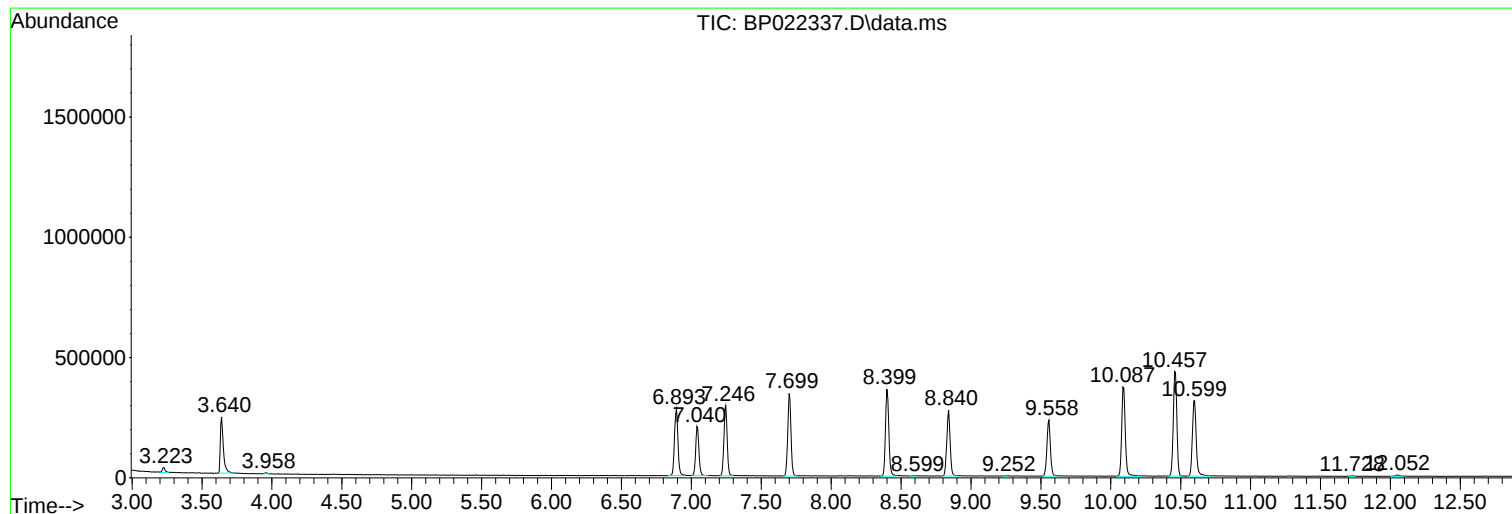

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101124\
Data File : BP022337.D
Acq On : 11 Oct 2024 16:49
Operator : RC/JU
Sample : PB163830BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK830

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101124\
Data File : BP022337.D
Acq On : 11 Oct 2024 16:49
Operator : RC/JU
Sample : PB163830BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK830

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc