
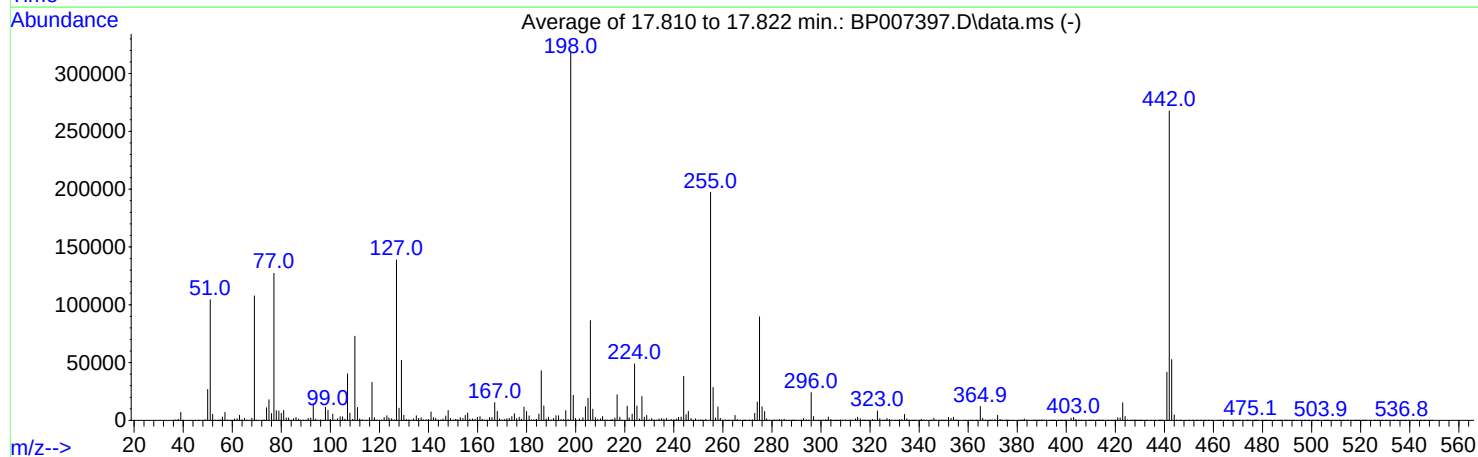


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101321\
 Data File : BP007397.D
 Acq On : 13 Oct 2021 10:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 13 14:54:20 2021

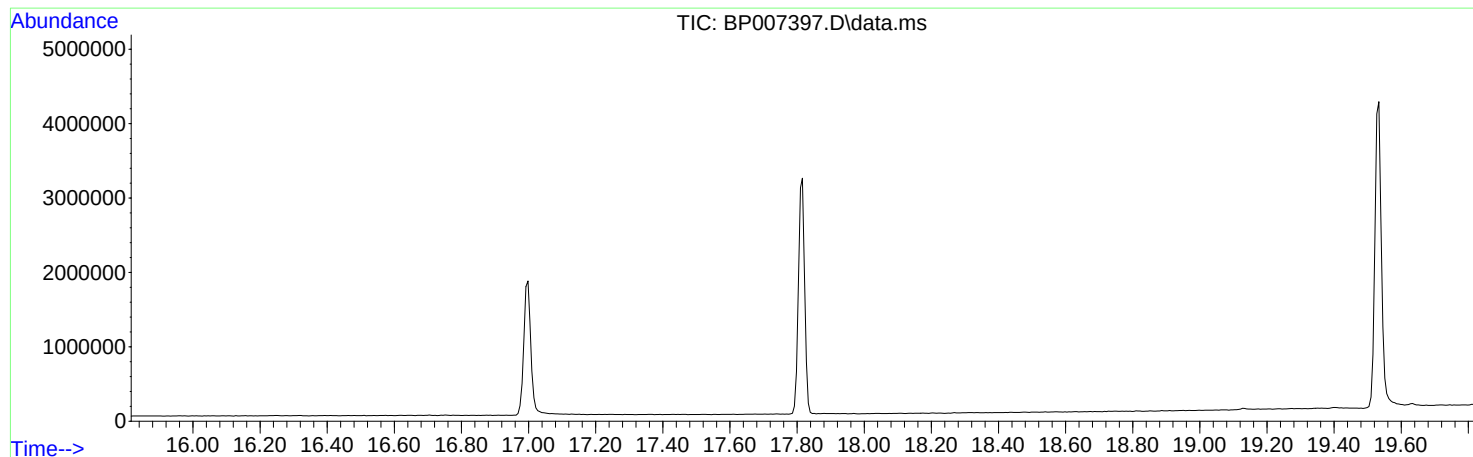




AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	104307	PASS
68	69	0.00	2	1.8	1899	PASS
69	198	0.00	100	33.9	107746	PASS
70	69	0.00	2	0.3	350	PASS
127	198	10	80	43.6	138866	PASS
197	198	0.00	2	0.2	724	PASS
198	198	100	100	100.0	318216	PASS
199	198	5	9	6.8	21760	PASS
275	198	10	60	28.1	89516	PASS
365	198	1	100	3.8	11993	PASS
441	198	0.01	100	13.1	41627	PASS
442	442	100	100	100.0	267669	PASS
443	442	15	24	19.7	52610	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101321\
Data File : BP007397.D
Acq On : 13 Oct 2021 10:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 14 04:42:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 14:54:20 2021
Response via : Initial Calibration

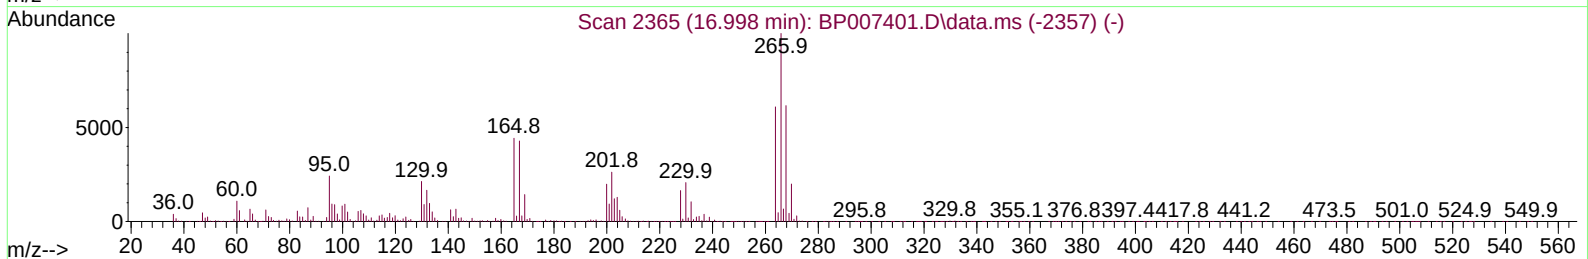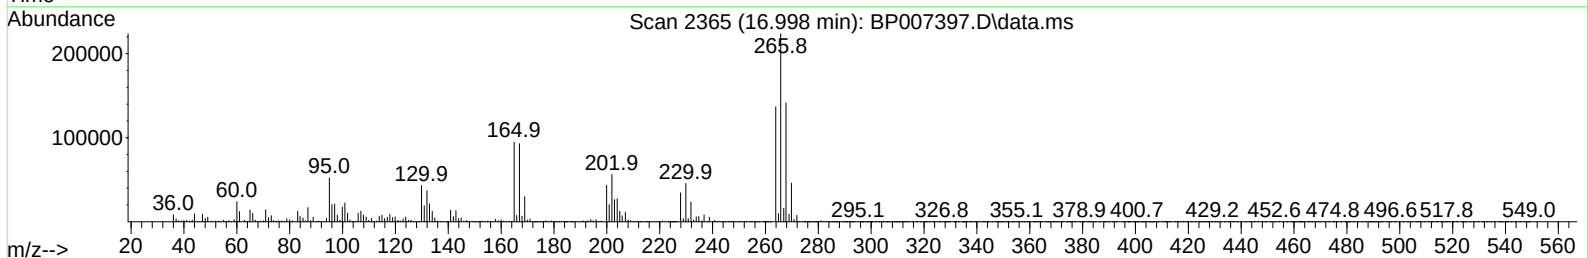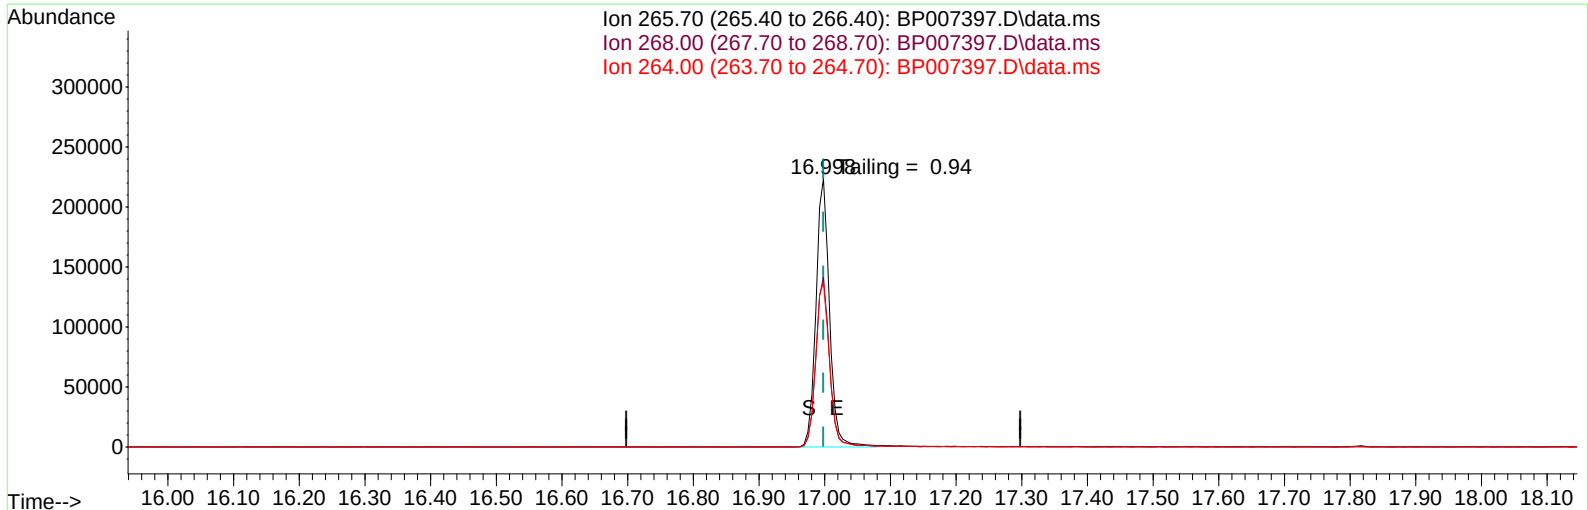

TIC: BP007397.D\data.ms

(70) Pentachlorophenol (C)

16.998min (+ 0.000) 2340004.81 ng




response 322723

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	63.32
264.00	60.90	61.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101321\
Data File : BP007397.D
Acq On : 13 Oct 2021 10:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 14 04:42:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 14:54:20 2021
Response via : Initial Calibration

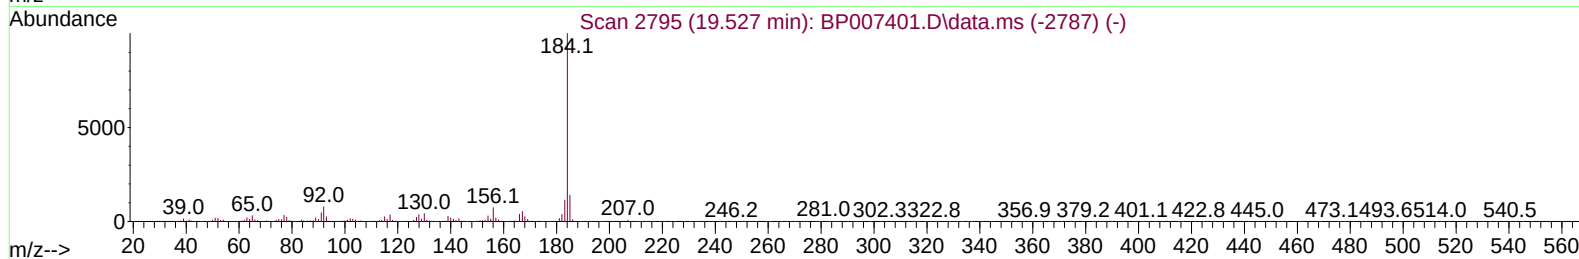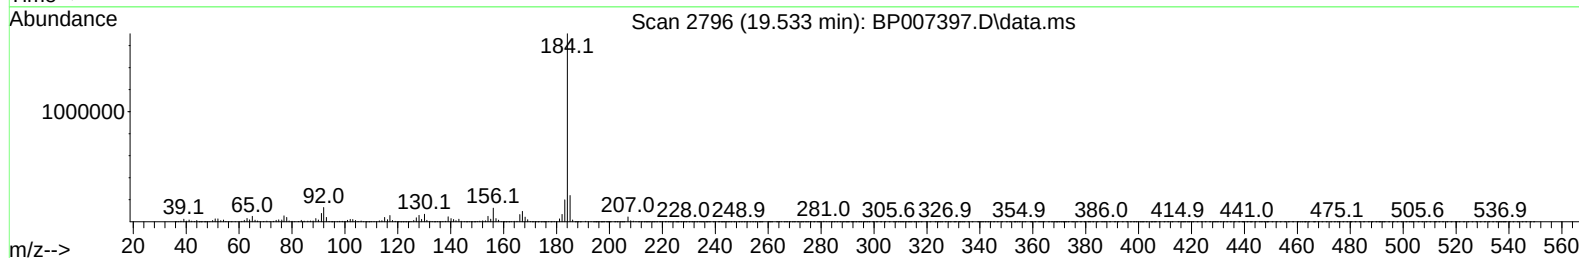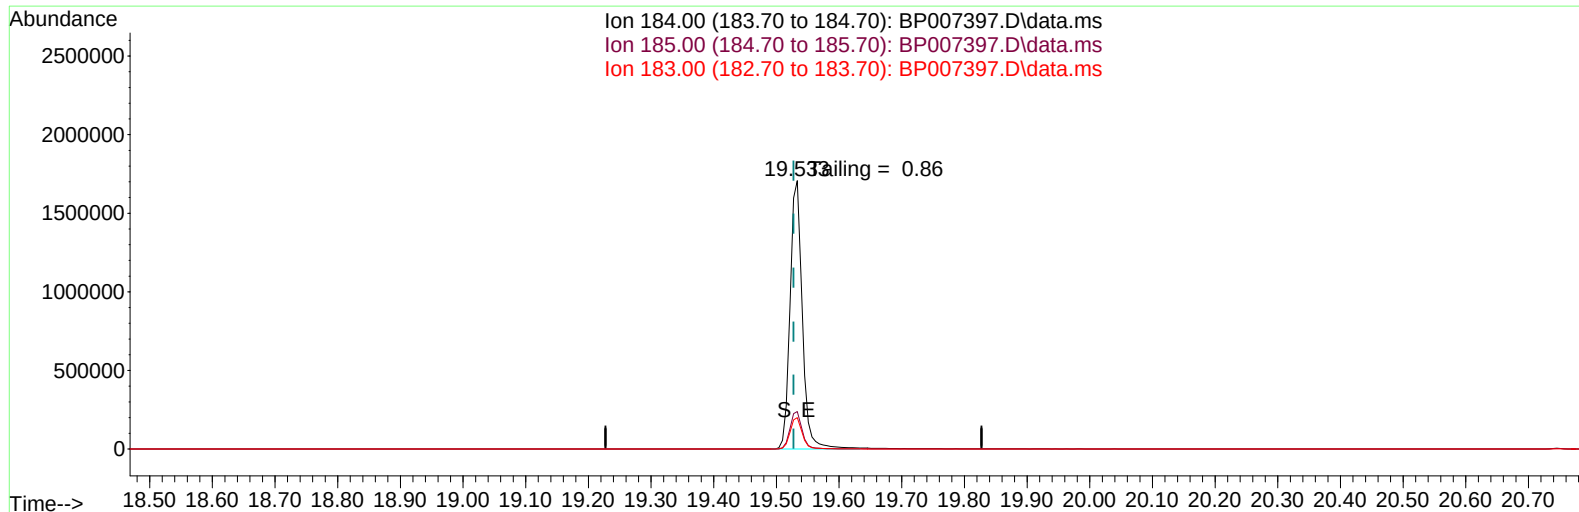

TIC: BP007397.D\data.ms

(77) Benzidine

19.533min (+ 0.006) 801167.14 ng

response 2352860

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.99
183.00	11.40	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/13/2021	BNA_P	BP007397.D
Compound Name	Response	Retention Time
DDT	988205	20.745
DDD	8160	20.369
DDE	833	19.816
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8993	997198	0.90

Instrument :
BNA_P
ClientSampleId :
DFTPP