
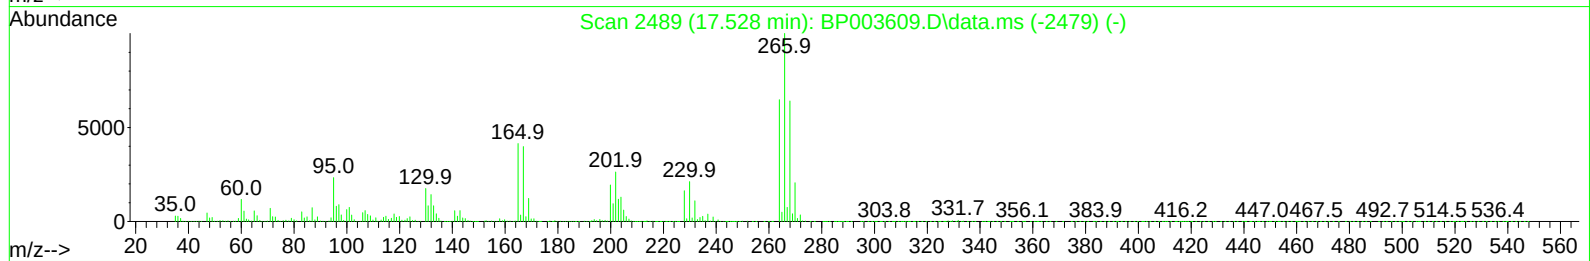
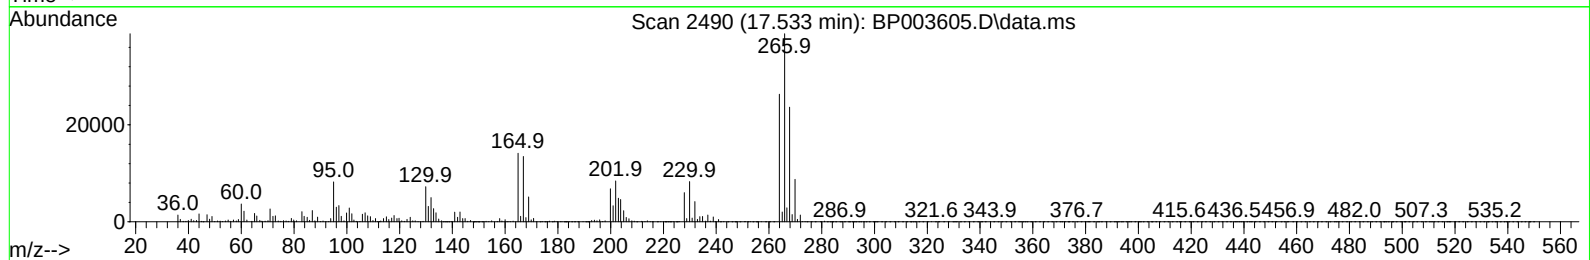


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101420\
Data File : BP003605.D
Acq On : 14 Oct 2020 11:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 15 03:02:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 14 17:03:23 2020
Response via : Initial Calibration

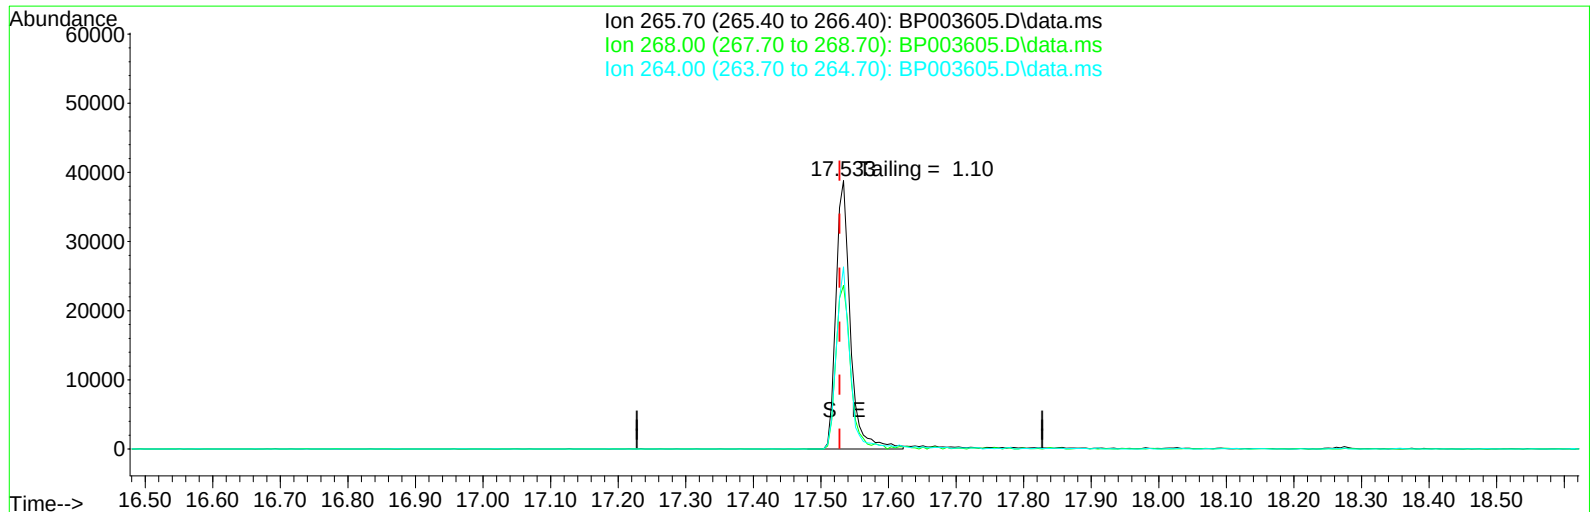

TIC: BP003605.D\data.ms

(70) Pentachlorophenol (C)




17.533min (+ 0.006) 932579.33 ng

response 57242

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	60.94
264.00	63.30	67.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101420\
Data File : BP003605.D
Acq On : 14 Oct 2020 11:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 15 03:02:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 14 17:03:23 2020
Response via : Initial Calibration

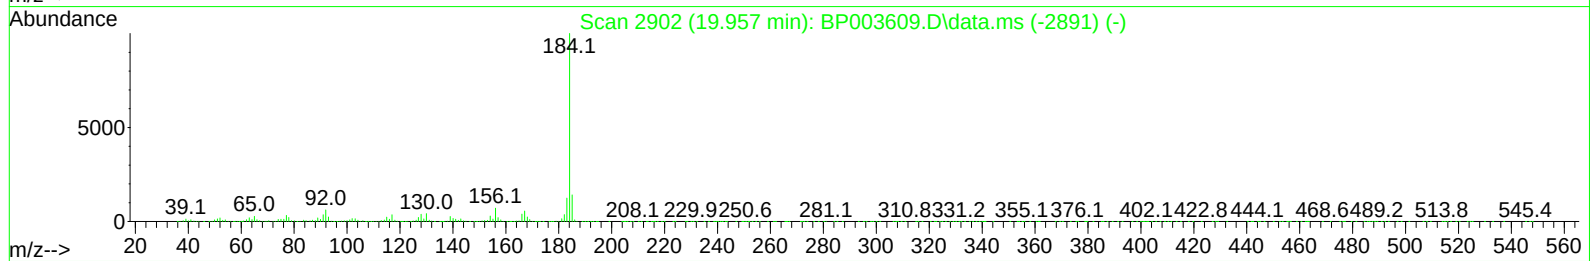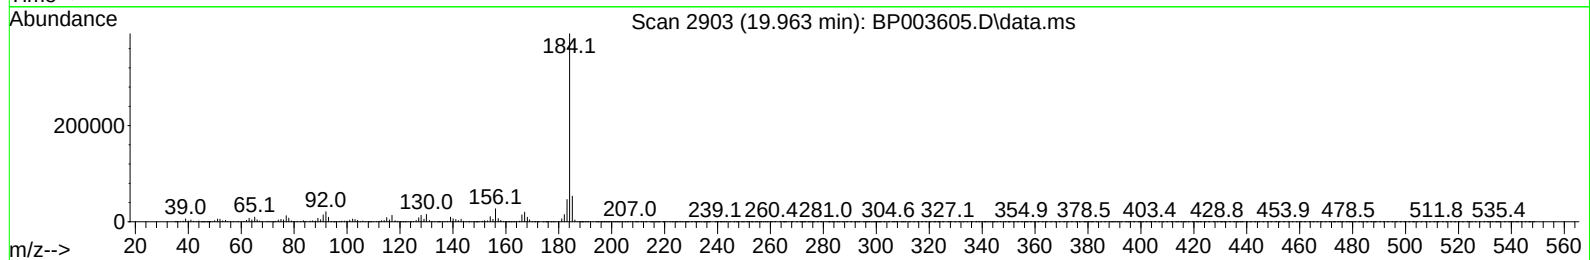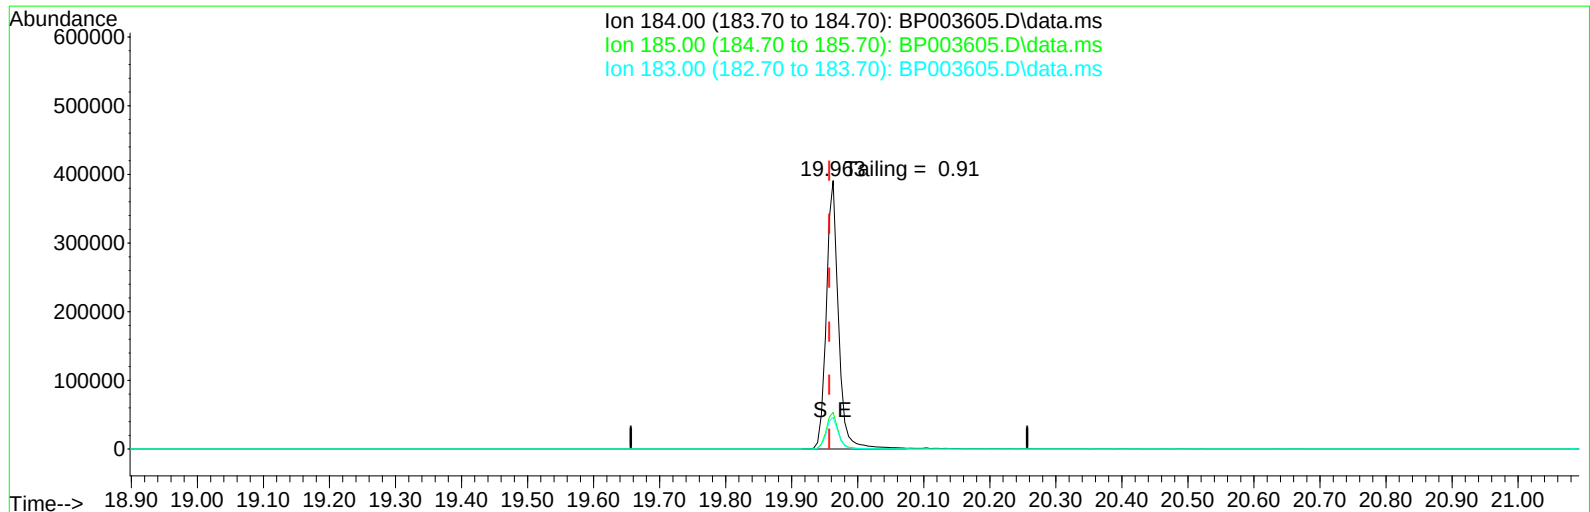

TIC: BP003605.D\data.ms

(77) Benzidine**19.963min (+ 0.006) 763559.50 ng****response 501202**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.65
183.00	12.00	11.81
0.00	0.00	0.00