
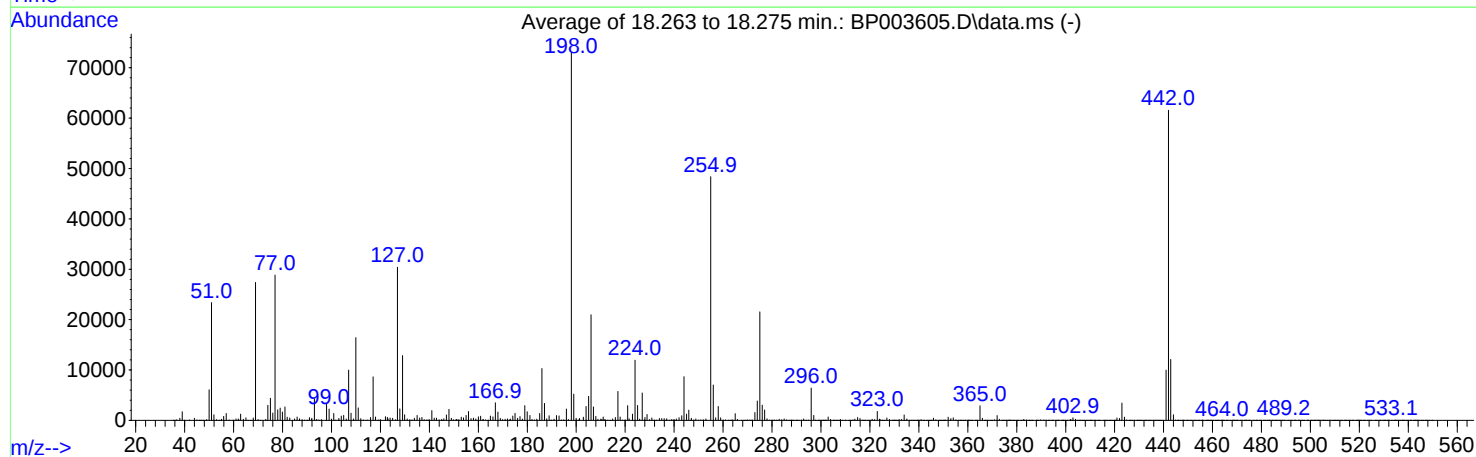


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101420\
 Data File : BP003605.D
 Acq On : 14 Oct 2020 11:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 14 17:03:23 2020

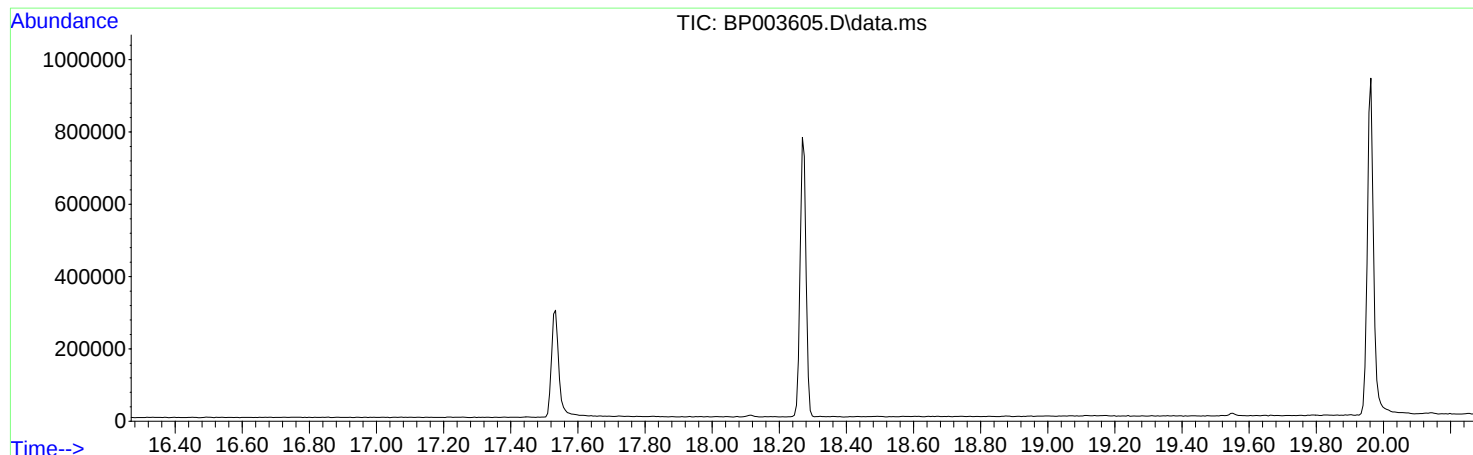

AutoFind: Scans 2614, 2615, 2616; Background Corrected with Scan 2606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	23392	PASS
68	69	0.00	2	1.8	488	PASS
69	198	0.00	100	37.5	27392	PASS
70	69	0.00	2	0.6	175	PASS
127	198	10	80	41.6	30412	PASS
197	198	0.00	2	0.2	161	PASS
198	198	100	100	100.0	73035	PASS
199	198	5	9	7.1	5218	PASS
275	198	10	60	29.5	21542	PASS
365	198	1	100	3.9	2879	PASS
441	198	0.01	100	13.7	9971	PASS
442	198	50	100	84.3	61579	PASS
443	442	15	24	19.7	12105	PASS