


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
Data File : BP007442.D
Acq On : 15 Oct 2021 13:11
Operator : CG/JU
Sample : M4126-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC8

Manual Integrations
APPROVED

mohammad
10/18/2021 10:31:06 AM

Quant Time: Oct 15 14:18:40 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 14 13:04:52 2021
Response via : Initial Calibration

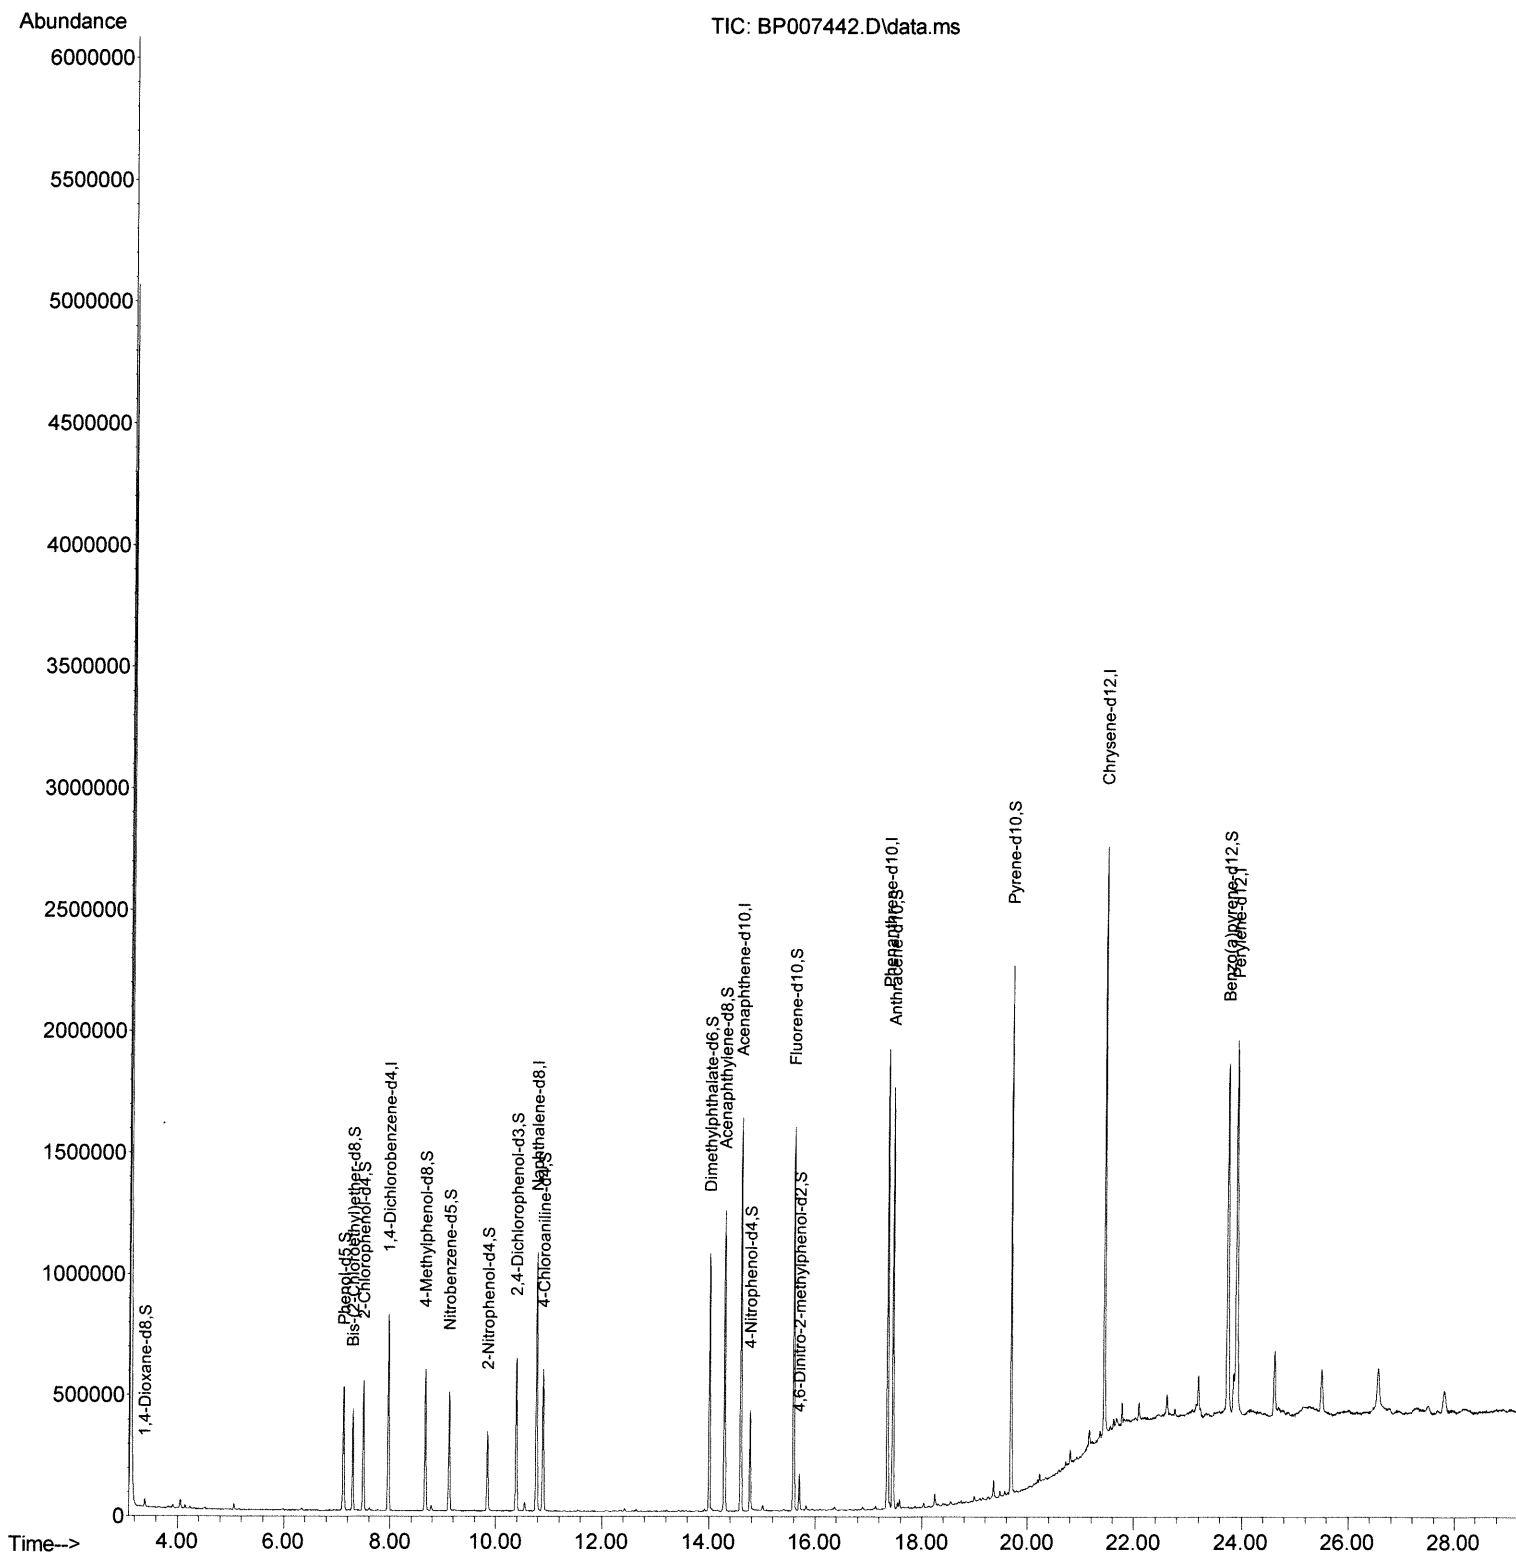




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
 Data File : BP007442.D
 Acq On : 15 Oct 2021 13:11
 Operator : CG/JU
 Sample : M4126-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC8

Manual Integrations
 APPROVED

mohammad
 10/18/2021 10:31:06 AM

Quant Time: Oct 15 14:18:40 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 14 13:04:52 2021
 Response via : Initial Calibration

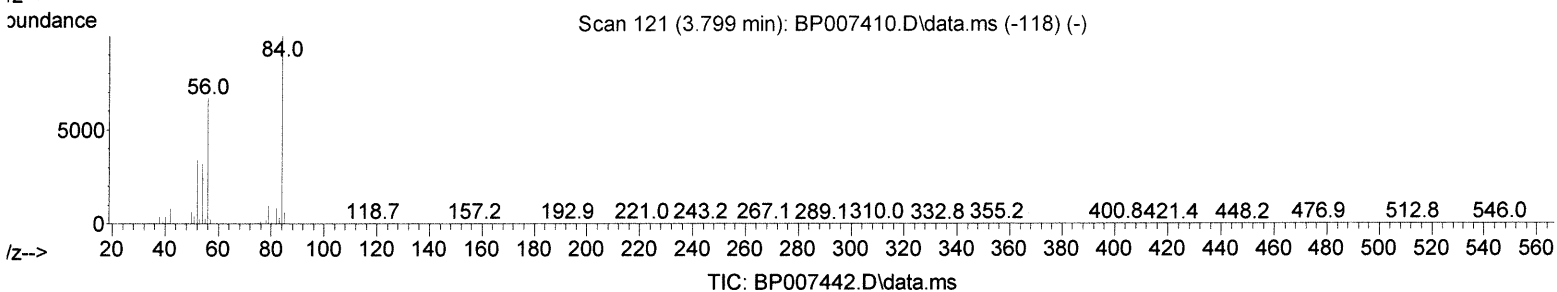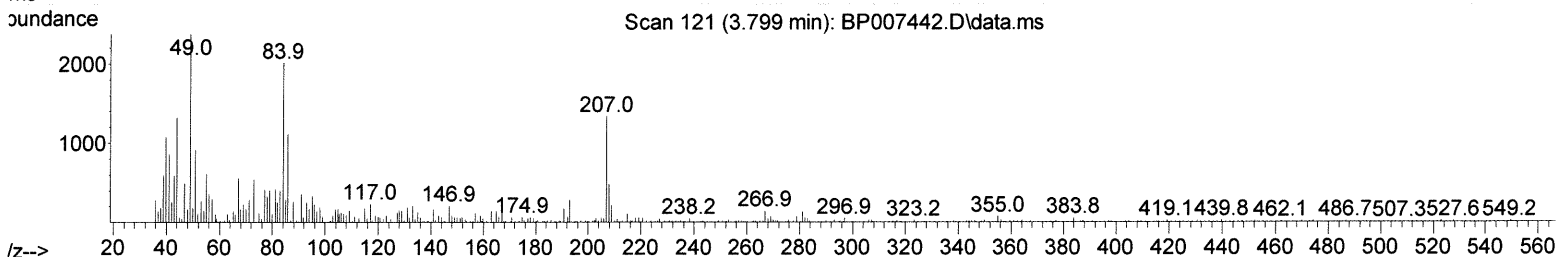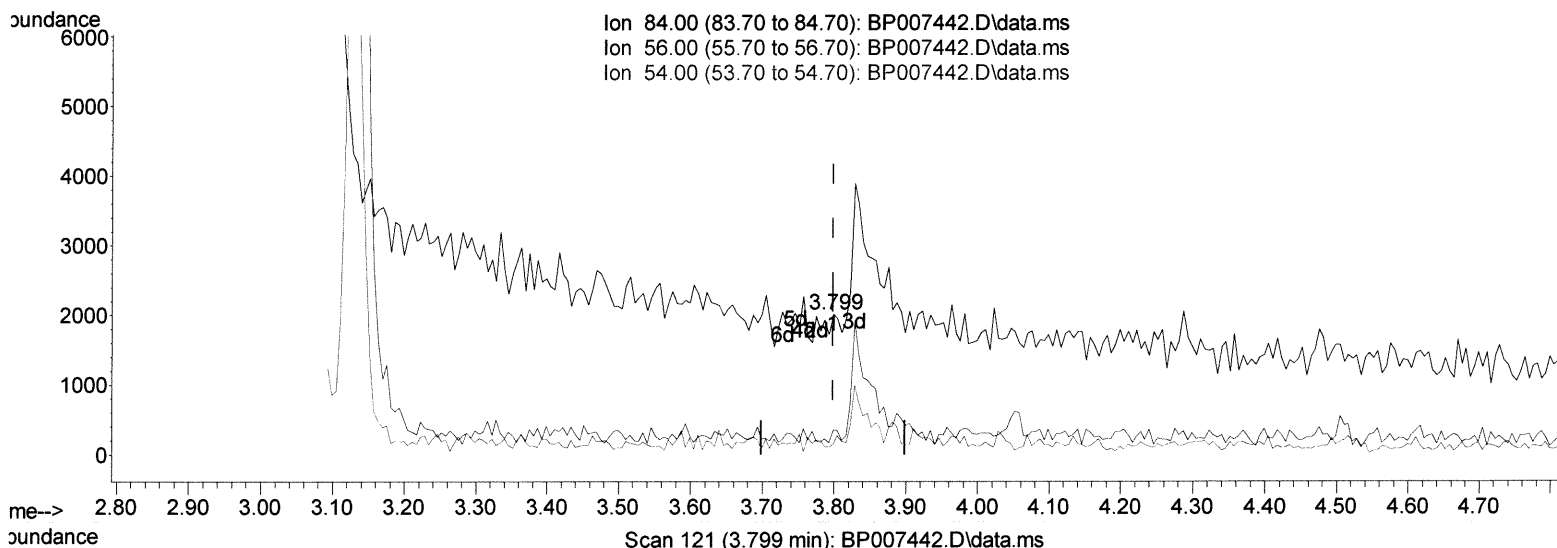

(4) Pyridine-d5 (S)

3.799min (-0.000) 0.01 ng/ul

response 200

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	66.30	17.48#
54.00	31.70	7.45#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
 Data File : BP007442.D
 Acq On : 15 Oct 2021 13:11
 Operator : CG/JU
 Sample : M4126-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC8

Manual Integrations
 APPROVED

mohammad
 10/18/2021 10:31:06 AM

Quant Time: Oct 15 14:18:40 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 14 13:04:52 2021
 Response via : Initial Calibration

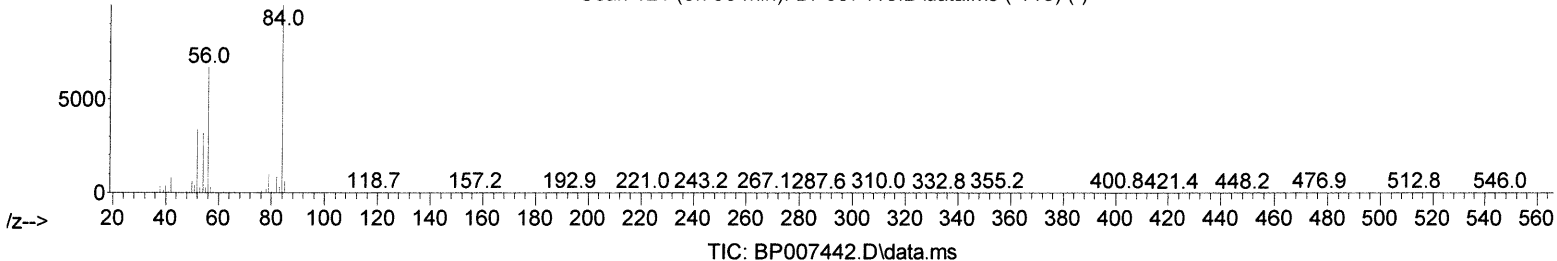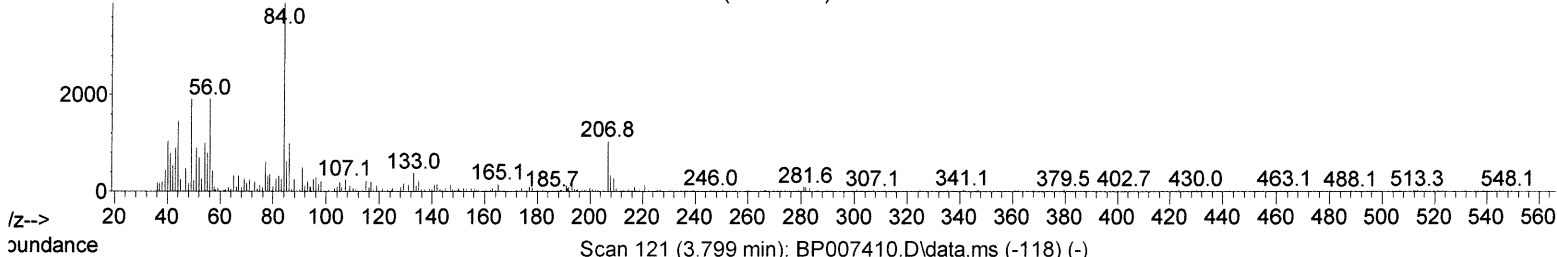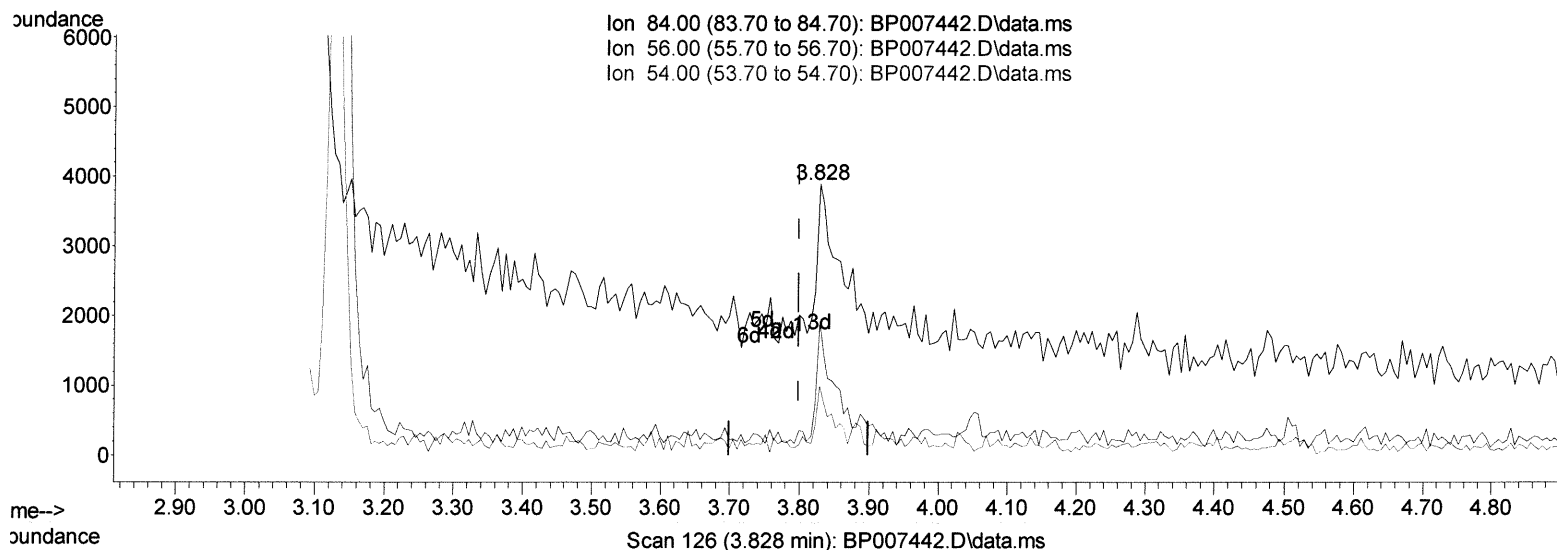

(4) Pyridine-d5 (S)

3.828min (+ 0.029) 0.31 ng/ul m

response 4824

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	66.30	49.09#
54.00	31.70	25.69
0.00	0.00	0.00

34 10/19/21

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
Data File : BP007442.D
Acq On : 15 Oct 2021 13:11
Operator : CG/JU
Sample : M4126-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC8

Manual Integrations
APPROVED
mohammad
10/18/2021 10:31:06 AM

Quant Time: Oct 15 14:18:40 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
Last Update : Thu Oct 14 13:04:52 2021
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	221227	20.000	ng/ul	0.00
20) Naphthalene-d8	10.769	136	884160	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.598	164	551569	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.351	188	1144581	20.000	ng/ul	0.00
79) Chrysene-d12	21.439	240	1151580	20.000	ng/ul	0.00
88) Perylene-d12	23.898	264	1174712	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	17981	3.210	ng/uL	0.00
4) Pyridine-d5	3.828	84	4824m	0.315	ng/ul	0.03
7) Phenol-d5	7.122	99	302653	17.518	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	181076	17.573	ng/ul	0.00
11) 2-Chlorophenol-d4	7.493	132	236467	17.398	ng/ul	0.00
15) 4-Methylphenol-d8	8.663	113	224000	16.832	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	114527	20.468	ng/ul	0.00
24) 2-Nitrophenol-d4	9.845	143	110957	21.230	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	236436	18.547	ng/ul	0.00
31) 4-Chloroaniline-d4	10.898	131	310356	18.004	ng/ul	0.00
46) Dimethylphthalate-d6	14.004	166	711808	18.653	ng/ul	-0.01
49) Acenaphthylene-d8	14.286	160	885925	18.473	ng/ul	0.00
54) 4-Nitrophenol-d4	14.775	143	90063	14.709	ng/ul	0.00
60) Fluorene-d10	15.592	176	623384	19.521	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.698	200	32393	7.063	ng/ul	0.00
73) Anthracene-d10	17.451	188	960390	19.758	ng/ul	0.00
81) Pyrene-d10	19.680	212	1132439	19.671	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.739	264	1174952	20.101	ng/ul	0.00

2010/19/21

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed