

Quantitation Report (QT Reviewed)


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
 Data File : BP007443.D
 Acq On : 15 Oct 2021 14:53
 Operator : CG/JU
 Sample : M4181-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B11

Quant Time: Oct 15 15:45:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 14 13:04:52 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 10/18/2021 10:31:09 AM

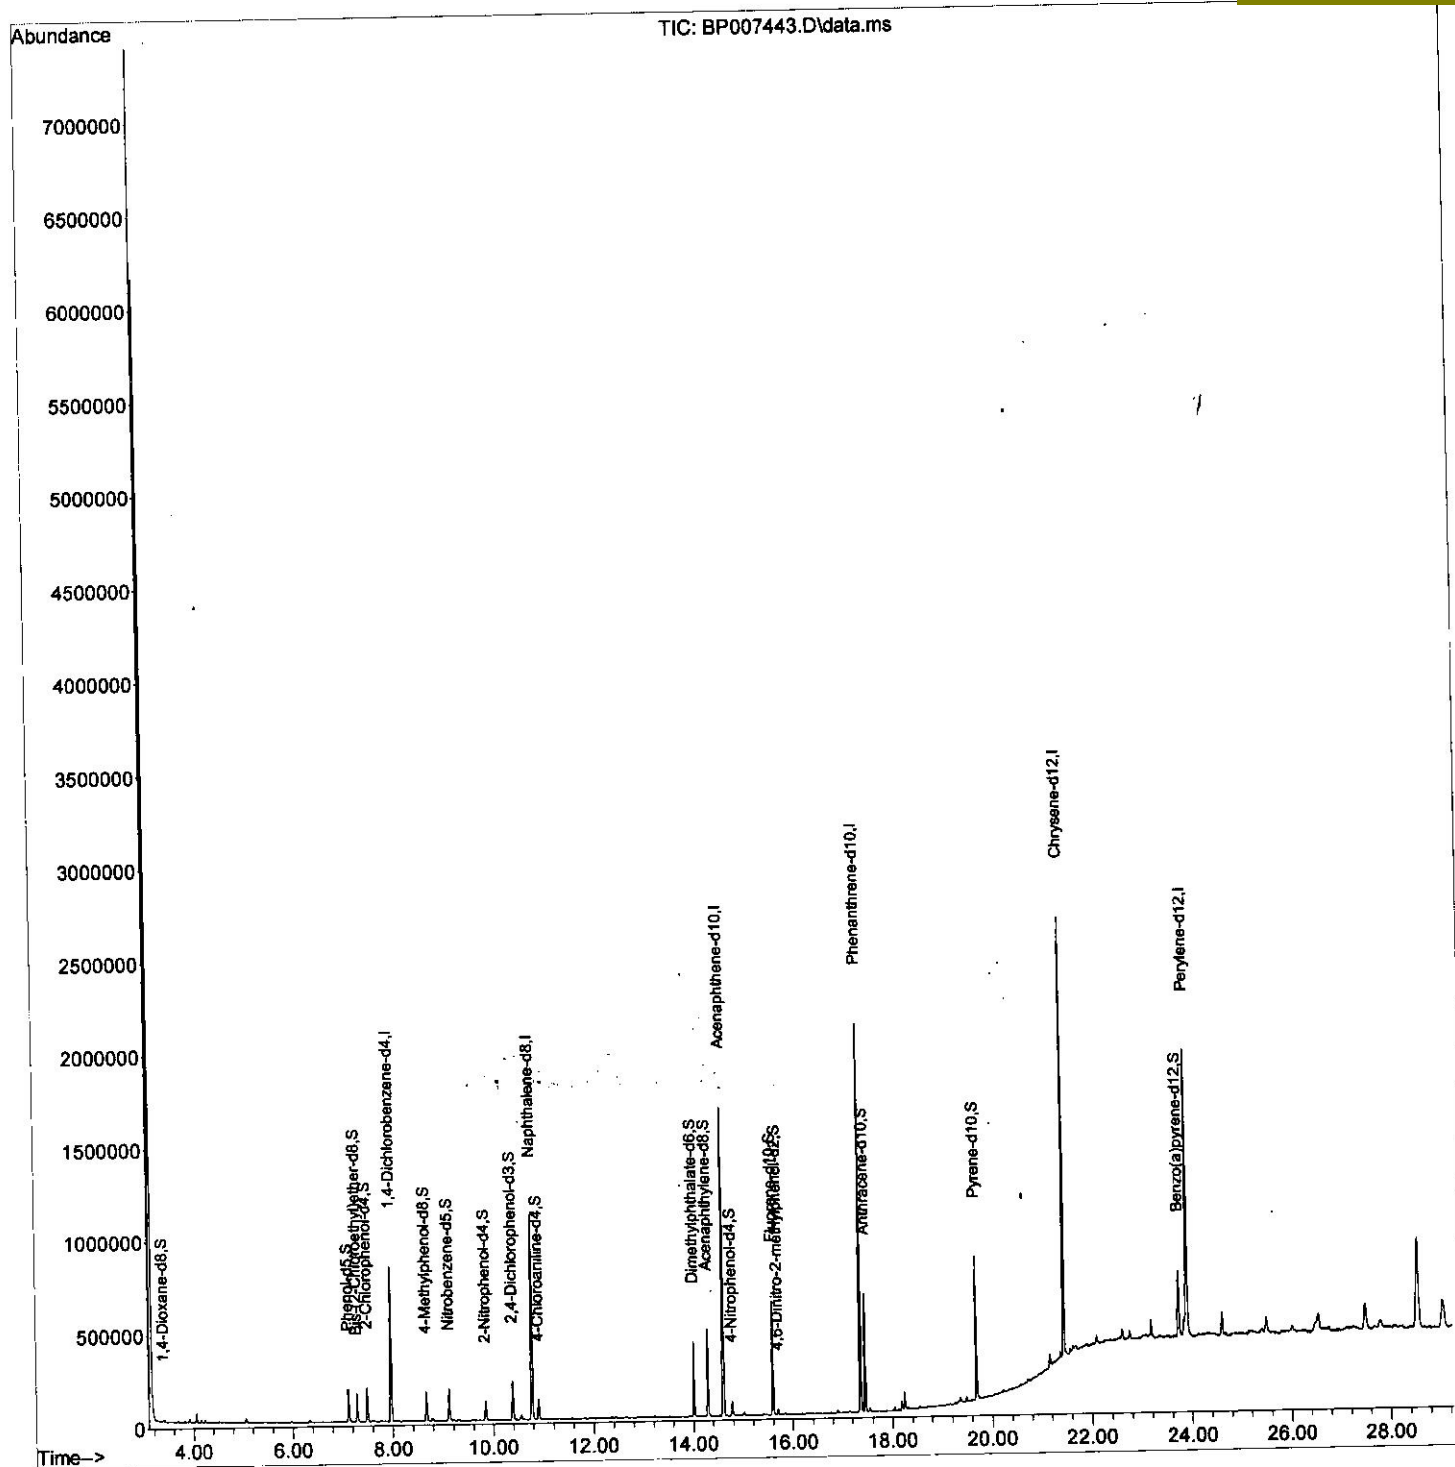

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
 Data File : BP007443.D
 Acq On : 15 Oct 2021 14:53
 Operator : CG/JU
 Sample : M4181-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B11

Manual Integrations
 APPROVED

mohammad
 10/18/2021 10:31:09 AM

Quant Time: Oct 15 15:45:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 14 13:04:52 2021
 Response via : Initial Calibration

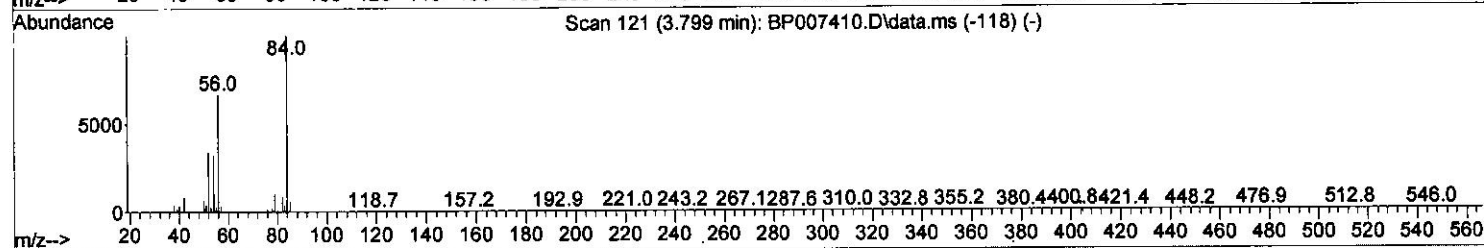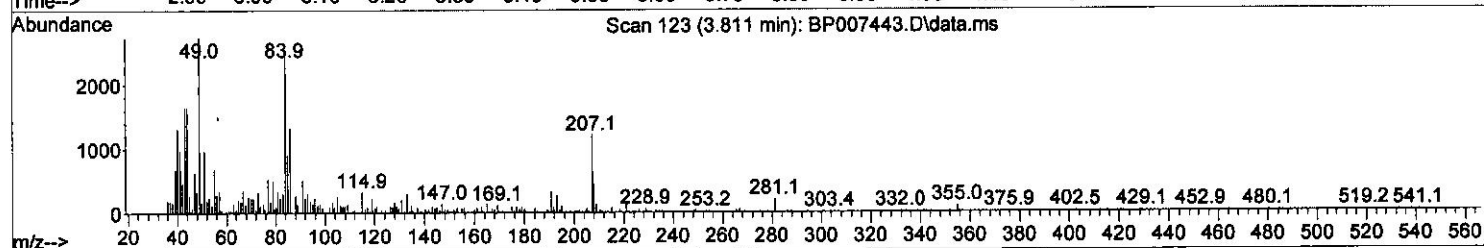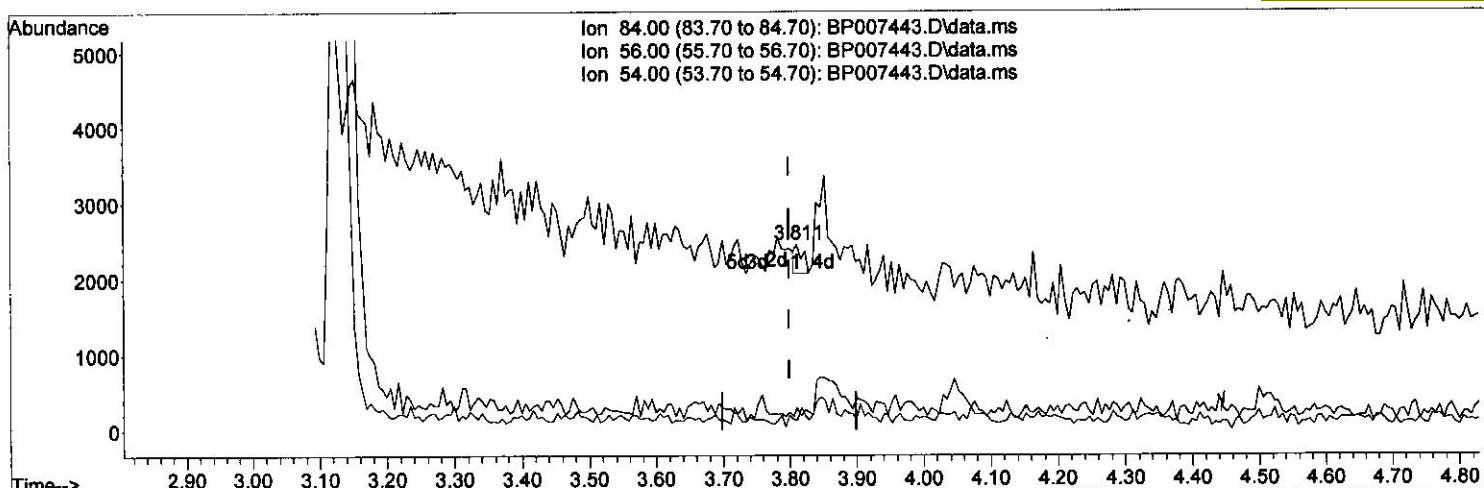

TIC: BP007443.D\data.ms

(4) Pyridine-d5 (S)

3.811min (+ 0.012) 0.02 ng/ul

response 301

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	66.30	11.71#
54.00	31.70	4.98#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
 Data File : BP007443.D
 Acq On : 15 Oct 2021 14:53
 Operator : CG/JU
 Sample : M4181-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B11

Manual Integrations
 APPROVED

mohammad
 10/18/2021 10:31:09 AM

Quant Time: Oct 15 15:45:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 14 13:04:52 2021
 Response via : Initial Calibration

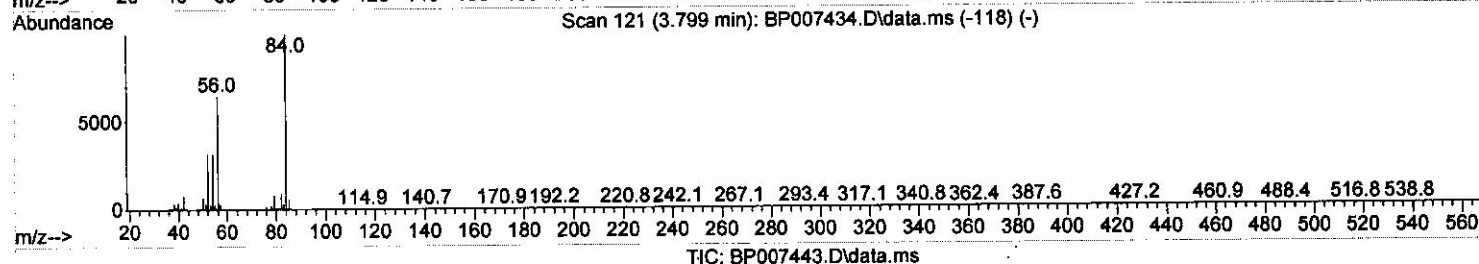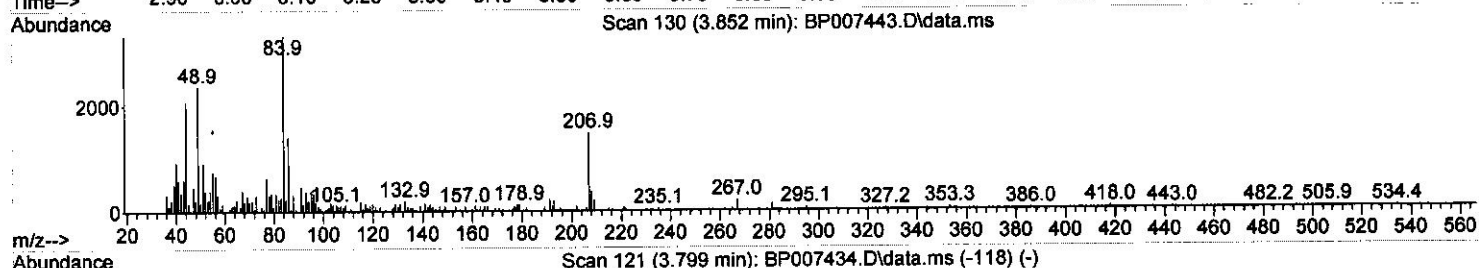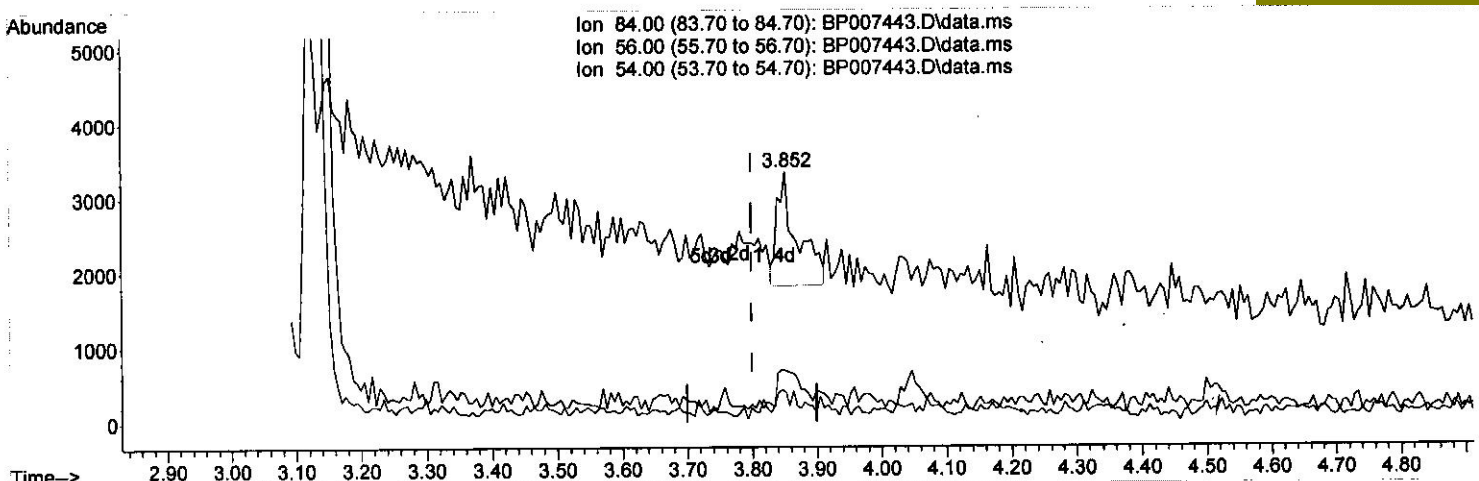

(4) Pyridine-d5 (S)

3.852min (+ 0.053) 0.22 ng/ul m

response 3349

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	66.30	20.32#
54.00	31.70	11.70#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
 Data File : BP007443.D
 Acq On : 15 Oct 2021 14:53
 Operator : CG/JU
 Sample : M4181-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B11

Manual Integrations
 APPROVED

mohammad
 10/18/2021 10:31:09 AM

Quant Time: Oct 15 15:45:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 14 13:04:52 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.964	152	224265	20.000	ng/ul	0.00
20) Naphthalene-d8	10.769	136	921892	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.598	164	577360	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.351	188	1180988	20.000	ng/ul	0.00
79) Chrysene-d12	21.439	240	1183480	20.000	ng/ul	0.00
88) Perylene-d12	23.898	264	1210665	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	6104	1.075	ng/ul	0.00
4) Pyridine-d5	3.852	84	3349m	0.215	ng/ul	0.05
7) Phenol-d5	7.117	99	105048	5.998	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	67864	6.497	ng/ul	0.00
11) 2-Chlorophenol-d4	7.493	132	86919	6.309	ng/ul	0.00
15) 4-Methylphenol-d8	8.664	113	57573	4.268	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	40313	6.910	ng/ul	0.00
24) 2-Nitrophenol-d4	9.840	143	35419	6.500	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.387	165	78324	5.893	ng/ul	0.00
31) 4-Chloroaniline-d4	10.899	131	59864	3.331	ng/ul	0.00
46) Dimethylphthalate-d6	14.004	166	259827	6.505	ng/ul	-0.01
49) Acenaphthylene-d8	14.287	160	333958	6.653	ng/ul	0.00
54) 4-Nitrophenol-d4	14.775	143	18414	2.873	ng/ul	0.00
60) Fluorene-d10	15.593	176	242285	7.248	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.698	200	7714	1.630	ng/ul	0.00
73) Anthracene-d10	17.451	188	363711	7.252	ng/ul	0.00
81) Pyrene-d10	19.681	212	387536	6.550	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.733	264	261442	4.340	ng/ul	0.00

JU
 10/27/21

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed