

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
 Data File : BP007417.D
 Acq On : 14 Oct 2021 15:12
 Operator : CG/JU
 Sample : M4030-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C00U0

Quant Time: Oct 14 15:55:09 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 14 13:04:52 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	145611	20.00	ng/ul	0.00
20) Naphthalene-d8	10.769	136	590834	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.598	164	392578	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.345	188	854720	20.00	ng/ul	-0.01
79) Chrysene-d12	21.427	240	891293	20.00	ng/ul	-0.02
88) Perylene-d12	23.880	264	912555	20.00	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	7723	2.09	ng/uL	0.00
4) Pyridine-d5	3.799	84	46591	4.62	ng/ul	0.00
7) Phenol-d5	7.116	99	112675	9.91	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	72821	10.74	ng/ul	0.00
11) 2-Chlorophenol-d4	7.493	132	89396	9.99	ng/ul	0.00
15) 4-Methylphenol-d8	8.663	113	53978	6.16	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	39825	10.65	ng/ul	0.00
24) 2-Nitrophenol-d4	9.840	143	36050	10.32	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.381	165	79538	9.34	ng/ul	0.00
31) 4-Chloroaniline-d4	10.898	131	114106	9.91	ng/ul	0.00
46) Dimethylphthalate-d6	14.004	166	312335	11.50	ng/ul	-0.01
49) Acenaphthylene-d8	14.287	160	367691	10.77	ng/ul	0.00
54) 4-Nitrophenol-d4	14.769	143	21733	4.99	ng/ul	-0.01
60) Fluorene-d10	15.586	176	272947	12.01	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.692	200	15192	4.44	ng/ul	-0.01
73) Anthracene-d10	17.445	188	420004	11.57	ng/ul	-0.01
81) Pyrene-d10	19.674	212	555799	12.47	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.721	264	513179	11.30	ng/ul	-0.02
Target Compounds						
					Qvalue	
80) Fluoranthene	19.351	202	76253	1.38	ng/ul	97
82) Pyrene	19.704	202	68873	1.24	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
Data File : BP007417.D
Acq On : 14 Oct 2021 15:12
Operator : CG/JU
Sample : M4030-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C00U0

Quant Time: Oct 14 15:55:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 14 13:04:52 2021
Response via : Initial Calibration




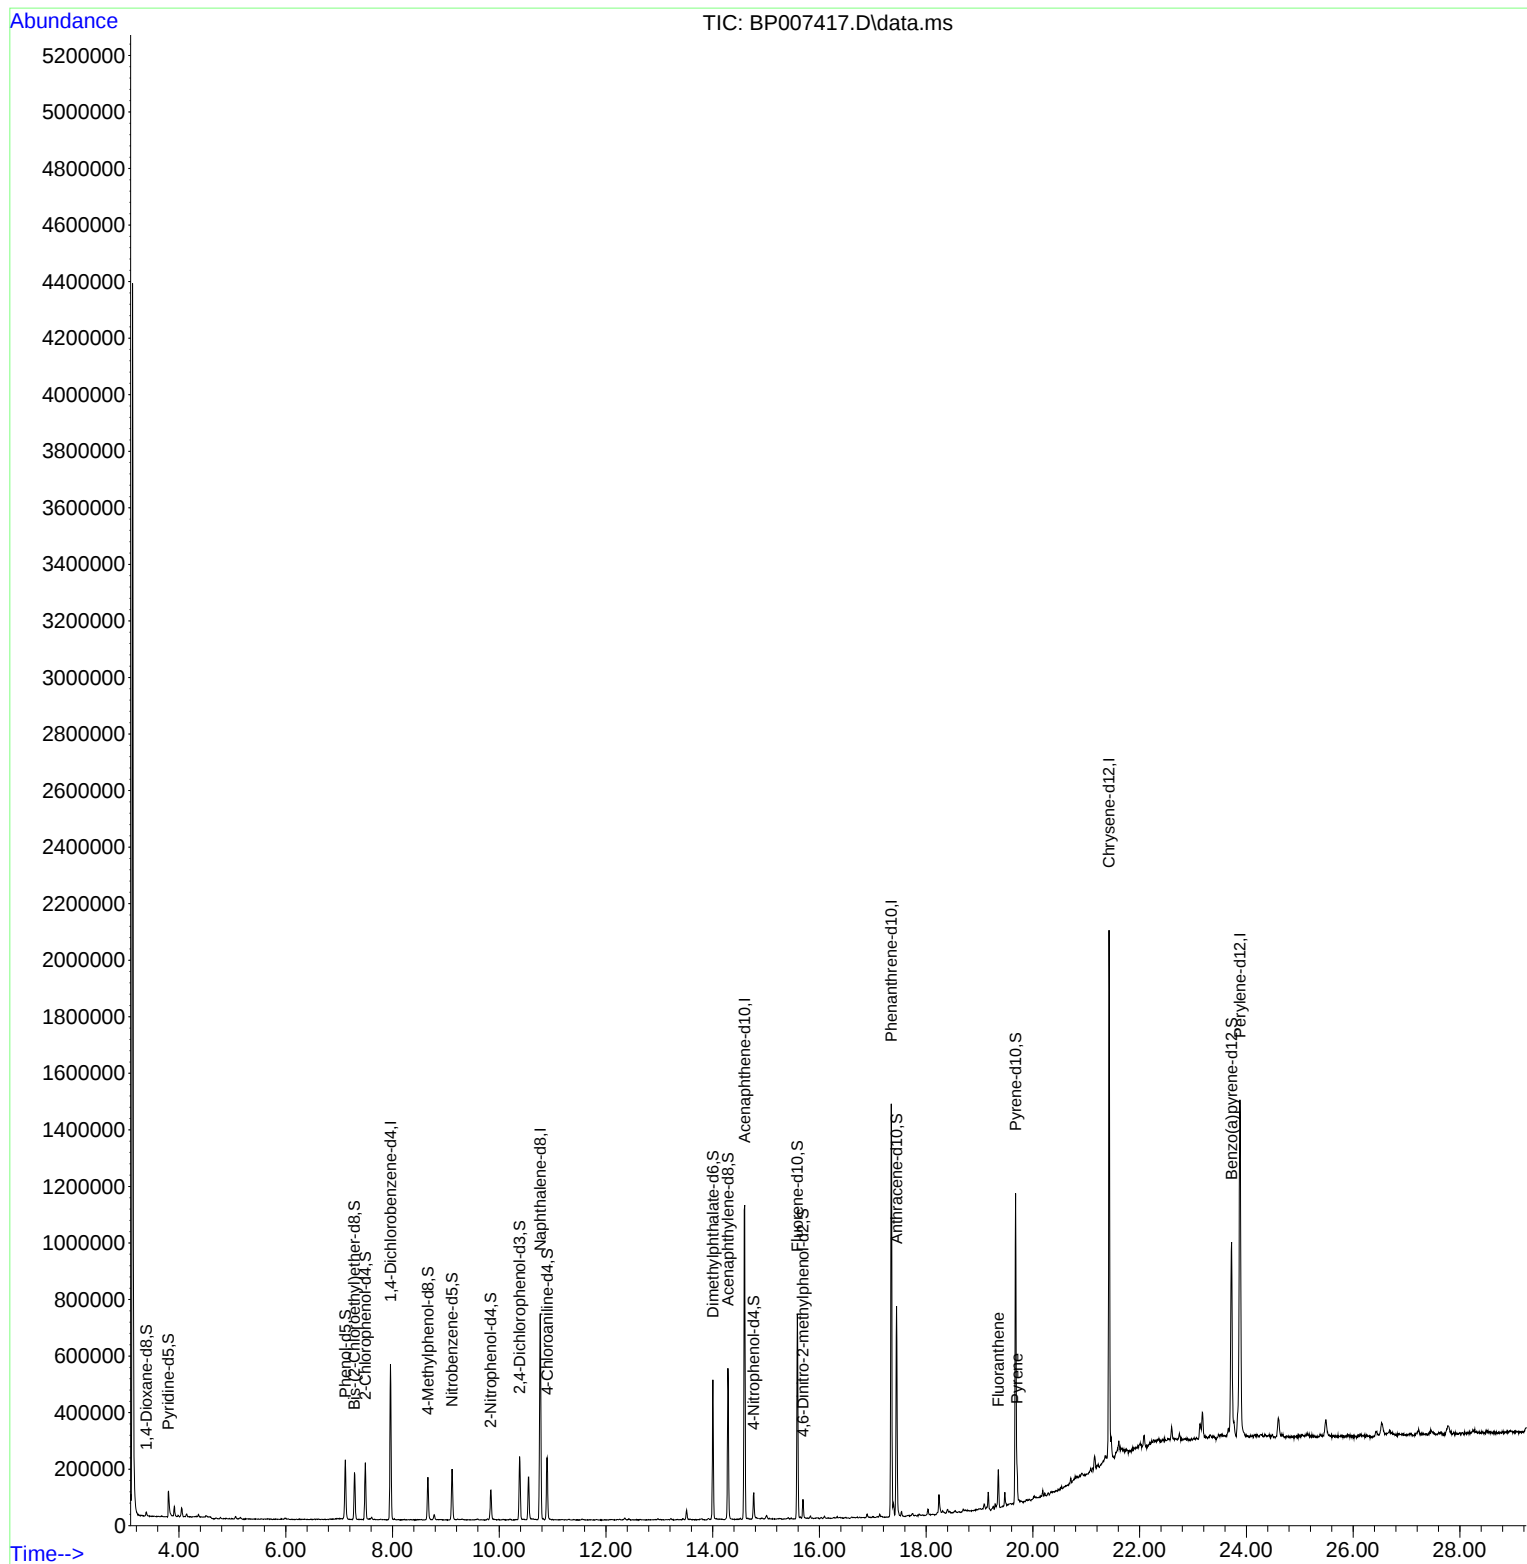


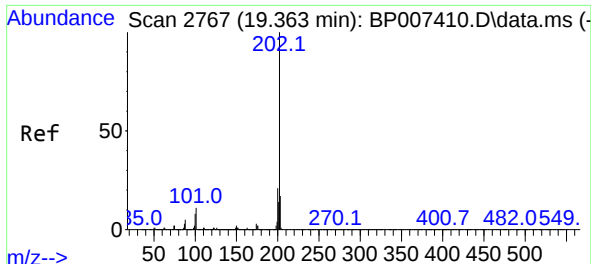

#80
Fluoranthene
Concen: 1.38 ng/ul
RT: 19.351 min Scan# 2765
Delta R.T. -0.012 min
Lab File: BP007417.D
Acq: 14 Oct 2021 15:12

Instrument :
BNA_P
ClientSampleId :
C00U0

Tgt Ion:202	Resp:	76253
Ion Ratio	Lower	Upper
202	100	
101	11.1	8.4 12.6
100	9.3	6.3 9.5

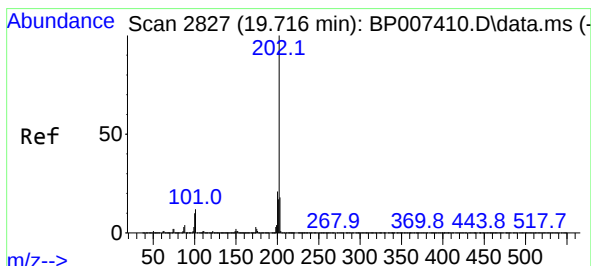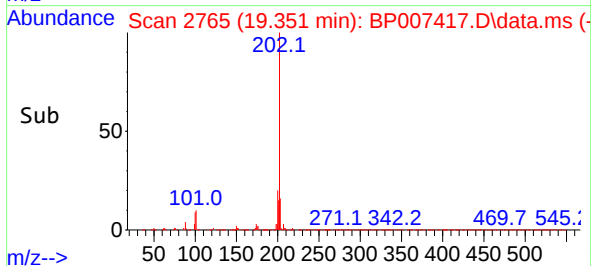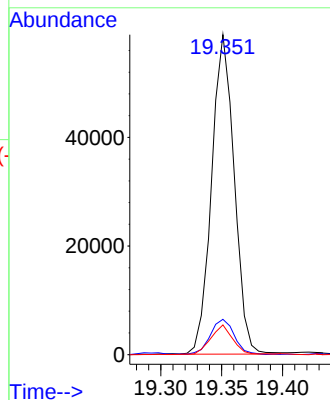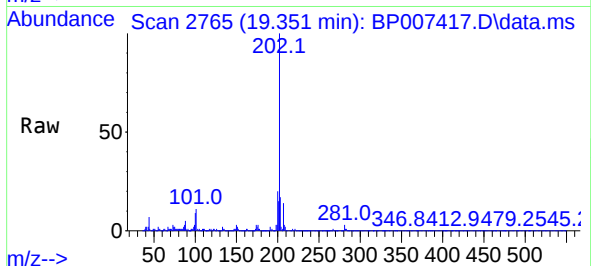

#82
Pyrene
Concen: 1.24 ng/ul
RT: 19.704 min Scan# 2825
Delta R.T. -0.012 min
Lab File: BP007417.D
Acq: 14 Oct 2021 15:12

Tgt Ion:202	Resp:	68873
Ion Ratio	Lower	Upper
202	100	
101	13.2	9.9 14.9
100	9.6	7.9 11.9

