

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
 Data File : BP007419.D
 Acq On : 14 Oct 2021 16:36
 Operator : CG/JU
 Sample : M4030-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C00T9

Quant Time: Oct 14 17:03:55 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 14 13:04:52 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	196945	20.00	ng/ul	0.00
20) Naphthalene-d8	10.769	136	769884	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.604	164	495481	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.357	188	1046934	20.00	ng/ul	0.00
79) Chrysene-d12	21.439	240	1113887	20.00	ng/ul	0.00
88) Perylene-d12	23.898	264	1156885	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	9012	1.81	ng/uL	0.00
4) Pyridine-d5	3.799	84	50502	3.70	ng/ul	0.00
7) Phenol-d5	7.116	99	131632	8.56	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	84213	9.18	ng/ul	0.00
11) 2-Chlorophenol-d4	7.493	132	104894	8.67	ng/ul	0.00
15) 4-Methylphenol-d8	8.663	113	71503	6.04	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	43426	8.91	ng/ul	0.00
24) 2-Nitrophenol-d4	9.846	143	36607	8.04	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	87295	7.86	ng/ul	0.00
31) 4-Chloroaniline-d4	10.899	131	113871	7.59	ng/ul	0.00
46) Dimethylphthalate-d6	14.010	166	321394	9.38	ng/ul	0.00
49) Acenaphthylene-d8	14.293	160	391108	9.08	ng/ul	0.00
54) 4-Nitrophenol-d4	14.775	143	28123	5.11	ng/ul	0.00
60) Fluorene-d10	15.598	176	285944	9.97	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	18360	4.38	ng/ul	0.00
73) Anthracene-d10	17.457	188	425021	9.56	ng/ul	0.00
81) Pyrene-d10	19.686	212	566424	10.17	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.739	264	545793	9.48	ng/ul	0.00
Target Compounds						
80) Fluoranthene	19.363	202	72841	1.05	ng/ul	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
Data File : BP007419.D
Acq On : 14 Oct 2021 16:36
Operator : CG/JU
Sample : M4030-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C00T9

Quant Time: Oct 14 17:03:55 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 14 13:04:52 2021
Response via : Initial Calibration

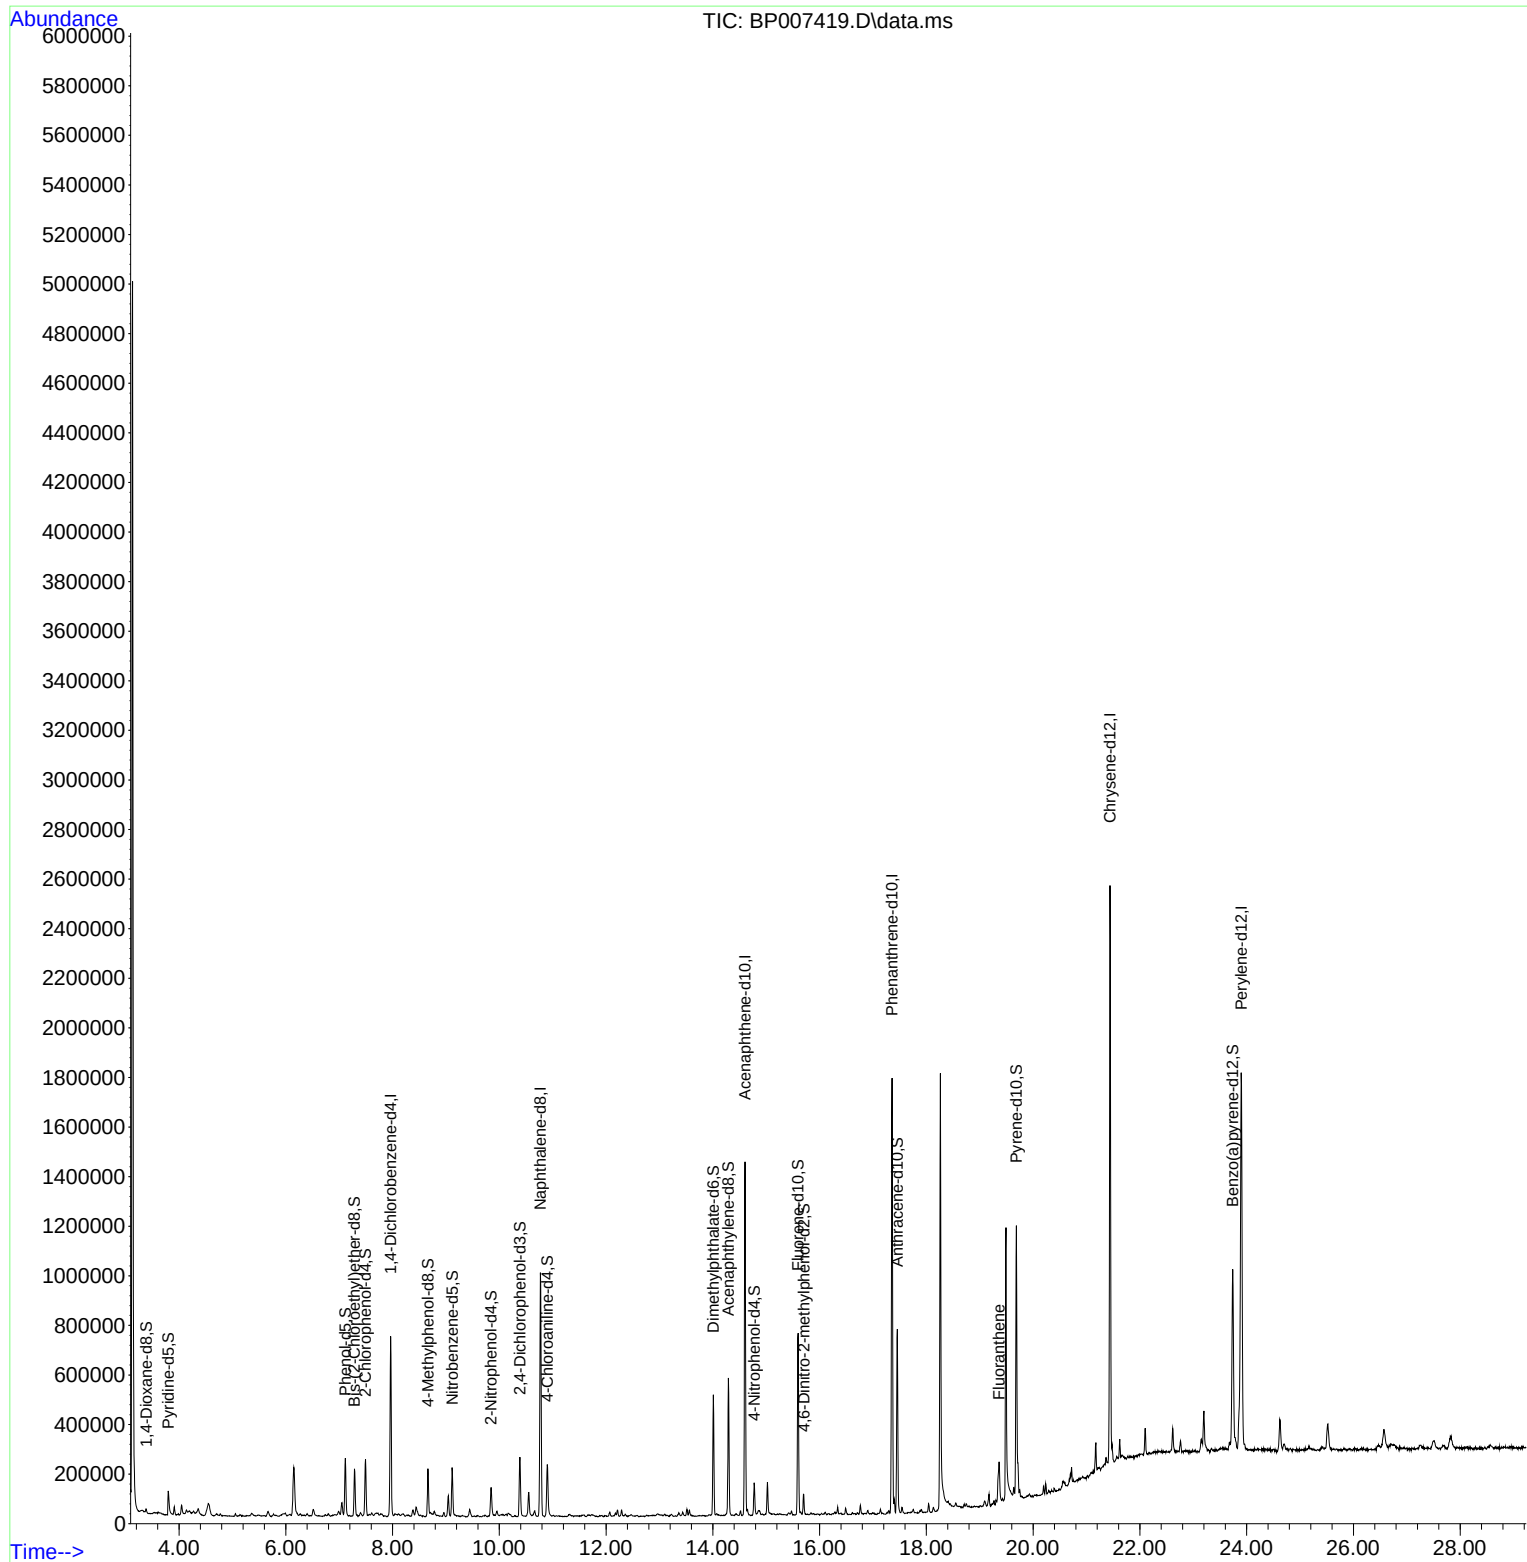

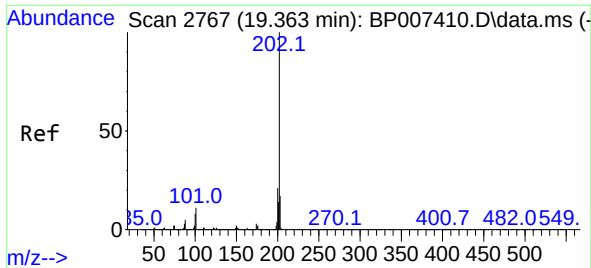

#80
 Fluoranthene
 Concen: 1.05 ng/ul
 RT: 19.363 min Scan# 2767
 Delta R.T. -0.000 min
 Lab File: BP007419.D
 Acq: 14 Oct 2021 16:36

Instrument :
 BNA_P
 ClientSampleId :
 C00T9

Tgt Ion:202 Resp: 72841
 Ion Ratio Lower Upper
 202 100
 101 10.4 8.4 12.6
 100 7.8 6.3 9.5

