

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
 Data File : BP007428.D
 Acq On : 14 Oct 2021 23:59
 Operator : CG/JU
 Sample : M4126-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA7

Quant Time: Oct 15 01:15:51 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 14 13:04:52 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.964	152	274632	20.00	ng/ul	0.00
20) Naphthalene-d8	10.769	136	1116646	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.593	164	690853	20.00	ng/ul	-0.01
64) Phenanthrene-d10	17.345	188	1432472	20.00	ng/ul	-0.01
79) Chrysene-d12	21.428	240	1451812	20.00	ng/ul	-0.02
88) Perylene-d12	23.880	264	1500655	20.00	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	9391	1.35	ng/uL	0.00
4) Pyridine-d5	3.811	84	20997	1.10	ng/ul	0.01
7) Phenol-d5	7.117	99	142370	6.64	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	92120	7.20	ng/ul	0.00
11) 2-Chlorophenol-d4	7.487	132	118200	7.01	ng/ul	0.00
15) 4-Methylphenol-d8	8.664	113	59402	3.60	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	53235	7.53	ng/ul	0.00
24) 2-Nitrophenol-d4	9.840	143	48035	7.28	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.381	165	108064	6.71	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	129740	5.96	ng/ul	0.00
46) Dimethylphthalate-d6	14.004	166	364397	7.62	ng/ul	-0.01
49) Acenaphthylene-d8	14.287	160	449949	7.49	ng/ul	0.00
54) 4-Nitrophenol-d4	14.769	143	33098	4.32	ng/ul	-0.01
60) Fluorene-d10	15.587	176	326003	8.15	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.693	200	12552	2.19	ng/ul	-0.01
73) Anthracene-d10	17.445	188	493910	8.12	ng/ul	-0.01
81) Pyrene-d10	19.675	212	471069	6.49	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.722	264	280917	3.76	ng/ul	-0.02
Target Compounds						
80) Fluoranthene	19.351	202	98163	1.09	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
Data File : BP007428.D
Acq On : 14 Oct 2021 23:59
Operator : CG/JU
Sample : M4126-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA7

Quant Time: Oct 15 01:15:51 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 14 13:04:52 2021
Response via : Initial Calibration

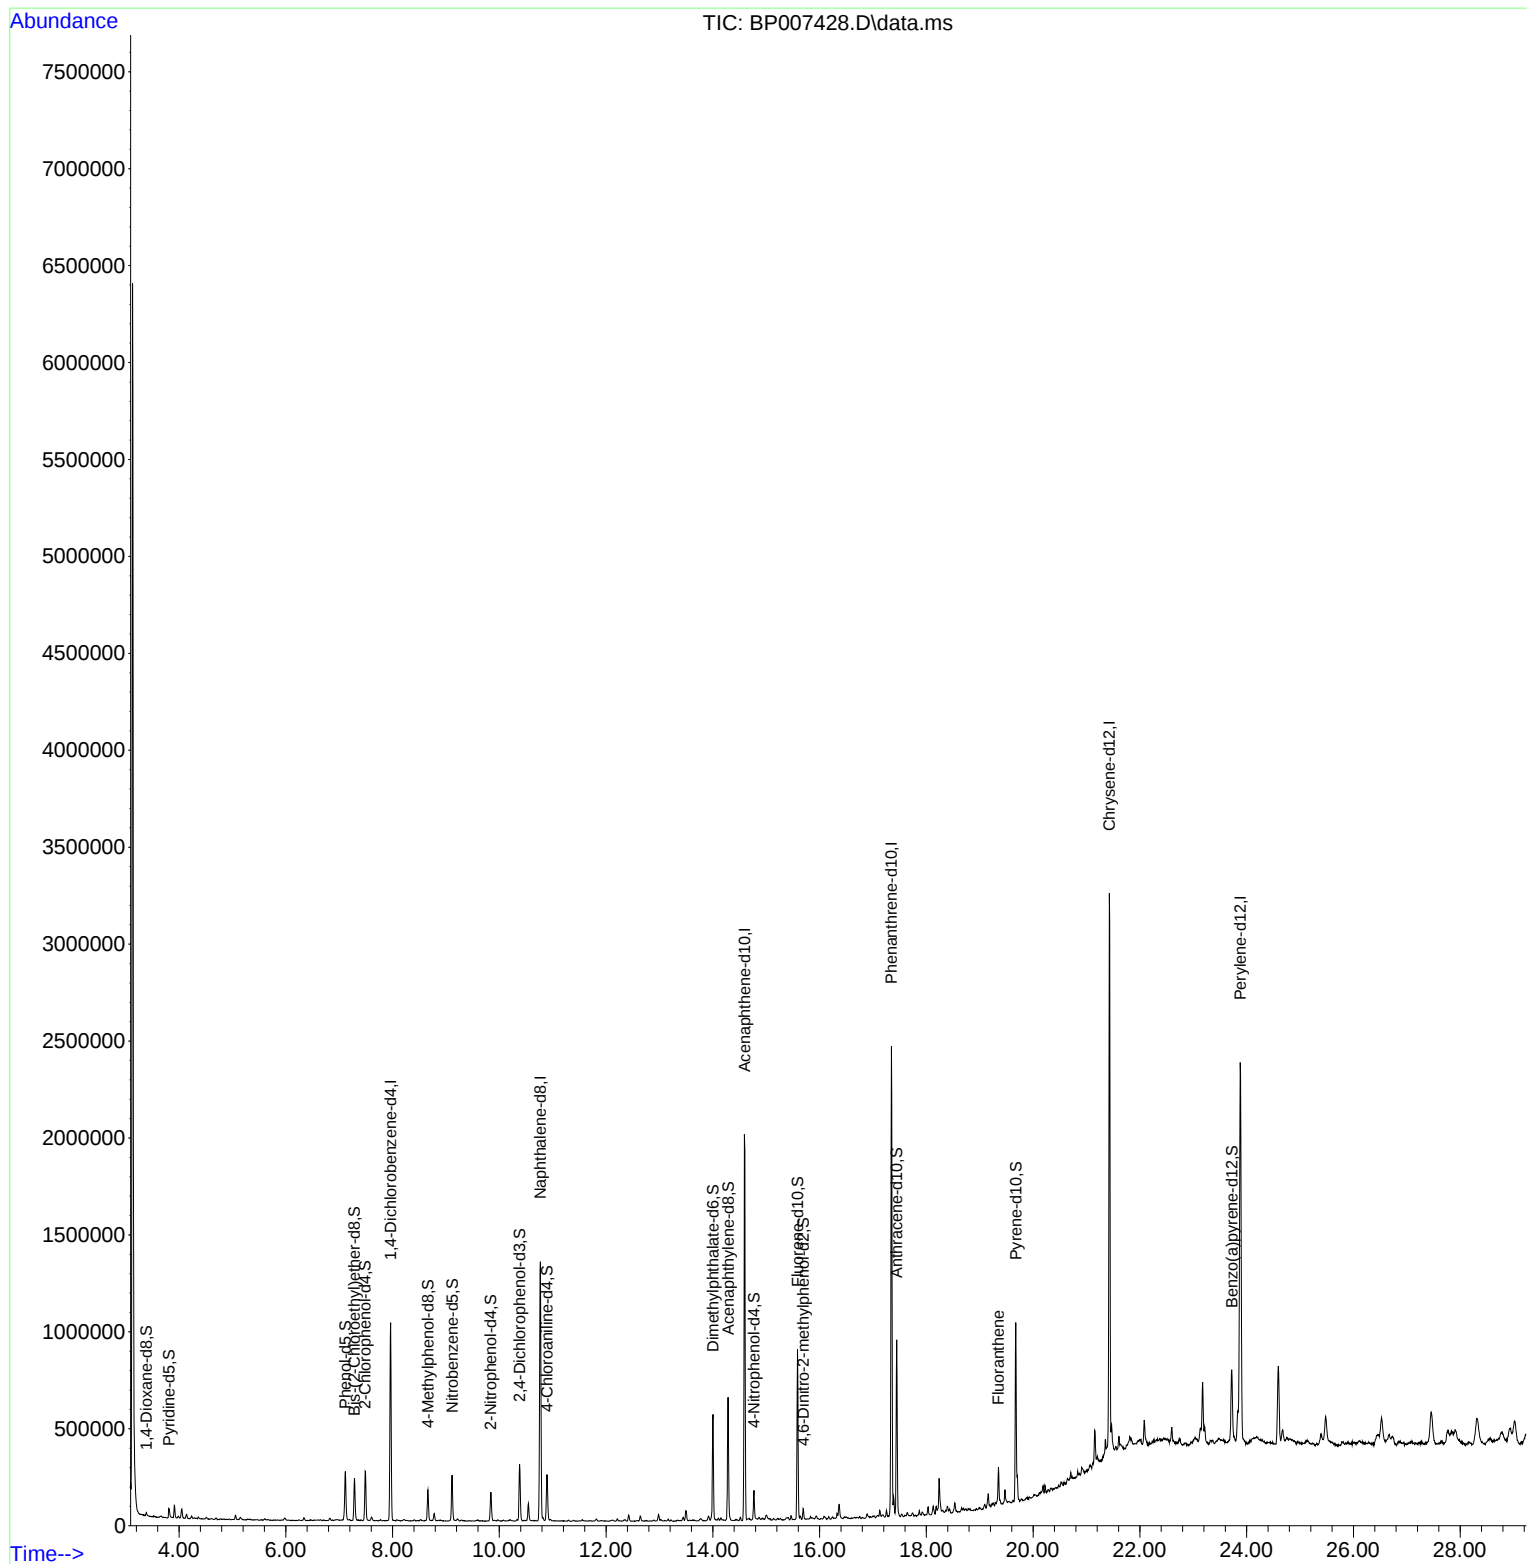

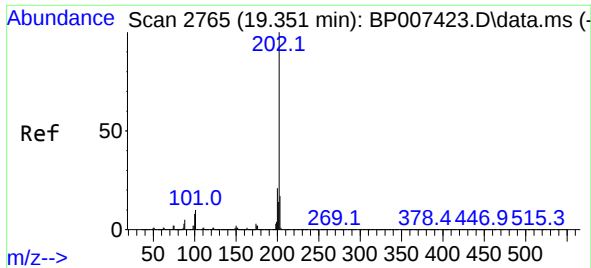

#80
 Fluoranthene
 Concen: 1.09 ng/ul
 RT: 19.351 min Scan# 2765
 Delta R.T. -0.012 min
 Lab File: BP007428.D
 Acq: 14 Oct 2021 23:59

Instrument :
 BNA_P
 ClientSampleId :
 C0AA7

Tgt Ion:202 Resp: 98163
 Ion Ratio Lower Upper
 202 100
 101 11.3 8.4 12.6
 100 8.0 6.3 9.5

