

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
 Data File : BP007444.D
 Acq On : 15 Oct 2021 15:27
 Operator : CG/JU
 Sample : M4181-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B43

Quant Time: Oct 15 16:53:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 14 13:04:52 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	215654	20.00	ng/ul	0.00
20) Naphthalene-d8	10.769	136	885534	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.598	164	557711	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.351	188	1135895	20.00	ng/ul	0.00
79) Chrysene-d12	21.439	240	1125247	20.00	ng/ul	0.00
88) Perylene-d12	23.898	264	1143679	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	19747	3.62	ng/uL	0.00
4) Pyridine-d5	3.817	84	10854	0.73	ng/ul	0.02
7) Phenol-d5	7.122	99	323405	19.20	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	192695	19.18	ng/ul	0.00
11) 2-Chlorophenol-d4	7.493	132	260457	19.66	ng/ul	0.00
15) 4-Methylphenol-d8	8.663	113	241398	18.61	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	114870	20.50	ng/ul	0.00
24) 2-Nitrophenol-d4	9.846	143	111344	21.27	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	242551	19.00	ng/ul	0.00
31) 4-Chloroaniline-d4	10.899	131	319185	18.49	ng/ul	0.00
46) Dimethylphthalate-d6	14.004	166	718912	18.63	ng/ul	-0.01
49) Acenaphthylene-d8	14.293	160	881245	18.17	ng/ul	0.00
54) 4-Nitrophenol-d4	14.775	143	97723	15.78	ng/ul	0.00
60) Fluorene-d10	15.592	176	623524	19.31	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.698	200	40605	8.92	ng/ul	0.00
73) Anthracene-d10	17.451	188	951278	19.72	ng/ul	0.00
81) Pyrene-d10	19.680	212	1036734	18.43	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.733	264	1040599	18.29	ng/ul	0.00
Target Compounds						Qvalue
80) Fluoranthene	19.357	202	92796	1.33	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
Data File : BP007444.D
Acq On : 15 Oct 2021 15:27
Operator : CG/JU
Sample : M4181-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B43

Quant Time: Oct 15 16:53:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 14 13:04:52 2021
Response via : Initial Calibration

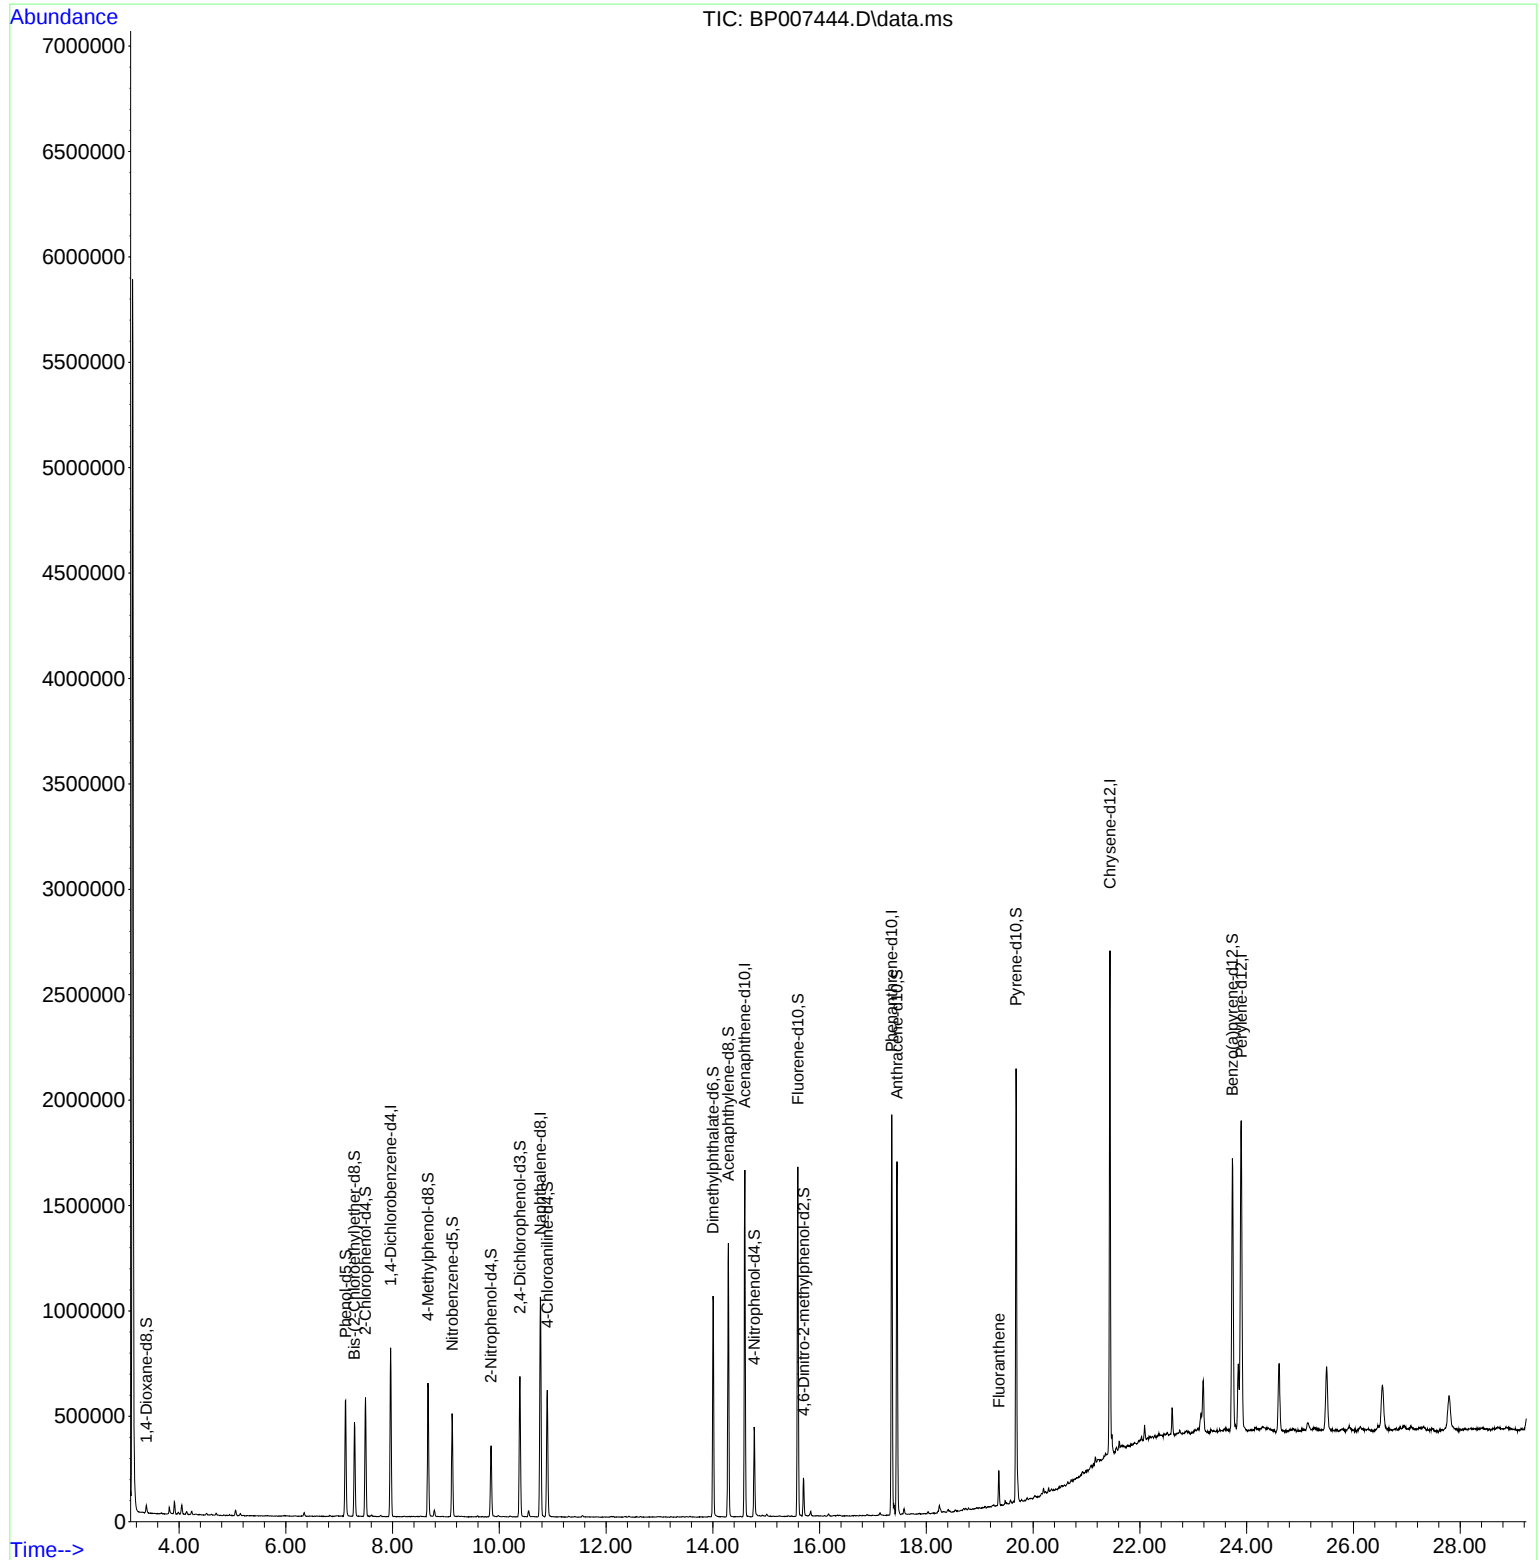

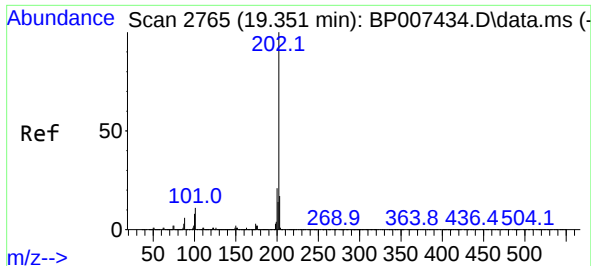

#80
 Fluoranthene
 Concen: 1.33 ng/ul
 RT: 19.357 min Scan# 2766
 Delta R.T. -0.006 min
 Lab File: BP007444.D
 Acq: 15 Oct 2021 15:27

Instrument :
 BNA_P
 ClientSampleId :
 C0B43

Tgt Ion:	202	Resp:	92796
Ion	Ratio	Lower	Upper
202	100		
101	10.9	8.4	12.6
100	8.5	6.3	9.5

