

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
 Data File : BP007424.D
 Acq On : 14 Oct 2021 20:01
 Operator : CG/JU
 Sample : PB139790BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK790

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007424.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.129	3	7	16	rVB	214206	309420	6.76%	0.605%
2	3.381	46	50	56	rVB	54557	70551	1.54%	0.138%
3	3.793	116	120	142	rBV	698978	1070946	23.40%	2.095%
4	4.140	174	179	184	rBV	15523	22290	0.49%	0.044%
5	4.575	251	253	259	rVB7	4587	8109	0.18%	0.016%
6	7.111	676	684	692	rBV	767811	1225347	26.77%	2.397%
7	7.287	707	714	726	rVB	620696	982709	21.47%	1.923%
8	7.487	738	748	763	rBV	785196	1238769	27.07%	2.424%
9	7.958	820	828	840	rVB	812761	1324081	28.93%	2.591%
10	8.658	940	947	959	rBV	945940	1513312	33.06%	2.961%
11	9.116	1016	1025	1035	rBV	674243	1147272	25.07%	2.245%
12	9.840	1136	1148	1160	rBV	474143	795094	17.37%	1.556%
13	10.381	1231	1240	1253	rBV	906789	1500746	32.79%	2.936%
14	10.763	1298	1305	1316	rVB	1068442	1845149	40.31%	3.610%
15	10.893	1318	1327	1339	rBV	938422	1605211	35.07%	3.141%
16	12.352	1569	1575	1581	rVB	19164	30449	0.67%	0.060%
17	13.569	1778	1782	1786	rVB5	3875	6184	0.14%	0.012%
18	14.004	1849	1856	1870	rBV	1640362	2350828	51.36%	4.600%
19	14.287	1895	1904	1915	rBV	1833681	2815840	61.52%	5.509%
20	14.593	1947	1956	1963	rBV	1671236	2539734	55.49%	4.969%
21	14.769	1979	1986	2000	rBV	726636	1064677	23.26%	2.083%
22	15.587	2118	2125	2133	rBV	2382838	3453377	75.45%	6.757%
23	15.693	2136	2143	2154	rBV	501098	690226	15.08%	1.350%
24	15.828	2161	2166	2173	rVB	30929	47007	1.03%	0.092%
25	16.151	2216	2221	2225	rBV8	3838	7094	0.15%	0.014%
26	16.369	2254	2258	2262	rBV6	4962	8113	0.18%	0.016%
27	17.128	2383	2387	2391	rVB	9475	12463	0.27%	0.024%
28	17.345	2417	2424	2434	rBV	2135604	3064356	66.95%	5.996%
29	17.445	2434	2441	2454	rBV	2576311	3757433	82.10%	7.352%
30	17.710	2484	2486	2491	rBV6	4366	5912	0.13%	0.012%
31	18.239	2572	2576	2580	rBV5	12801	20857	0.46%	0.041%
32	19.251	2744	2748	2753	rVB3	31420	40212	0.88%	0.079%
33	19.322	2756	2760	2764	rBV	37555	50400	1.10%	0.099%
34	19.475	2783	2786	2791	rBV6	10302	13096	0.29%	0.026%
35	19.675	2814	2820	2829	rBV	3388401	4500535	98.33%	8.806%
36	21.428	3113	3118	3125	rBV	2636746	3499115	76.45%	6.846%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
Data File : BP007424.D
Acq On : 14 Oct 2021 20:01
Operator : CG/JU
Sample : PB139790BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK790

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Title : SVOA CALIBRATION

37	23.716	3500	3507	3520	rVB2	2214917	4576863	100.00%	8.955%
38	23.874	3523	3534	3545	rVB2	1728026	3896342	85.13%	7.623%




Sum of corrected areas: 51110119

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
Data File : BP007424.D
Acq On : 14 Oct 2021 20:01
Operator : CG/JU
Sample : PB139790BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK790

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

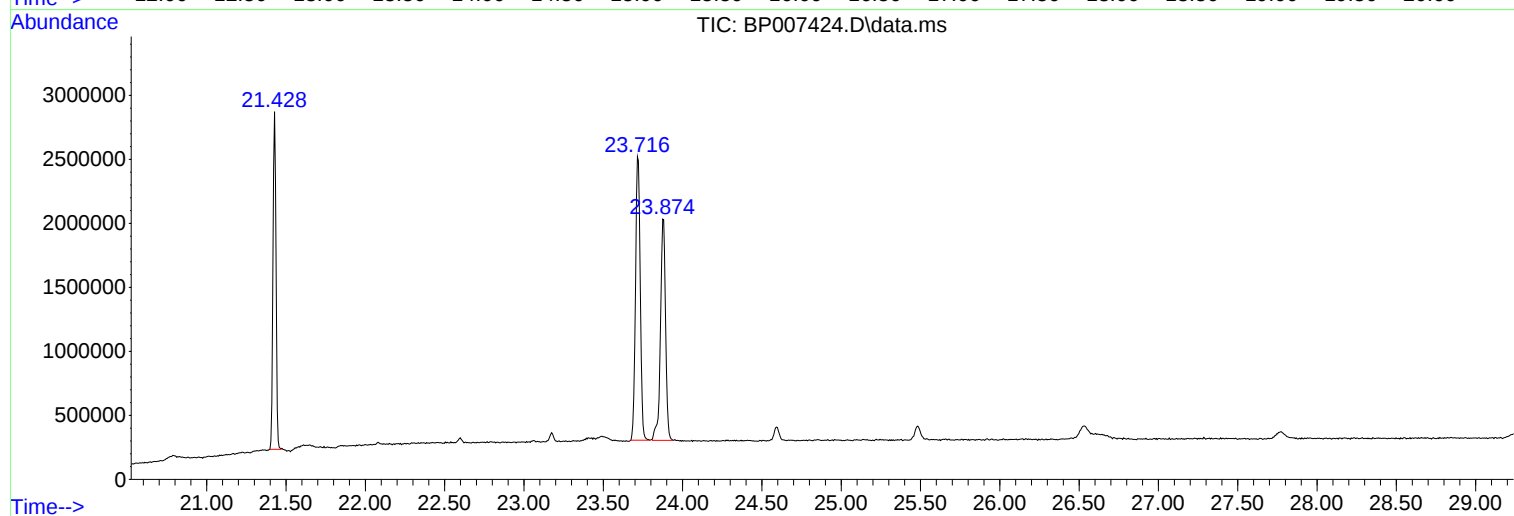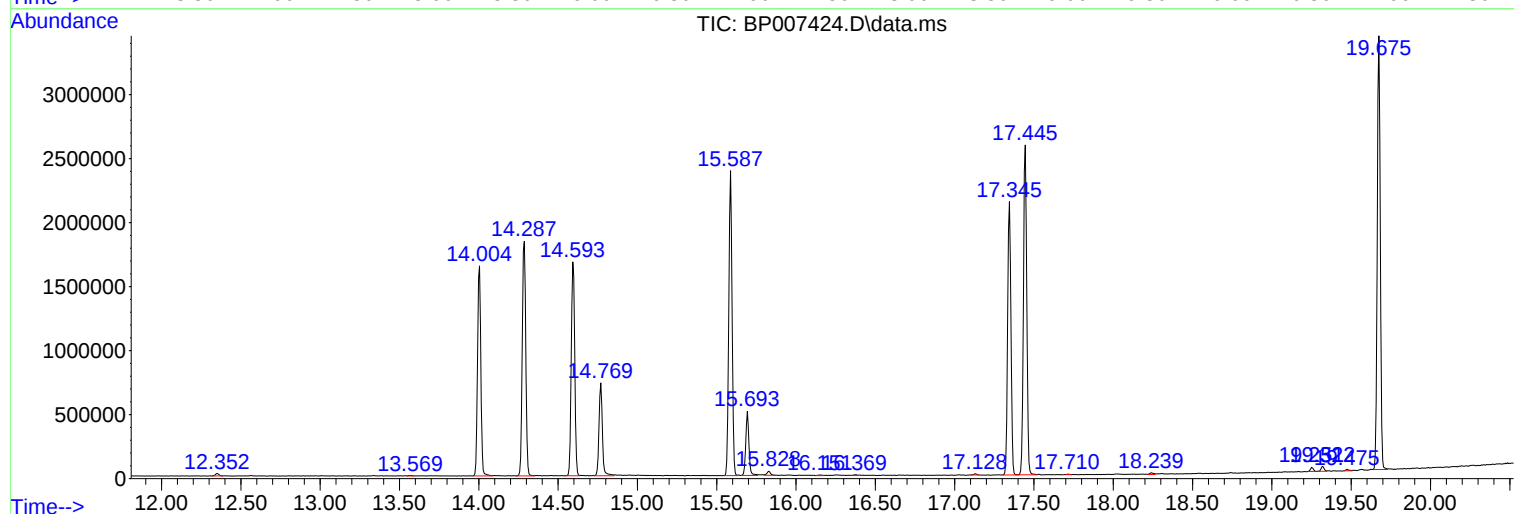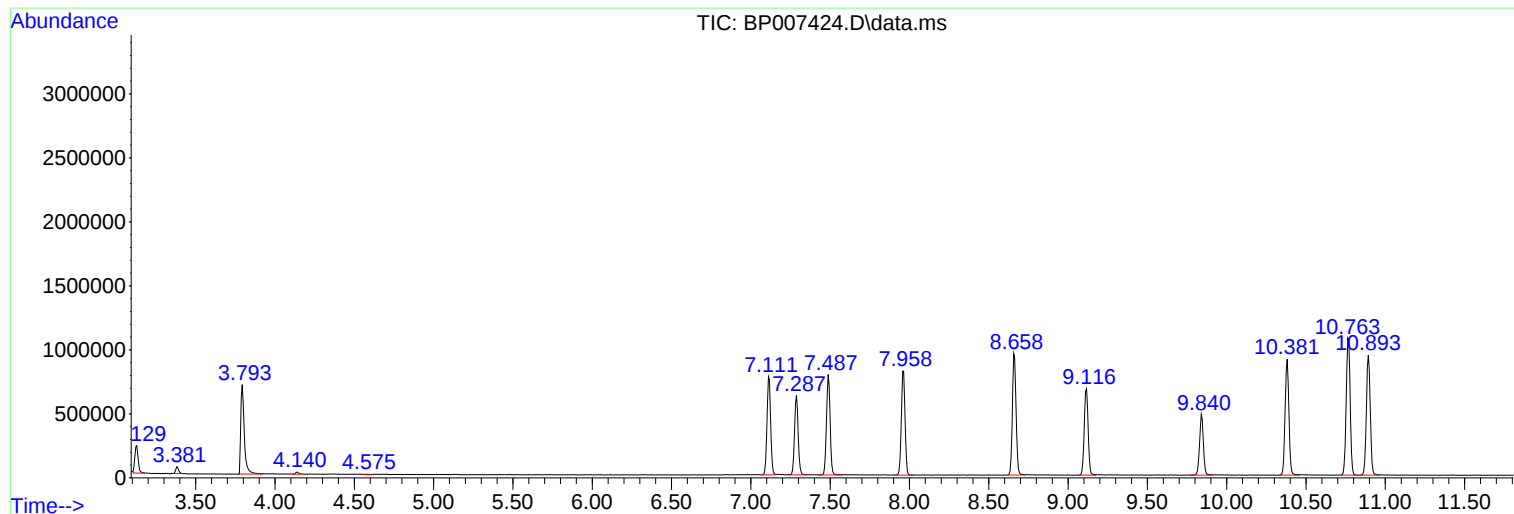

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
Data File : BP007424.D
Acq On : 14 Oct 2021 20:01
Operator : CG/JU
Sample : PB139790BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK790










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.129	4.67 ng/ul	309420	1,4-Dichlorobenzene-d4	7.964

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
4			Silane, ethyltrimethyl-	102	C5H14Si	003439-38-1	36
5			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	22

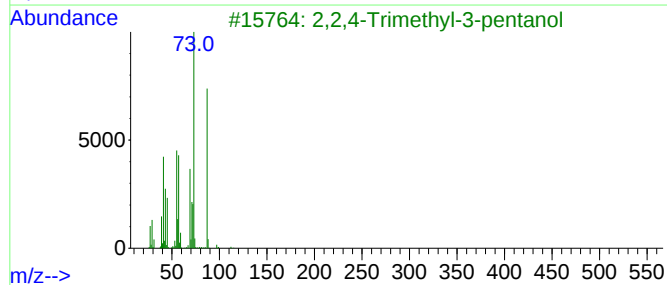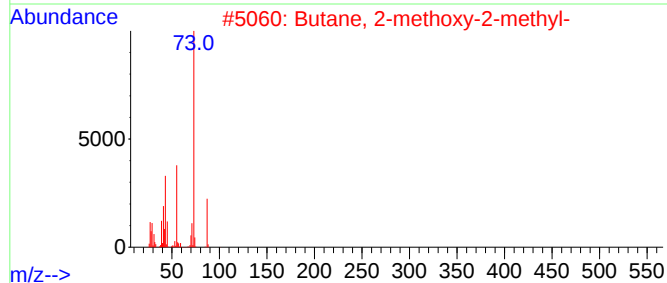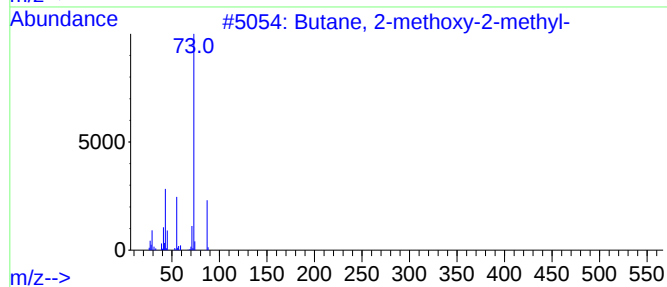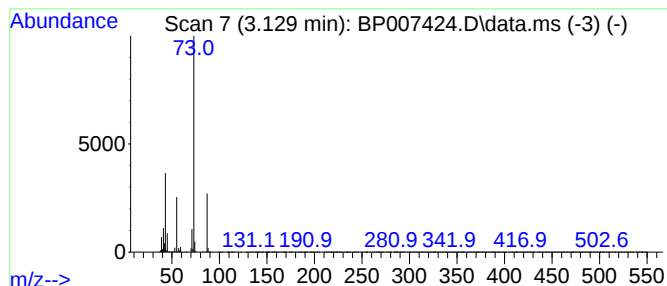

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101421\
Data File : BP007424.D
Acq On : 14 Oct 2021 20:01
Operator : CG/JU
Sample : PB139790BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK790

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.129	4.7	ng/ul	309420	1	7.964	1324080	20.0