

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012138.D
 Acq On : 14 Oct 2022 15:16
 Operator : CG/JU
 Sample : N4982-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Oct 14 23:03:41 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 12 23:03:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.845	152	279319	20.000	ng/ul	0.00
20) Naphthalene-d8	10.651	136	1175107	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.498	164	665300	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.257	188	1390603	20.000	ng/ul	0.00
79) Chrysene-d12	21.345	240	1454702	20.000	ng/ul	0.00
88) Perylene-d12	23.768	264	1544102	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	22800	3.218	ng/uL	0.00
4) Pyridine-d5	3.710	84	43677	2.318	ng/ul	0.01
7) Phenol-d5	7.016	99	140097	6.236	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	357584	28.043	ng/ul	0.00
11) 2-Chlorophenol-d4	7.375	132	403165	22.609	ng/ul	0.00
15) 4-Methylphenol-d8	8.563	113	214784	12.448	ng/ul	0.00
21) Nitrobenzene-d5	9.016	128	248082	29.892	ng/ul	0.00
24) 2-Nitrophenol-d4	9.734	143	251239	29.855	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.275	165	392340	24.057	ng/ul	0.00
31) 4-Chloroaniline-d4	10.798	131	87651	3.647	ng/ul	0.00
46) Dimethylphthalate-d6	13.910	166	1188218	28.201	ng/ul	0.00
49) Acenaphthylene-d8	14.186	160	1434327	27.529	ng/ul	0.00
54) 4-Nitrophenol-d4	14.716	143	35064	4.239	ng/ul	0.00
60) Fluorene-d10	15.492	176	1102999	28.934	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.616	200	148601	20.238	ng/ul	0.00
73) Anthracene-d10	17.357	188	1715366	28.407	ng/ul	0.00
81) Pyrene-d10	19.592	212	2162498	29.017	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.609	264	2295211	30.577	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.045	94	23673	1.004	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012138.D
Acq On : 14 Oct 2022 15:16
Operator : CG/JU
Sample : N4982-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Oct 14 23:03:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 12 23:03:21 2022
Response via : Initial Calibration

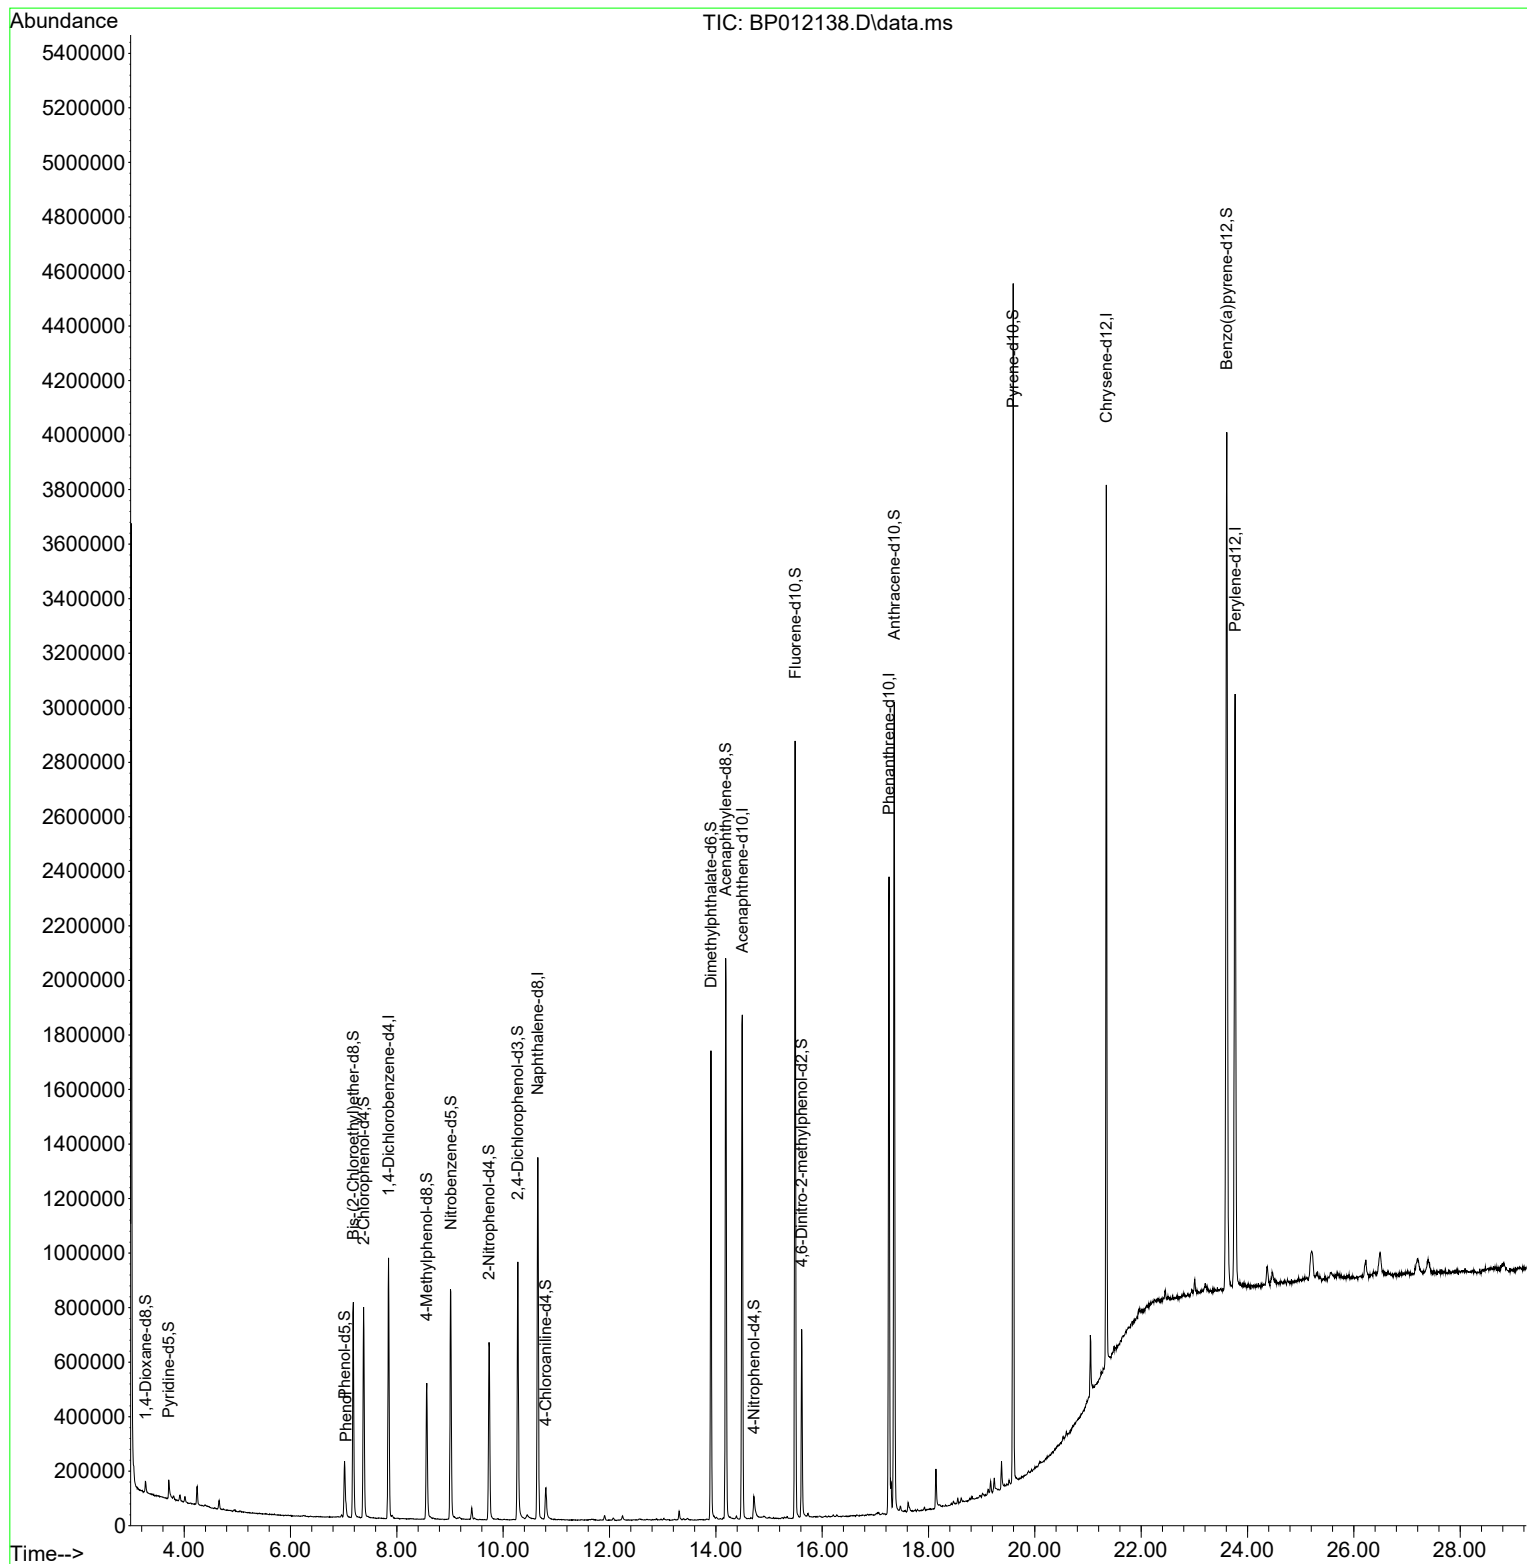

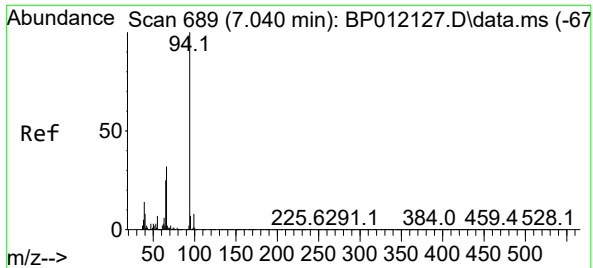

#8
Phenol
Concen: 1.004 ng/ul
RT: 7.045 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP012138.D
Acq: 14 Oct 2022 15:16

Instrument :
BNA_P
ClientSampleId :

Tgt Ion: 94 Resp: 23673
Ion Ratio Lower Upper
94 100
65 24.2 19.4 29.0
66 30.8 24.6 37.0

